

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052629.D
 Acq On : 06 Jan 2023 15:41
 Operator : JC/MD
 Sample : 01036-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052629.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	51	56	64	rBV	8780	8985	0.56%	0.078%
2	1.601	73	81	97	rVB	222576	260502	16.16%	2.262%
3	1.909	169	177	200	rVB	177335	249617	15.49%	2.168%
4	2.565	369	381	397	rBV	331743	542659	33.66%	4.713%
5	2.713	423	427	429	rBV2	675	554	0.03%	0.005%
6	2.861	471	473	478	rVB2	324	255	0.02%	0.002%
7	2.932	493	495	499	rBV2	406	216	0.01%	0.002%
8	3.047	523	531	540	rVB3	2764	4237	0.26%	0.037%
9	3.096	543	546	548	rBV	255	194	0.01%	0.002%
10	3.183	558	573	589	rBV	25439	60673	3.76%	0.527%
11	3.411	635	644	647	rBV3	296	525	0.03%	0.005%
12	3.758	748	752	755	rBB2	319	237	0.01%	0.002%
13	3.970	814	818	823	rBV2	356	444	0.03%	0.004%
14	4.012	828	831	834	rBV2	247	182	0.01%	0.002%
15	4.092	852	856	861	rVB2	316	300	0.02%	0.003%
16	4.125	863	866	870	rBV2	311	226	0.01%	0.002%
17	4.163	874	878	881	rVB3	247	172	0.01%	0.001%
18	4.195	882	888	892	rBV3	471	587	0.04%	0.005%
19	4.234	897	900	902	rBV2	224	148	0.01%	0.001%
20	4.269	908	911	914	rVB2	297	169	0.01%	0.001%
21	4.318	924	926	928	rBV2	254	167	0.01%	0.001%
22	4.488	977	979	982	rBV	399	185	0.01%	0.002%
23	4.527	988	991	996	rVB2	438	445	0.03%	0.004%
24	4.549	996	998	1001	rVB	234	141	0.01%	0.001%
25	4.620	1001	1020	1063	rBV	156451	427564	26.52%	3.713%
26	4.903	1104	1108	1109	rBV2	295	201	0.01%	0.002%
27	5.060	1140	1157	1184	rBV	282285	617633	38.32%	5.364%
28	5.218	1201	1206	1207	rBV	415	319	0.02%	0.003%
29	5.260	1215	1219	1221	rBV	372	304	0.02%	0.003%
30	5.356	1246	1249	1251	rBV2	292	208	0.01%	0.002%
31	5.427	1268	1271	1273	rVV	298	176	0.01%	0.002%
32	5.449	1276	1278	1283	rVB2	212	175	0.01%	0.002%
33	5.507	1292	1296	1298	rVB	224	170	0.01%	0.001%
34	5.543	1298	1307	1308	rBV	340	375	0.02%	0.003%
35	5.584	1318	1320	1324	rVB	259	177	0.01%	0.002%
36	5.620	1324	1331	1332	rBV2	252	214	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052629.D
 Acq On : 06 Jan 2023 15:41
 Operator : JC/MD
 Sample : 01036-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

37	5.723	1339	1363	1395	rBV2	590941	1611980	100.00%	13.999%
38	5.973	1437	1441	1443	rBV3	389	365	0.02%	0.003%
39	6.025	1453	1457	1458	rBV	552	418	0.03%	0.004%
40	6.038	1458	1461	1466	rVB2	738	626	0.04%	0.005%
41	6.092	1476	1478	1481	rBV2	346	293	0.02%	0.003%
42	6.247	1510	1526	1550	rBV	434055	824085	51.12%	7.157%
43	6.475	1595	1597	1601	rVB2	260	170	0.01%	0.001%
44	6.494	1601	1603	1606	rBV2	351	189	0.01%	0.002%
45	6.533	1608	1615	1618	rBV3	745	800	0.05%	0.007%
46	6.549	1618	1620	1624	rVB2	321	195	0.01%	0.002%
47	6.591	1631	1633	1635	rBV2	263	171	0.01%	0.001%
48	6.623	1640	1643	1646	rBV	238	179	0.01%	0.002%
49	6.687	1647	1663	1685	rBV	386496	753652	46.75%	6.545%
50	6.838	1707	1710	1713	rBV3	436	321	0.02%	0.003%
51	6.925	1733	1737	1740	rBV2	279	300	0.02%	0.003%
52	7.070	1777	1782	1785	rBV2	378	408	0.03%	0.004%
53	7.108	1790	1794	1798	rVB2	373	287	0.02%	0.002%
54	7.131	1798	1801	1804	rBV2	343	262	0.02%	0.002%
55	7.186	1810	1818	1830	rVB4	1548	2673	0.17%	0.023%
56	7.237	1830	1834	1839	rBV3	338	369	0.02%	0.003%
57	7.369	1872	1875	1876	rBV2	271	177	0.01%	0.002%
58	7.398	1881	1884	1891	rVV2	368	439	0.03%	0.004%
59	7.436	1891	1896	1898	rVB3	288	257	0.02%	0.002%
60	7.562	1922	1935	1962	rVV	190444	340143	21.10%	2.954%
61	7.896	2024	2039	2055	rBV	663394	1147947	71.21%	9.969%
62	8.060	2087	2090	2093	rBV3	307	220	0.01%	0.002%
63	8.099	2099	2102	2104	rBV3	298	185	0.01%	0.002%
64	8.176	2113	2126	2147	rBV	136500	233461	14.48%	2.027%
65	8.449	2207	2211	2212	rBV2	322	234	0.01%	0.002%
66	8.468	2212	2217	2221	rVV3	1091	1392	0.09%	0.012%
67	8.584	2247	2253	2255	rBV3	272	295	0.02%	0.003%
68	8.632	2255	2268	2302	rBV2	420107	797102	49.45%	6.922%
69	8.829	2326	2329	2334	rBV5	424	457	0.03%	0.004%
70	9.028	2389	2391	2394	rBV2	244	144	0.01%	0.001%
71	9.282	2466	2470	2473	rVV3	377	345	0.02%	0.003%
72	9.414	2496	2511	2533	rBV	607972	996813	61.84%	8.657%
73	9.687	2593	2596	2598	rBV2	228	154	0.01%	0.001%
74	9.758	2615	2618	2624	rVB3	307	399	0.02%	0.003%
75	9.793	2624	2629	2631	rBV	473	388	0.02%	0.003%
76	9.825	2636	2639	2641	rBV	247	153	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052629.D
 Acq On : 06 Jan 2023 15:41
 Operator : JC/MD
 Sample : 01036-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

77	10.012	2694	2697	2700	rBV	261	199	0.01%	0.002%
78	10.031	2700	2703	2707	rVB2	267	238	0.01%	0.002%
79	10.237	2764	2767	2773	rVB3	324	241	0.01%	0.002%
80	10.423	2822	2825	2827	rBV2	220	146	0.01%	0.001%
81	10.478	2838	2842	2843	rBV2	362	242	0.02%	0.002%
82	10.603	2874	2881	2885	rBV2	390	419	0.03%	0.004%
83	10.642	2885	2893	2894	rBV2	289	389	0.02%	0.003%
84	10.751	2912	2927	2953	rBV	470881	759929	47.14%	6.599%
85	10.867	2960	2963	2964	rBV2	510	275	0.02%	0.002%
86	10.883	2964	2968	2979	rVB5	1550	2369	0.15%	0.021%
87	10.983	2996	2999	3001	rBV	261	202	0.01%	0.002%
88	11.131	3042	3045	3047	rBV3	374	267	0.02%	0.002%
89	11.301	3094	3098	3099	rBV3	339	247	0.02%	0.002%
90	11.327	3103	3106	3111	rVB	271	191	0.01%	0.002%
91	11.362	3114	3117	3119	rBV2	328	202	0.01%	0.002%
92	11.472	3148	3151	3155	rVB3	345	259	0.02%	0.002%
93	11.562	3176	3179	3183	rVB2	585	451	0.03%	0.004%
94	11.581	3183	3185	3187	rBV	267	144	0.01%	0.001%
95	11.738	3230	3234	3235	rBV3	656	454	0.03%	0.004%
96	11.809	3243	3256	3278	rBV	546424	869410	53.93%	7.550%
97	12.060	3324	3334	3353	rBV3	12327	26086	1.62%	0.227%
98	12.189	3361	3374	3400	rBV	603863	952711	59.10%	8.274%
99	12.295	3405	3407	3410	rVB2	818	390	0.02%	0.003%
100	13.841	3884	3888	3895	rVB5	1593	1804	0.11%	0.016%




Sum of corrected areas: 11515049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052629.D
Acq On : 06 Jan 2023 15:41
Operator : JC/MD
Sample : 01036-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

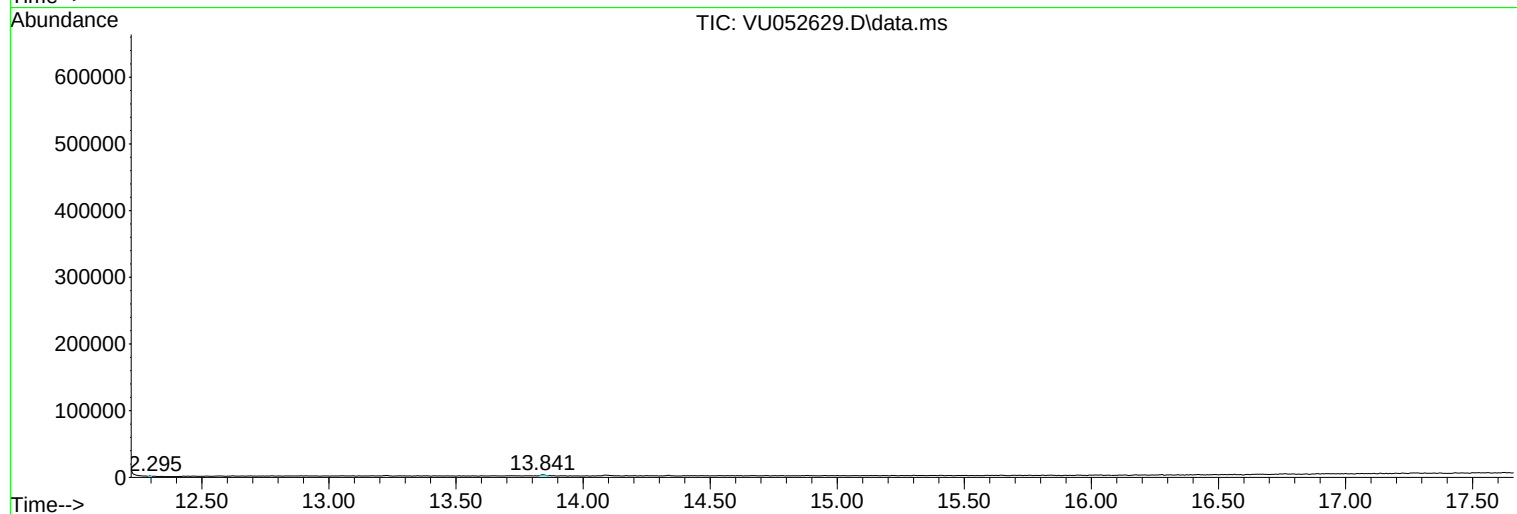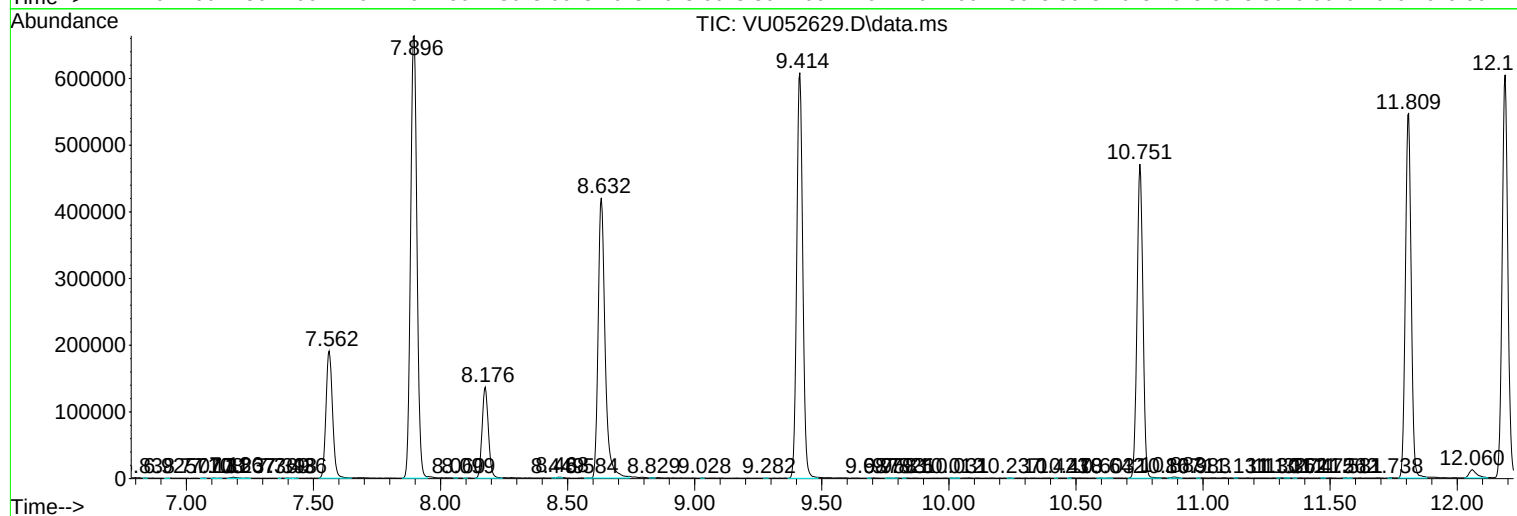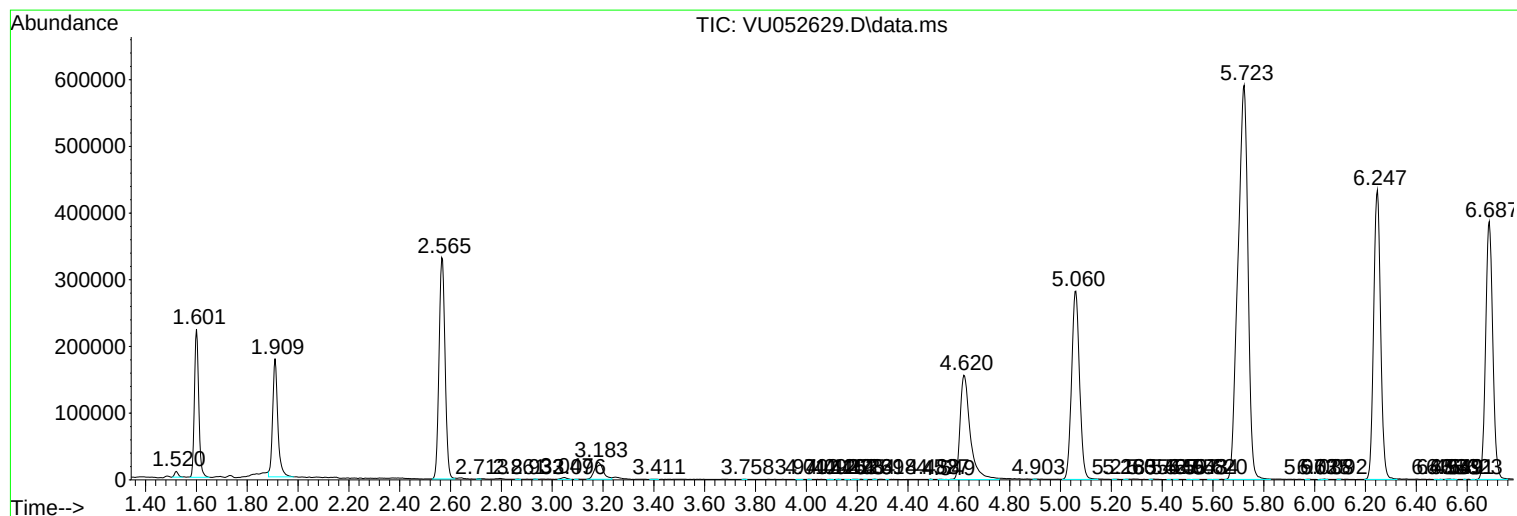

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052629.D
Acq On : 06 Jan 2023 15:41
Operator : JC/MD
Sample : 01036-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052629.D
Acq On : 06 Jan 2023 15:41
Operator : JC/MD
Sample : 01036-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc