

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052631.D
 Acq On : 06 Jan 2023 16:26
 Operator : JC/MD
 Sample : 01036-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	52	56	62	rBV2	4080	4173	0.27%	0.037%
2	1.600	73	81	99	rVB	215123	249574	16.16%	2.216%
3	1.912	170	178	208	rVB	166849	241855	15.66%	2.147%
4	2.565	369	381	395	rBV	317691	513308	33.24%	4.557%
5	2.639	396	404	421	rVB	9045	19179	1.24%	0.170%
6	2.774	442	446	447	rBV	728	444	0.03%	0.004%
7	2.838	463	466	469	rBV2	487	342	0.02%	0.003%
8	3.009	516	519	521	rBV3	357	240	0.02%	0.002%
9	3.041	522	529	539	rVV5	1986	3815	0.25%	0.034%
10	3.186	558	574	587	rBV2	21523	50581	3.28%	0.449%
11	3.661	718	722	726	rBV2	341	349	0.02%	0.003%
12	3.790	757	762	763	rBV2	305	223	0.01%	0.002%
13	3.803	763	766	771	rVV3	364	303	0.02%	0.003%
14	3.899	793	796	802	rVB2	366	271	0.02%	0.002%
15	4.073	847	850	855	rVB	300	278	0.02%	0.002%
16	4.121	861	865	870	rBV2	277	276	0.02%	0.002%
17	4.176	878	882	884	rBV2	312	199	0.01%	0.002%
18	4.192	884	887	892	rVB	300	213	0.01%	0.002%
19	4.411	951	955	959	rVB2	294	294	0.02%	0.003%
20	4.481	974	977	981	rBV2	243	203	0.01%	0.002%
21	4.623	1004	1021	1063	rBV	134889	382060	24.74%	3.392%
22	4.864	1093	1096	1099	rBV2	333	256	0.02%	0.002%
23	4.925	1111	1115	1118	rBV3	291	257	0.02%	0.002%
24	5.060	1139	1157	1178	rBV	272741	602045	38.98%	5.345%
25	5.192	1194	1198	1200	rBV3	321	242	0.02%	0.002%
26	5.253	1213	1217	1219	rBV3	386	255	0.02%	0.002%
27	5.279	1219	1225	1226	rBV2	459	372	0.02%	0.003%
28	5.378	1250	1256	1259	rVV2	564	567	0.04%	0.005%
29	5.430	1269	1272	1274	rVV3	311	229	0.01%	0.002%
30	5.462	1278	1282	1285	rBV3	329	279	0.02%	0.002%
31	5.520	1297	1300	1304	rVB3	301	261	0.02%	0.002%
32	5.558	1309	1312	1315	rBV	239	215	0.01%	0.002%
33	5.722	1341	1363	1391	rBV2	569656	1544370	100.00%	13.711%
34	5.841	1397	1400	1408	rVB3	523	422	0.03%	0.004%
35	6.009	1449	1452	1454	rBV	400	246	0.02%	0.002%
36	6.247	1512	1526	1547	rBV	423332	798926	51.73%	7.093%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052631.D
 Acq On : 06 Jan 2023 16:26
 Operator : JC/MD
 Sample : 01036-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

37	6.414	1576	1578	1585	rVB2	351	353	0.02%	0.003%
38	6.523	1605	1612	1620	rVB6	752	1078	0.07%	0.010%
39	6.587	1626	1632	1633	rBV3	274	239	0.02%	0.002%
40	6.687	1648	1663	1687	rBV	378062	728751	47.19%	6.470%
41	6.787	1690	1694	1695	rBV4	266	200	0.01%	0.002%
42	6.800	1696	1698	1701	rVB2	479	225	0.01%	0.002%
43	6.941	1738	1742	1745	rBV3	282	214	0.01%	0.002%
44	7.057	1775	1778	1783	rVB2	299	264	0.02%	0.002%
45	7.124	1796	1799	1802	rVB2	385	256	0.02%	0.002%
46	7.147	1802	1806	1809	rBV2	467	425	0.03%	0.004%
47	7.173	1811	1814	1816	rBV2	533	400	0.03%	0.004%
48	7.185	1816	1818	1824	rVB5	672	475	0.03%	0.004%
49	7.234	1830	1833	1839	rVB2	265	290	0.02%	0.003%
50	7.317	1857	1859	1865	rVB2	352	292	0.02%	0.003%
51	7.404	1884	1886	1890	rVB2	445	263	0.02%	0.002%
52	7.430	1890	1894	1896	rBV3	323	327	0.02%	0.003%
53	7.504	1914	1917	1923	rVB	295	269	0.02%	0.002%
54	7.562	1923	1935	1953	rBV	187829	328025	21.24%	2.912%
55	7.677	1969	1971	1972	rVV	451	207	0.01%	0.002%
56	7.687	1972	1974	1978	rVB4	613	416	0.03%	0.004%
57	7.780	1999	2003	2006	rBV2	288	290	0.02%	0.003%
58	7.893	2025	2038	2061	rBV	642146	1103425	71.45%	9.796%
59	8.008	2072	2074	2078	rVB2	539	380	0.02%	0.003%
60	8.044	2082	2085	2087	rBV2	321	208	0.01%	0.002%
61	8.176	2112	2126	2142	rBV	129025	222512	14.41%	1.975%
62	8.443	2203	2209	2210	rVV3	441	425	0.03%	0.004%
63	8.468	2213	2217	2227	rVB3	1801	2480	0.16%	0.022%
64	8.635	2255	2269	2306	rBV2	391776	773546	50.09%	6.867%
65	8.893	2346	2349	2355	rVB2	631	518	0.03%	0.005%
66	8.941	2360	2364	2365	rBV2	311	244	0.02%	0.002%
67	9.086	2403	2409	2414	rBV3	284	320	0.02%	0.003%
68	9.217	2445	2450	2454	rBV2	479	487	0.03%	0.004%
69	9.275	2464	2468	2470	rBV3	297	256	0.02%	0.002%
70	9.343	2485	2489	2492	rBV2	331	258	0.02%	0.002%
71	9.414	2498	2511	2530	rBV	597410	985821	63.83%	8.752%
72	9.632	2574	2579	2582	rBV3	199	216	0.01%	0.002%
73	9.697	2592	2599	2604	rBV4	497	753	0.05%	0.007%
74	9.896	2656	2661	2665	rBV3	311	354	0.02%	0.003%
75	9.979	2682	2687	2694	rVB3	389	602	0.04%	0.005%
76	10.025	2698	2701	2704	rBV3	294	203	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052631.D
 Acq On : 06 Jan 2023 16:26
 Operator : JC/MD
 Sample : 01036-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

77	10.044	2704	2707	2711	rVB2	410	281	0.02%	0.002%
78	10.066	2711	2714	2719	rVB	367	270	0.02%	0.002%
79	10.246	2764	2770	2775	rBV2	437	450	0.03%	0.004%
80	10.298	2781	2786	2789	rBV3	304	333	0.02%	0.003%
81	10.340	2797	2799	2804	rVB3	336	245	0.02%	0.002%
82	10.394	2807	2816	2818	rBV2	453	588	0.04%	0.005%
83	10.594	2876	2878	2883	rVB	335	280	0.02%	0.002%
84	10.626	2883	2888	2891	rBV2	529	493	0.03%	0.004%
85	10.648	2891	2895	2898	rBV2	328	291	0.02%	0.003%
86	10.751	2915	2927	2948	rVV	464952	748958	48.50%	6.649%
87	10.889	2968	2970	2982	rVB5	1564	1795	0.12%	0.016%
88	10.967	2991	2994	2996	rBV	379	250	0.02%	0.002%
89	10.986	2997	3000	3004	rVB2	359	301	0.02%	0.003%
90	11.124	3039	3043	3044	rBV	478	361	0.02%	0.003%
91	11.262	3083	3086	3090	rBV2	282	275	0.02%	0.002%
92	11.394	3124	3127	3129	rBV2	319	223	0.01%	0.002%
93	11.475	3147	3152	3158	rBV4	933	1088	0.07%	0.010%
94	11.655	3204	3208	3213	rBV2	547	682	0.04%	0.006%
95	11.745	3227	3236	3243	rBV4	2403	3658	0.24%	0.032%
96	11.809	3243	3256	3287	rBV	570287	904178	58.55%	8.027%
97	12.060	3324	3334	3345	rBV3	12925	24171	1.57%	0.215%
98	12.143	3357	3360	3362	rBV	682	429	0.03%	0.004%
99	12.188	3362	3374	3393	rVV	605222	1000485	64.78%	8.882%
100	12.471	3454	3462	3463	rBV2	460	602	0.04%	0.005%


Sum of corrected areas: 11264076

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052631.D
Acq On : 06 Jan 2023 16:26
Operator : JC/MD
Sample : 01036-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

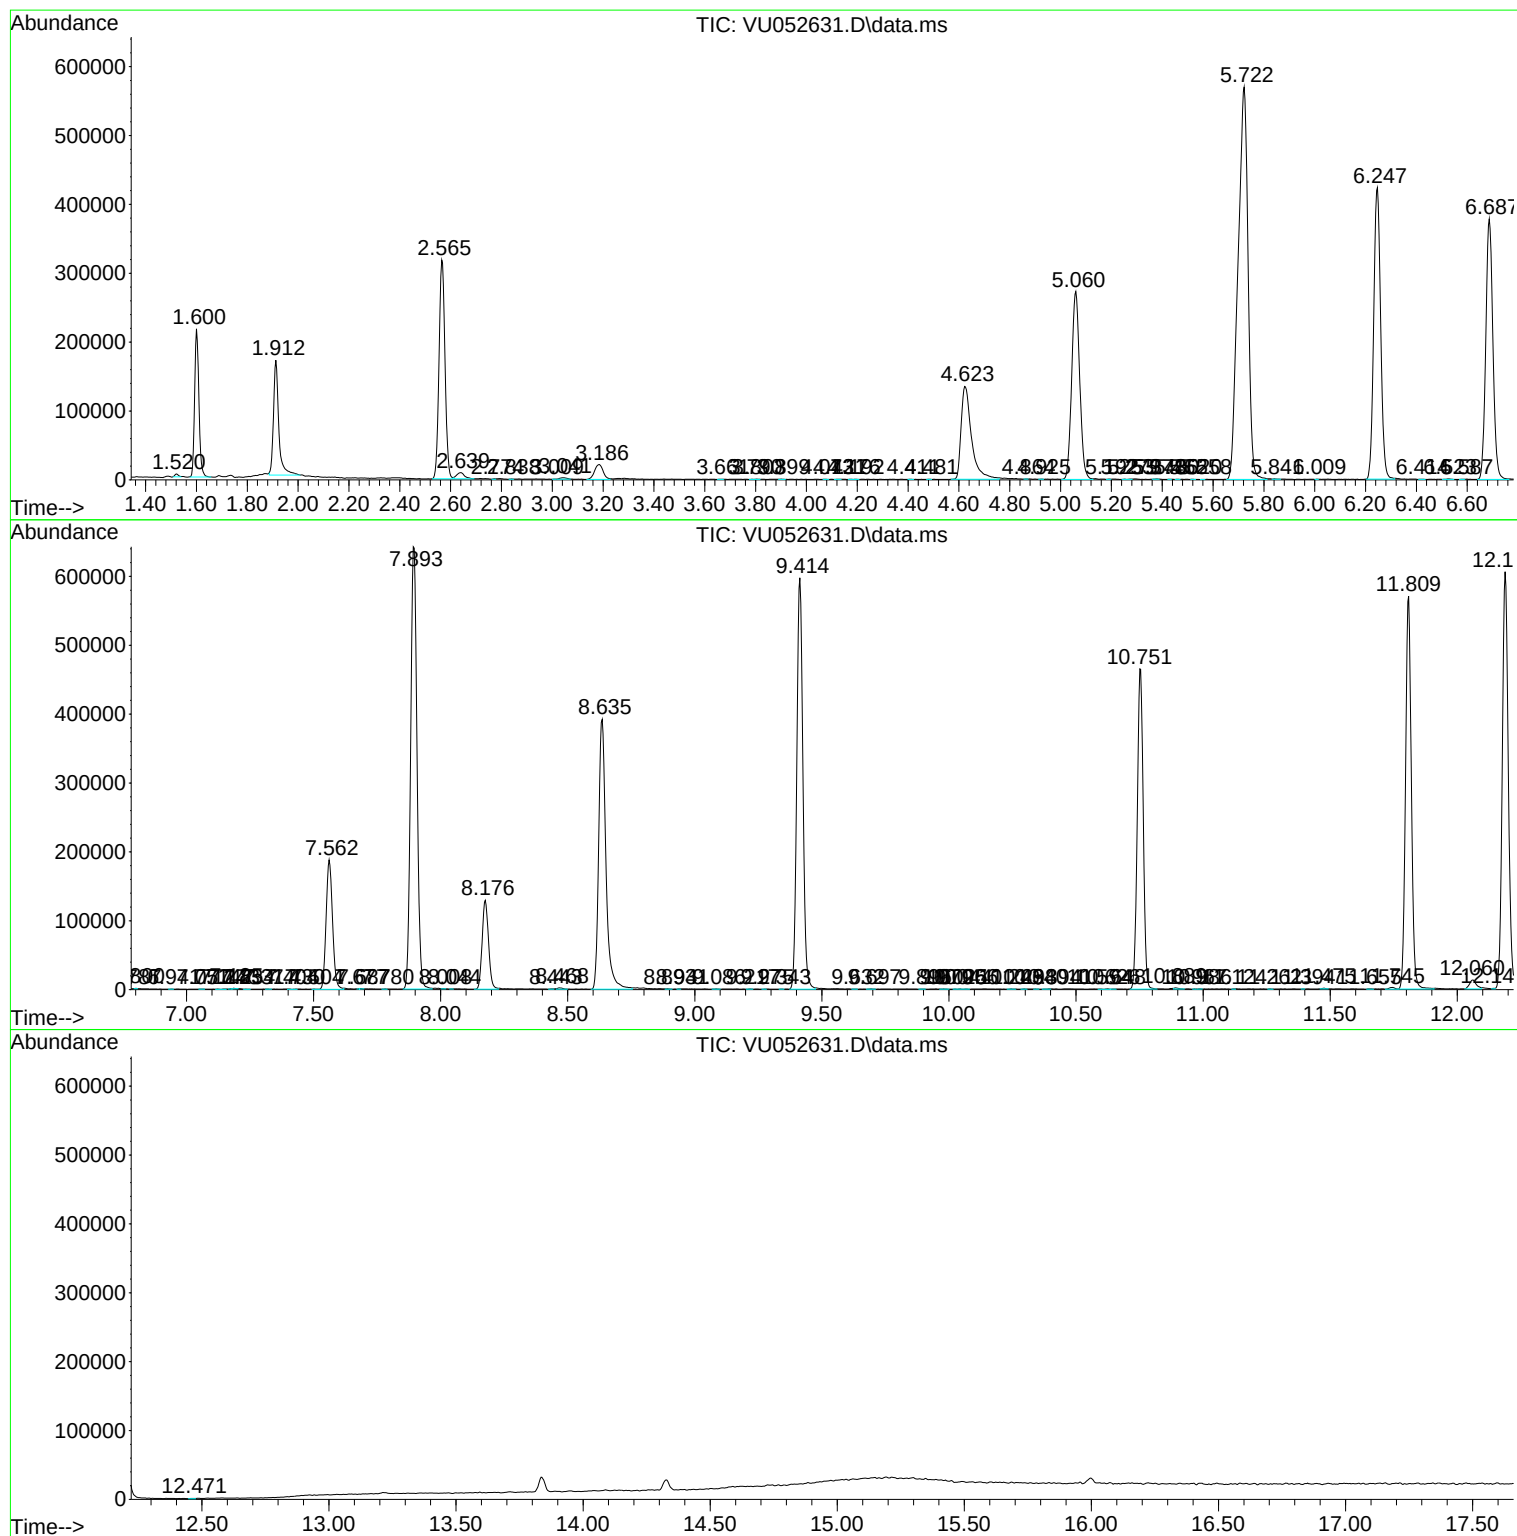

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052631.D
Acq On : 06 Jan 2023 16:26
Operator : JC/MD
Sample : 01036-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052631.D
Acq On : 06 Jan 2023 16:26
Operator : JC/MD
Sample : 01036-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc