

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052632.D
 Acq On : 06 Jan 2023 17:44
 Operator : JC/MD
 Sample : 01036-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	42	47	61	rBV	26543	30775	2.05%	0.273%
2	1.600	73	81	101	rVB	216118	251194	16.75%	2.228%
3	1.909	170	177	194	rVB	162725	225685	15.05%	2.002%
4	2.568	369	382	396	rBV	313121	510053	34.01%	4.525%
5	2.633	397	402	419	rVB3	3668	7657	0.51%	0.068%
6	2.710	423	426	428	rBV2	572	323	0.02%	0.003%
7	2.800	445	454	462	rVV3	937	1563	0.10%	0.014%
8	2.864	471	474	478	rBV3	391	326	0.02%	0.003%
9	2.951	497	501	505	rVB3	452	432	0.03%	0.004%
10	3.047	521	531	541	rVB2	4256	7830	0.52%	0.069%
11	3.179	567	572	577	rBV3	759	1022	0.07%	0.009%
12	3.266	596	599	603	rVB3	390	289	0.02%	0.003%
13	3.472	661	663	667	rBV3	272	234	0.02%	0.002%
14	3.575	691	695	698	rBV2	278	223	0.01%	0.002%
15	3.874	786	788	794	rVB3	403	320	0.02%	0.003%
16	3.964	811	816	823	rVB3	270	368	0.02%	0.003%
17	4.009	827	830	834	rBV2	307	270	0.02%	0.002%
18	4.124	862	866	869	rBV2	439	365	0.02%	0.003%
19	4.256	902	907	910	rVB2	338	273	0.02%	0.002%
20	4.292	916	918	925	rVV2	241	267	0.02%	0.002%
21	4.382	943	946	949	rVB3	321	217	0.01%	0.002%
22	4.407	950	954	958	rBV2	493	361	0.02%	0.003%
23	4.430	958	961	964	rBV2	341	237	0.02%	0.002%
24	4.620	1006	1020	1053	rBV	177194	461535	30.77%	4.094%
25	4.944	1117	1121	1124	rVB4	478	332	0.02%	0.003%
26	4.967	1124	1128	1132	rVB3	507	389	0.03%	0.003%
27	5.060	1140	1157	1180	rBV	261341	573521	38.24%	5.088%
28	5.205	1198	1202	1204	rBV3	307	221	0.01%	0.002%
29	5.279	1220	1225	1226	rBV3	672	485	0.03%	0.004%
30	5.359	1248	1250	1253	rVV3	425	332	0.02%	0.003%
31	5.378	1253	1256	1262	rVB4	696	610	0.04%	0.005%
32	5.507	1292	1296	1299	rVB2	269	228	0.02%	0.002%
33	5.526	1299	1302	1307	rVB2	288	217	0.01%	0.002%
34	5.555	1307	1311	1317	rBV2	503	645	0.04%	0.006%
35	5.722	1338	1363	1385	rBV2	552025	1499925	100.00%	13.305%
36	5.964	1433	1438	1441	rBV3	357	399	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052632.D
 Acq On : 06 Jan 2023 17:44
 Operator : JC/MD
 Sample : 01036-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

37	6.002	1448	1450	1453	rVB2	438	220	0.01%	0.002%
38	6.034	1453	1460	1463	rBV5	604	825	0.06%	0.007%
39	6.108	1481	1483	1489	rVB4	405	353	0.02%	0.003%
40	6.147	1489	1495	1499	rBV2	366	400	0.03%	0.004%
41	6.247	1511	1526	1558	rBV	426894	804461	53.63%	7.136%
42	6.436	1581	1585	1589	rVB3	349	271	0.02%	0.002%
43	6.526	1608	1613	1619	rVB6	988	1179	0.08%	0.010%
44	6.687	1649	1663	1688	rBV	360799	702374	46.83%	6.231%
45	6.800	1694	1698	1705	rBV5	721	884	0.06%	0.008%
46	6.864	1715	1718	1721	rBV	398	240	0.02%	0.002%
47	6.899	1726	1729	1732	rVB	378	221	0.01%	0.002%
48	6.922	1732	1736	1738	rBV2	377	348	0.02%	0.003%
49	7.015	1762	1765	1769	rVB2	424	315	0.02%	0.003%
50	7.041	1769	1773	1777	rBV2	339	256	0.02%	0.002%
51	7.185	1810	1818	1828	rBV4	1528	2413	0.16%	0.021%
52	7.562	1923	1935	1955	rBV	180613	321770	21.45%	2.854%
53	7.690	1969	1975	1983	rVB5	1107	1770	0.12%	0.016%
54	7.758	1993	1996	2000	rVB2	400	292	0.02%	0.003%
55	7.780	2000	2003	2006	rBV	529	377	0.03%	0.003%
56	7.896	2025	2039	2060	rBV	627479	1067292	71.16%	9.468%
57	8.082	2092	2097	2099	rVB2	425	364	0.02%	0.003%
58	8.102	2100	2103	2110	rVB3	537	589	0.04%	0.005%
59	8.176	2113	2126	2144	rBV	129768	221198	14.75%	1.962%
60	8.426	2202	2204	2210	rBV2	414	386	0.03%	0.003%
61	8.488	2220	2223	2227	rVB3	456	321	0.02%	0.003%
62	8.632	2254	2268	2296	rBV	519556	971037	64.74%	8.614%
63	8.935	2356	2362	2365	rBV2	628	699	0.05%	0.006%
64	8.989	2375	2379	2382	rBV2	261	227	0.02%	0.002%
65	9.008	2382	2385	2389	rVB3	361	289	0.02%	0.003%
66	9.115	2415	2418	2420	rVB4	361	227	0.02%	0.002%
67	9.131	2420	2423	2427	rVB	364	266	0.02%	0.002%
68	9.172	2432	2436	2437	rBV	380	228	0.02%	0.002%
69	9.414	2496	2511	2531	rBV	601788	990035	66.01%	8.782%
70	9.584	2563	2564	2567	rVB2	483	227	0.02%	0.002%
71	9.697	2592	2599	2610	rVB3	892	1421	0.09%	0.013%
72	9.754	2610	2617	2624	rBV3	497	776	0.05%	0.007%
73	9.816	2632	2636	2641	rBV3	339	356	0.02%	0.003%
74	9.841	2641	2644	2650	rVB2	494	376	0.03%	0.003%
75	9.870	2650	2653	2657	rBV3	368	386	0.03%	0.003%
76	10.047	2701	2708	2709	rBV	431	430	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052632.D
 Acq On : 06 Jan 2023 17:44
 Operator : JC/MD
 Sample : 01036-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

77	10.079	2713	2718	2720	rBV2	258	257	0.02%	0.002%
78	10.121	2728	2731	2736	rVB5	698	537	0.04%	0.005%
79	10.227	2760	2764	2767	rBV	281	251	0.02%	0.002%
80	10.439	2826	2830	2834	rVB3	256	220	0.01%	0.002%
81	10.481	2840	2843	2845	rBV	314	260	0.02%	0.002%
82	10.526	2854	2857	2862	rBV2	368	377	0.03%	0.003%
83	10.626	2881	2888	2891	rBV3	452	519	0.03%	0.005%
84	10.658	2896	2898	2903	rBV	275	236	0.02%	0.002%
85	10.751	2913	2927	2946	rBV	491622	788576	52.57%	6.995%
86	10.886	2966	2969	2973	rBV2	291	247	0.02%	0.002%
87	10.989	2997	3001	3007	rVB3	394	486	0.03%	0.004%
88	11.089	3029	3032	3038	rVB2	309	352	0.02%	0.003%
89	11.127	3038	3044	3045	rBV2	832	748	0.05%	0.007%
90	11.217	3068	3072	3075	rBV	402	312	0.02%	0.003%
91	11.385	3122	3124	3130	rVB2	408	377	0.03%	0.003%
92	11.417	3130	3134	3137	rBV2	425	321	0.02%	0.003%
93	11.439	3137	3141	3144	rBV2	567	439	0.03%	0.004%
94	11.516	3160	3165	3169	rBV3	468	514	0.03%	0.005%
95	11.664	3203	3211	3214	rBV3	536	830	0.06%	0.007%
96	11.738	3230	3234	3240	rVB5	767	901	0.06%	0.008%
97	11.809	3243	3256	3277	rBV	562595	885196	59.02%	7.852%
98	12.188	3361	3374	3395	rBV	568013	910211	60.68%	8.074%
99	13.841	3883	3888	3893	rVB4	2538	2619	0.17%	0.023%
100	14.330	4034	4040	4047	rBV8	2220	2996	0.20%	0.027%


Sum of corrected areas: 11273004

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052632.D
Acq On : 06 Jan 2023 17:44
Operator : JC/MD
Sample : 01036-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

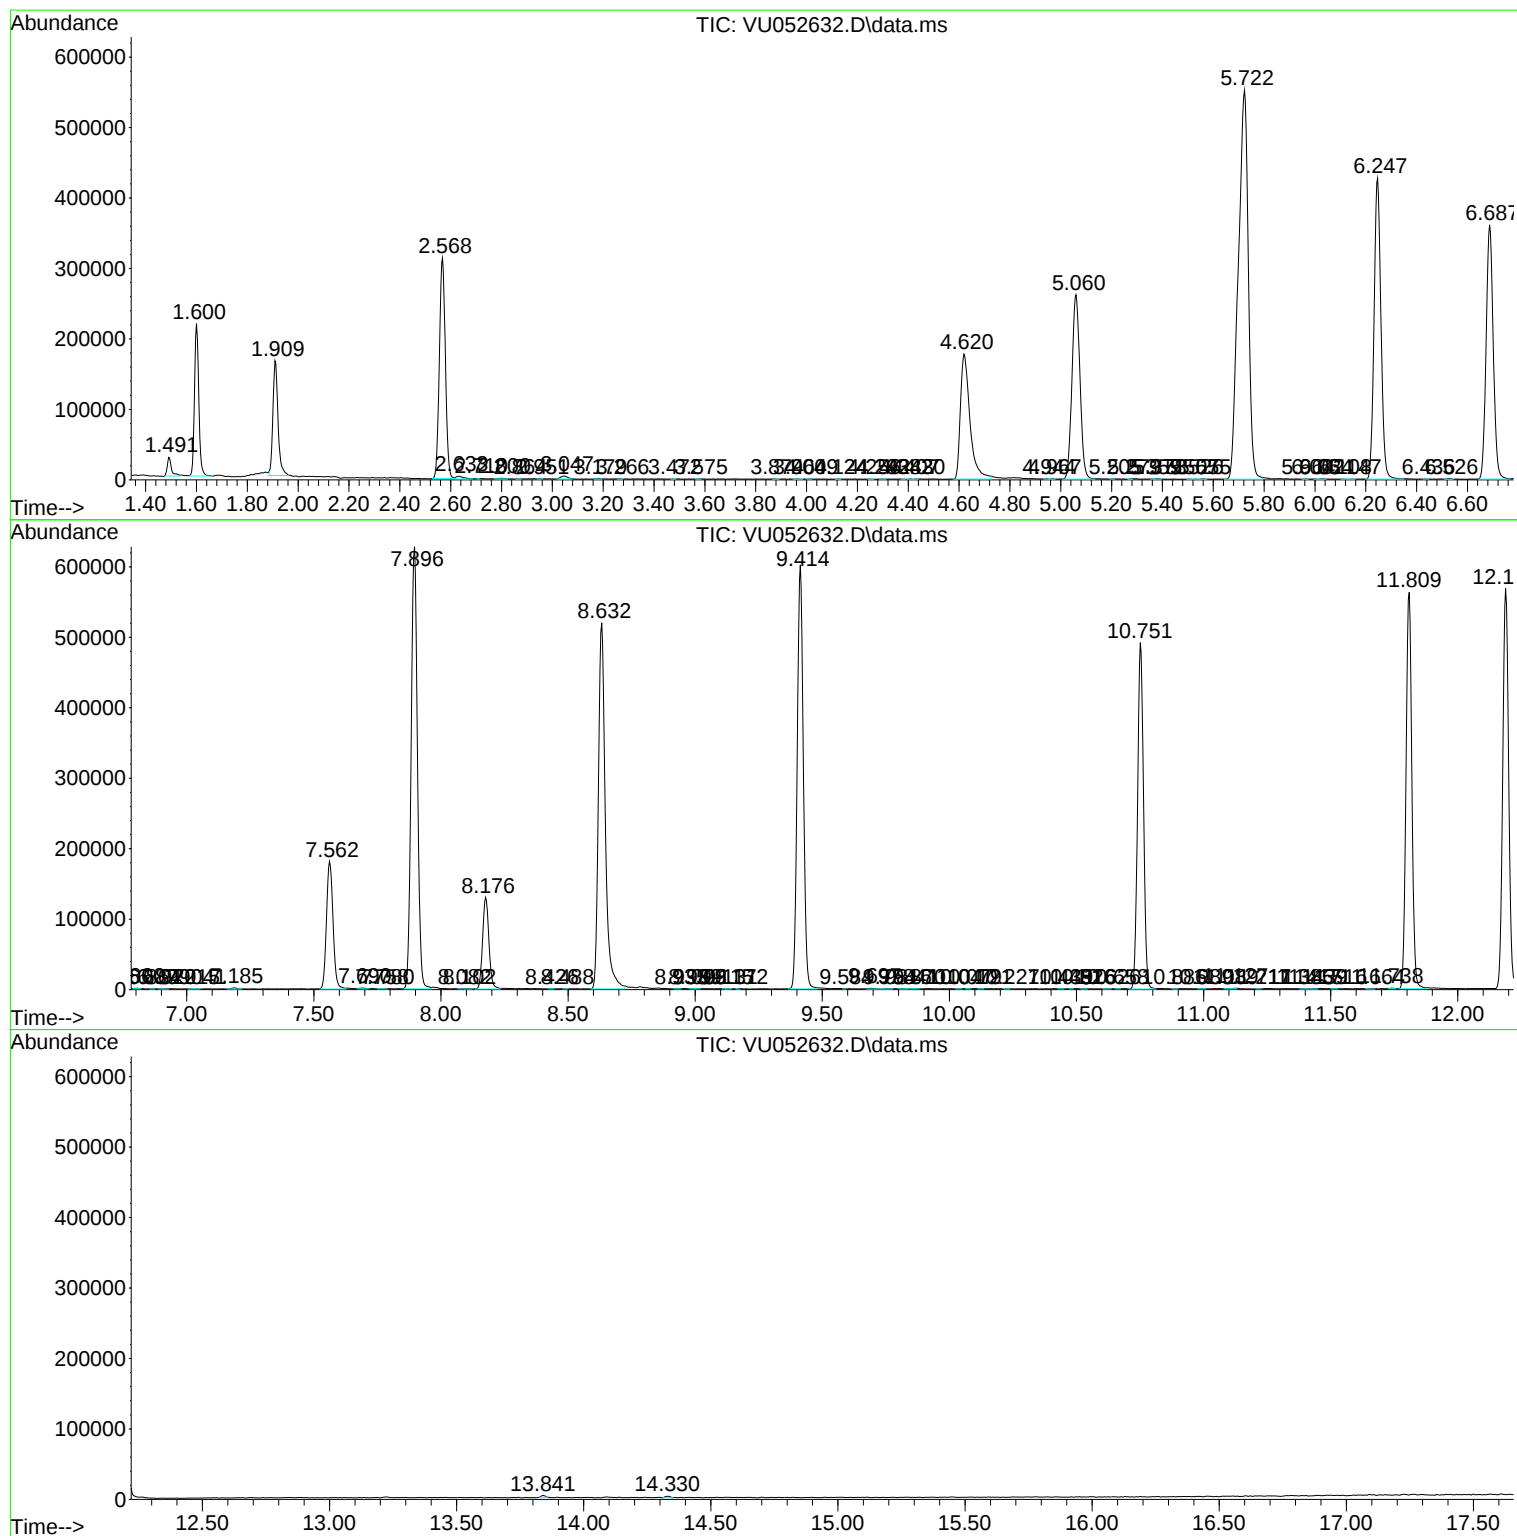

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052632.D
Acq On : 06 Jan 2023 17:44
Operator : JC/MD
Sample : 01036-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052632.D
Acq On : 06 Jan 2023 17:44
Operator : JC/MD
Sample : 01036-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------