
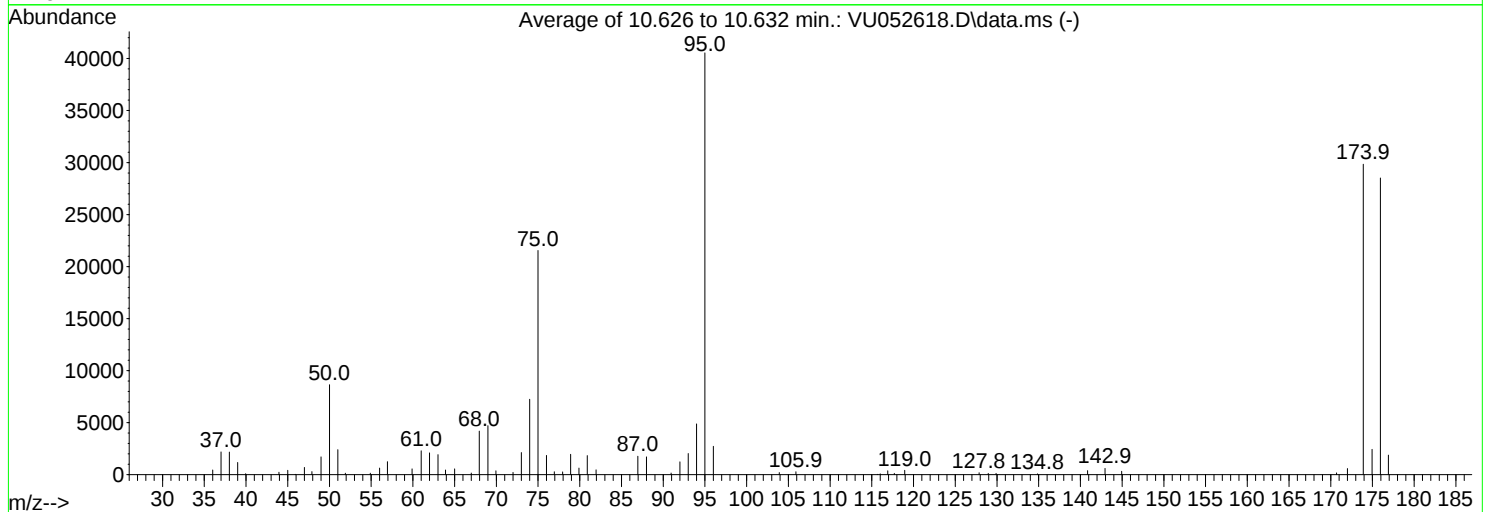


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052618.D
Acq On : 06 Jan 2023 10:08
Operator : JC/MD
Sample : BFB151
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB151

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Title : VOC Analysis
Last Update : Sat Jan 07 00:30:36 2023

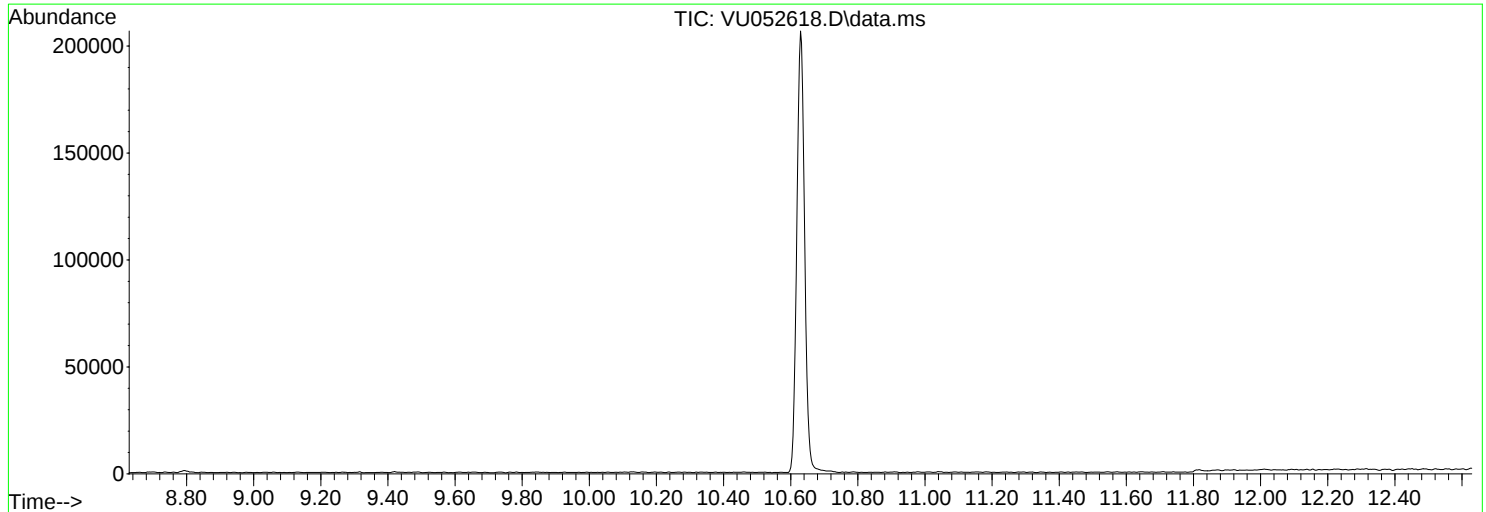

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.3	8639	PASS
75	95	30	80	53.2	21555	PASS
95	95	100	100	100.0	40547	PASS
96	95	5	9	6.7	2720	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.6	29832	PASS
175	174	5	9	8.1	2424	PASS
176	174	95	101	95.6	28517	PASS
177	176	5	9	6.6	1883	PASS

Scan 2876 (10.587 min): VU052618.D\data.ms
BFB151

m/z	Abundance
39.90	108.0
43.90	605.0

Instrument :
MSVOA_U
ClientSampleId :
BFB151

m/z	Abundance
36.00	393.0
37.00	2162.0
38.00	2126.0
39.00	1167.0
40.10	201.0
44.00	851.0
45.00	367.0
47.00	787.0
48.00	291.0
49.00	1620.0
50.00	8717.0
51.00	2203.0
51.90	125.0
54.90	140.0
56.00	603.0
57.00	1203.0
59.90	564.0
61.00	2269.0
62.00	2091.0
63.00	1940.0
63.90	470.0
65.00	614.0
67.00	121.0
68.00	4123.0
69.00	4512.0
70.00	386.0
72.00	201.0
73.00	2102.0
74.00	7328.0
75.00	21032.0
76.00	1945.0
76.90	262.0
78.00	221.0
78.90	1954.0
79.90	557.0
80.90	1813.0
81.90	435.0
86.90	1675.0
88.00	1670.0
90.90	172.0
92.00	1134.0
93.00	1757.0
94.00	4629.0
95.00	39616.0
96.00	2611.0
103.90	179.0
105.90	269.0
116.00	108.0
116.90	308.0
117.70	111.0
118.90	435.0
127.80	184.0
128.90	112.0
129.90	114.0
140.90	360.0
142.90	549.0
145.00	269.0
170.70	169.0
172.00	511.0
173.90	27920.0
174.90	2430.0
175.90	27016.0
176.90	1885.0

Instrument :
MSVOA_U
ClientSampleId :
BFB151

m/z	Abundance
36.00	462.0
37.00	2238.0
38.00	2246.0
39.00	1218.0
40.00	224.0
44.00	849.0
45.00	446.0
47.00	741.0
47.90	305.0
49.00	1743.0
50.00	8931.0
51.00	2425.0
51.90	158.0
54.90	129.0
56.00	660.0
57.00	1323.0
59.90	569.0
61.00	2383.0
62.00	2123.0
63.00	1978.0
63.90	452.0
65.00	557.0
67.00	160.0
67.90	4306.0
69.00	4932.0
70.00	372.0
72.00	217.0
73.00	2237.0
74.00	7472.0
75.00	22224.0
76.00	1936.0
77.00	289.0
77.90	253.0
78.90	2064.0
79.90	654.0
80.90	1881.0
82.00	456.0
86.90	1831.0
88.00	1717.0
90.90	146.0
92.00	1286.0
93.00	2096.0
94.00	5039.0
95.00	41584.0
96.00	2831.0
103.90	230.0
105.90	292.0
116.00	118.0
116.90	376.0
117.70	131.0
118.90	425.0
127.80	197.0
128.90	118.0
129.90	123.0
134.80	101.0
140.80	386.0
143.00	603.0
144.90	349.0
170.70	186.0
172.00	586.0
173.90	30752.0
174.90	2521.0
176.00	29384.0
176.90	1978.0

Instrument :
MSVOA_U
ClientSampleId :
BFB151

m/z	Abundance
36.00	464.0
37.00	2133.0
38.00	2155.0
39.00	1107.0
39.90	201.0
44.00	833.0
45.00	436.0
45.90	114.0
47.00	536.0
47.80	301.0
49.00	1754.0
50.00	8268.0
51.00	2576.0
51.90	148.0
54.90	135.0
56.00	637.0
56.90	1210.0
59.90	519.0
61.00	2208.0
62.00	2055.0
63.00	1875.0
63.90	424.0
65.00	489.0
67.00	179.0
67.90	4127.0
69.00	4658.0
69.90	330.0
72.00	213.0
73.00	2047.0
74.00	6950.0
75.00	21408.0
76.00	1660.0
77.00	285.0
77.90	295.0
78.90	1857.0
79.90	681.0
80.90	1789.0
82.00	502.0
87.00	1811.0
88.00	1720.0
91.00	147.0
92.00	1298.0
93.00	2260.0
94.00	4982.0
95.00	40440.0
96.00	2717.0
103.90	219.0
105.90	267.0
115.70	114.0
116.90	413.0
117.70	125.0
119.00	382.0
127.90	190.0
129.00	125.0
129.90	139.0
134.90	130.0
140.80	399.0
143.00	671.0
144.90	361.0
170.70	170.0
172.00	644.0
173.90	30824.0
175.00	2322.0
176.00	29152.0
176.90	1785.0

Instrument :
MSVOA_U
ClientSampleId :
BFB151