

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU010719\
Quantitation Report (QT Reviewed)


Data File : VU029050.D
Acq On : 07 Jan 2019 11:15
Operator : MD/SY
Sample : K1048-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0945

Manual Integrations
APPROVED

MMDadoda
1/8/2019 9:11:22 AM

Quant Time: Jan 08 01:56:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 08 01:37:07 2019
Response via : Initial Calibration

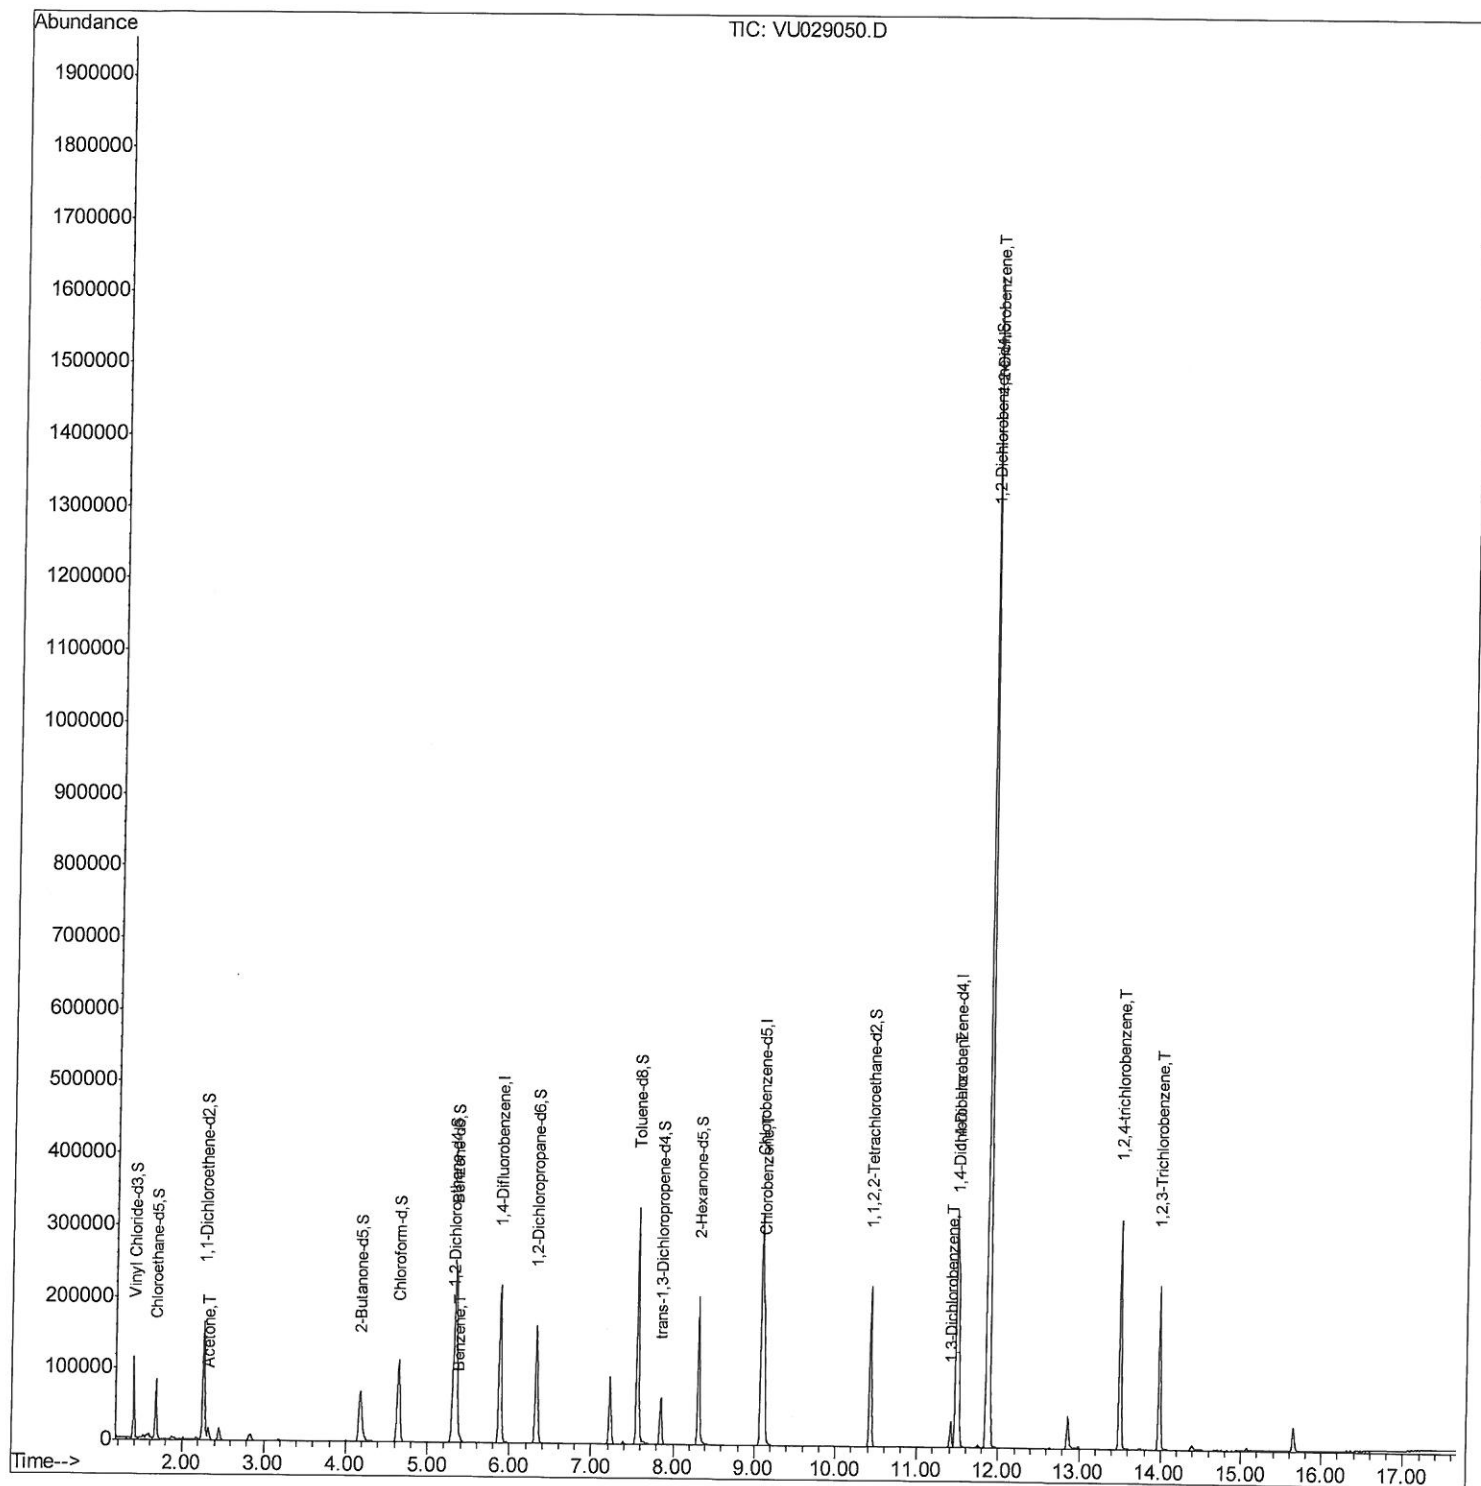

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU010719\
Quantitation Report (Qedit)


Data File : VU029050.D
Acq On : 07 Jan 2019 11:15
Operator : MD/SY
Sample : K1048-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C0945

Manual Integrations
APPROVED

MMDadoda
1/8/2019 9:11:22 AM

Quant Time: Jan 08 01:40:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 08 01:37:07 2019
Response via : Initial Calibration

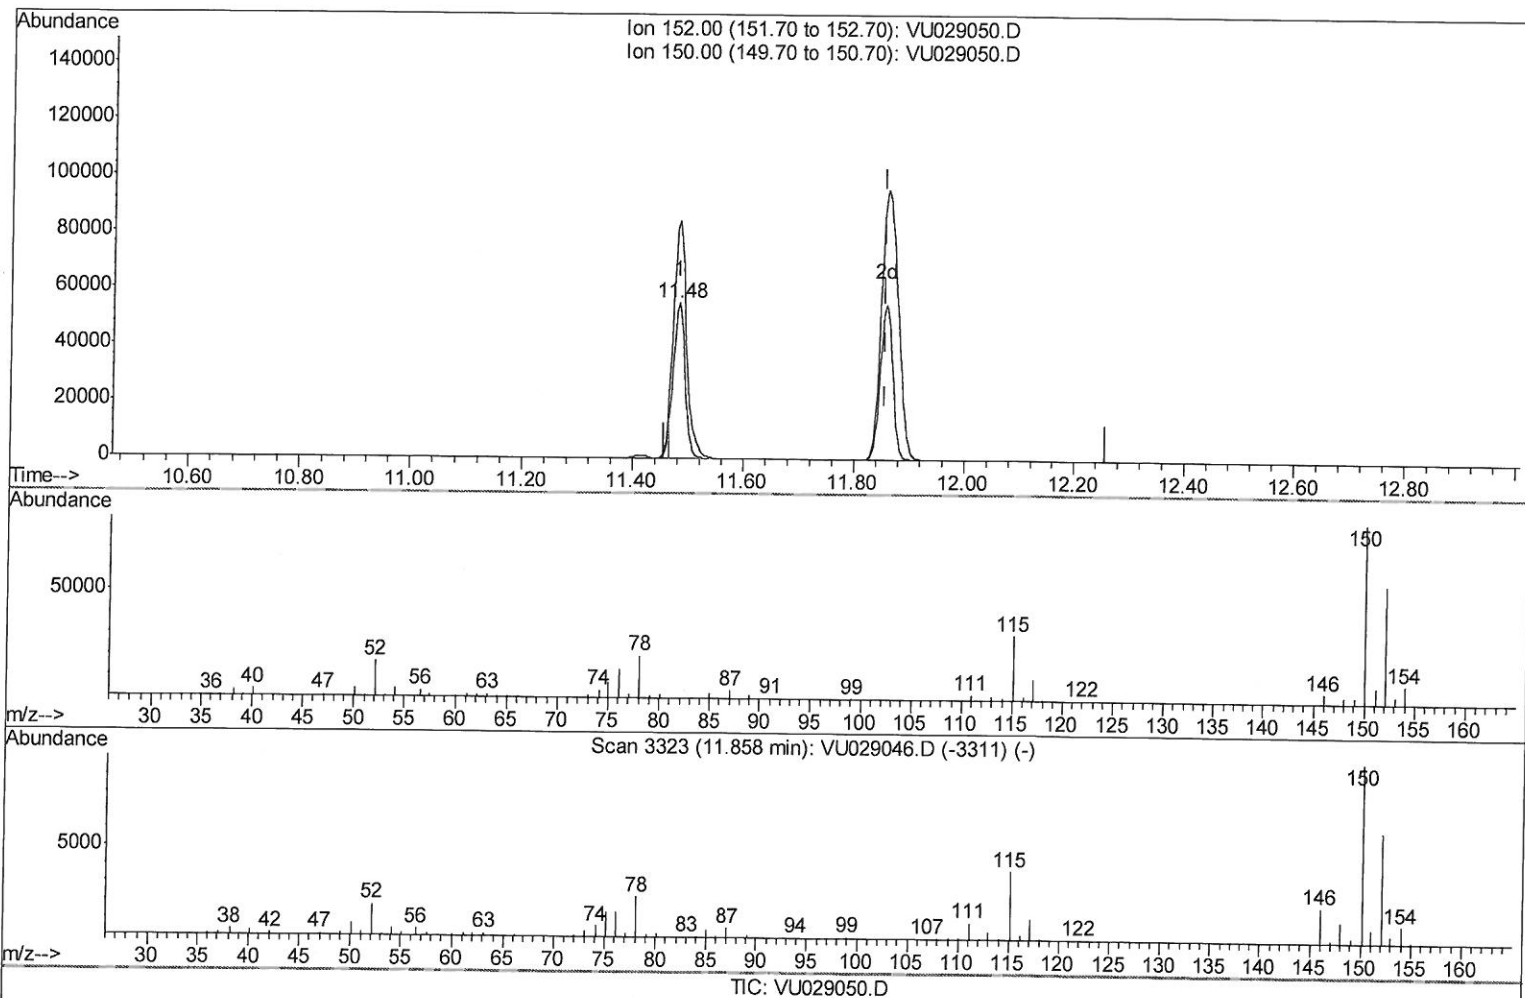

(64) 1,2-Dichlorobenzene-d4 (S)

11.482min (-0.376) 46.00ug/L

response 76327

Ion	Exp%	Act%
152.00	100	100
150.00	174.60	169.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU010719\
Quantitation Report (Qedit)


Data File : VU029050.D
Acq On : 07 Jan 2019 11:15
Operator : MD/SY
Sample : K1048-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C0945

Manual Integrations
APPROVED

MMDadoda
1/8/2019 9:11:22 AM

Quant Time: Jan 08 01:40:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 08 01:37:07 2019
Response via : Initial Calibration

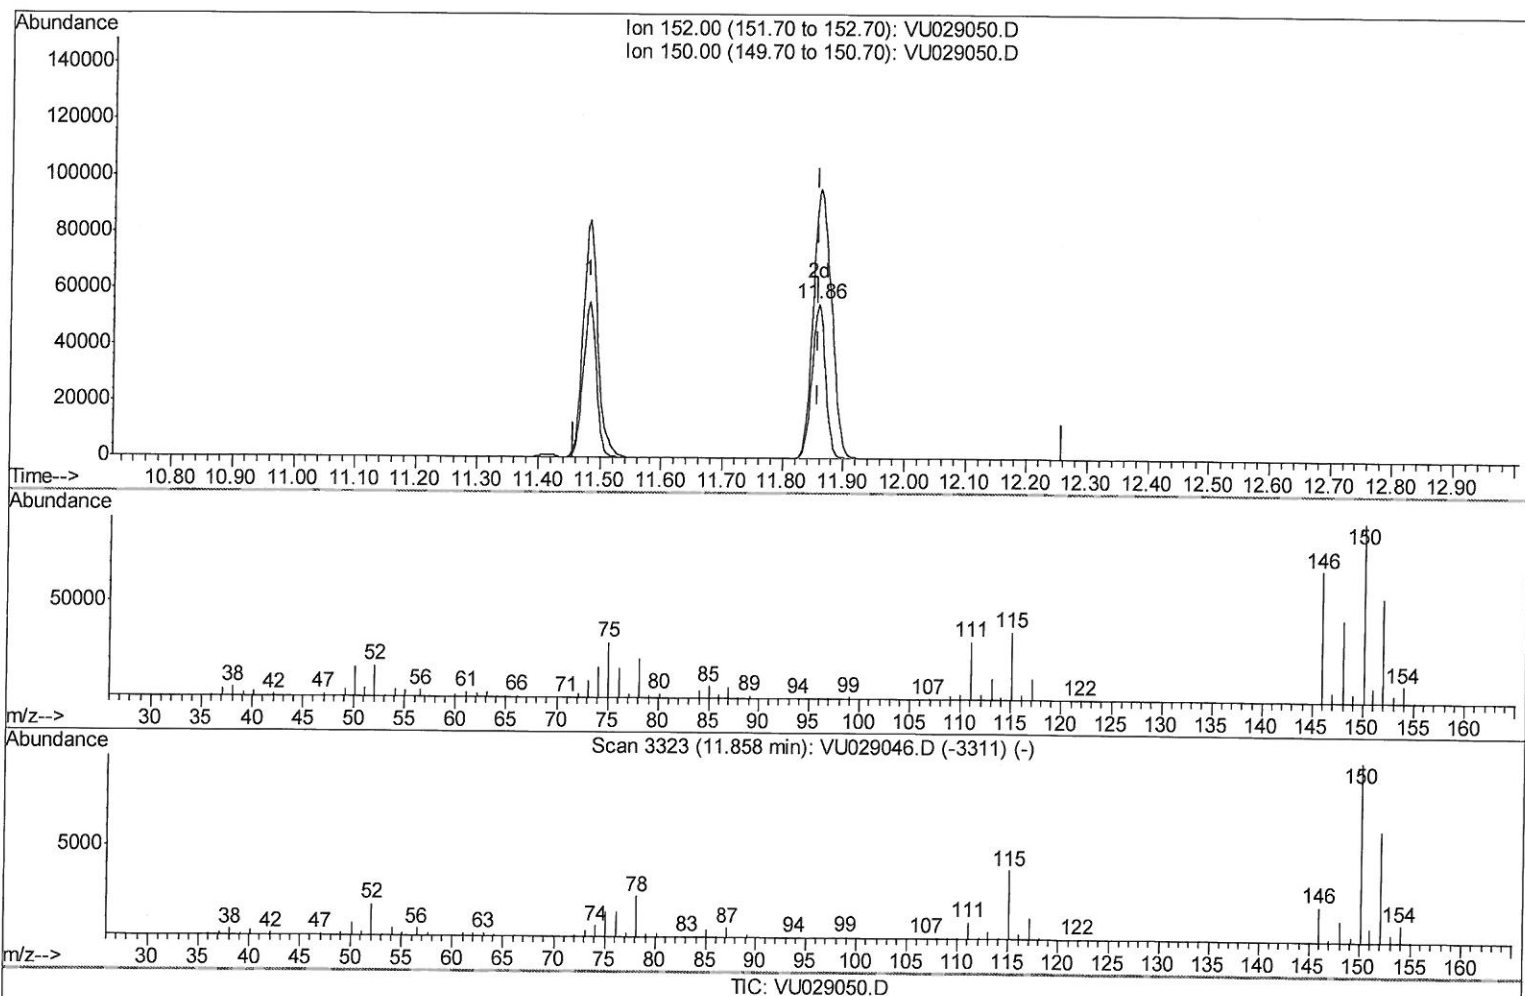

(64) 1,2-Dichlorobenzene-d4 (S)

11.858min (-0.000) 52.04ug/L m

response 86348

Ion Exp% Act%

152.00 100 100

150.00 174.60 149.91

0.00 0.00 0.00

0.00 0.00 0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU010719\
Quantitation Report (QT Reviewed)

Data File : VU029050.D
Acq On : 07 Jan 2019 11:15
Operator : MD/SY
Sample : K1048-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0945

Manual Integrations
APPROVED

MMDadoda
1/8/2019 9:11:22 AM

Quant Time: Jan 08 01:56:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 08 01:37:07 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	188327	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	182426	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	82034	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	74575	49.39	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	98.78%		
7) Chloroethane-d5	1.67	69	58559	50.22	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	100.44%		
11) 1,1-Dichloroethene-d2	2.27	63	93248	36.73	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.46%		
21) 2-Butanone-d5	4.17	46	103422	97.77	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.77%		
24) Chloroform-d	4.65	84	114857	48.38	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.76%		
26) 1,2-Dichloroethane-d4	5.31	65	71829	49.08	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.16%		
32) Benzene-d6	5.34	84	257179	49.90	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.80%		
36) 1,2-Dichloropropane-d6	6.33	67	85910	49.07	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.14%		
41) Toluene-d8	7.56	98	229244	49.08	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.16%		
43) trans-1,3-Dichloropropene-	7.85	79	37485	47.78	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	95.56%		
47) 2-Hexanone-d5	8.31	63	74782	89.93	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.93%		
57) 1,1,2,2-Tetrachloroethane-	10.43	84	118368	48.73	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	97.46%		
64) 1,2-Dichlorobenzene-d4	11.86	152	86348m	52.04	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.08%		

MD
01/08/19

Target Compounds

					Qvalue
13) Acetone	2.32	43	16144	14.976	ug/L 100
33) Benzene	5.39	78	6371	1.097	ug/L 100
51) Chlorobenzene	9.12	112	110705	29.836	ug/L 99
62) 1,3-Dichlorobenzene	11.42	146	15587	5.981	ug/L 97
63) 1,4-Dichlorobenzene	11.50	146	98643	36.741	ug/L 99
65) 1,2-Dichlorobenzene	11.88	146	636992	234.326	ug/L 98
68) 1,2,4-trichlorobenzene	13.50	180	103426	64.281	ug/L 99
70) 1,2,3-Trichlorobenzene	13.99	180	76350	44.007	ug/L 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed