


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010719\
 Data File : VU029045.D
 Acq On : 07 Jan 2019 09:05
 Operator : MD/SY
 Sample : BFB67
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB67

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis
 Last Update : Tue Jan 08 03:12:02 2019

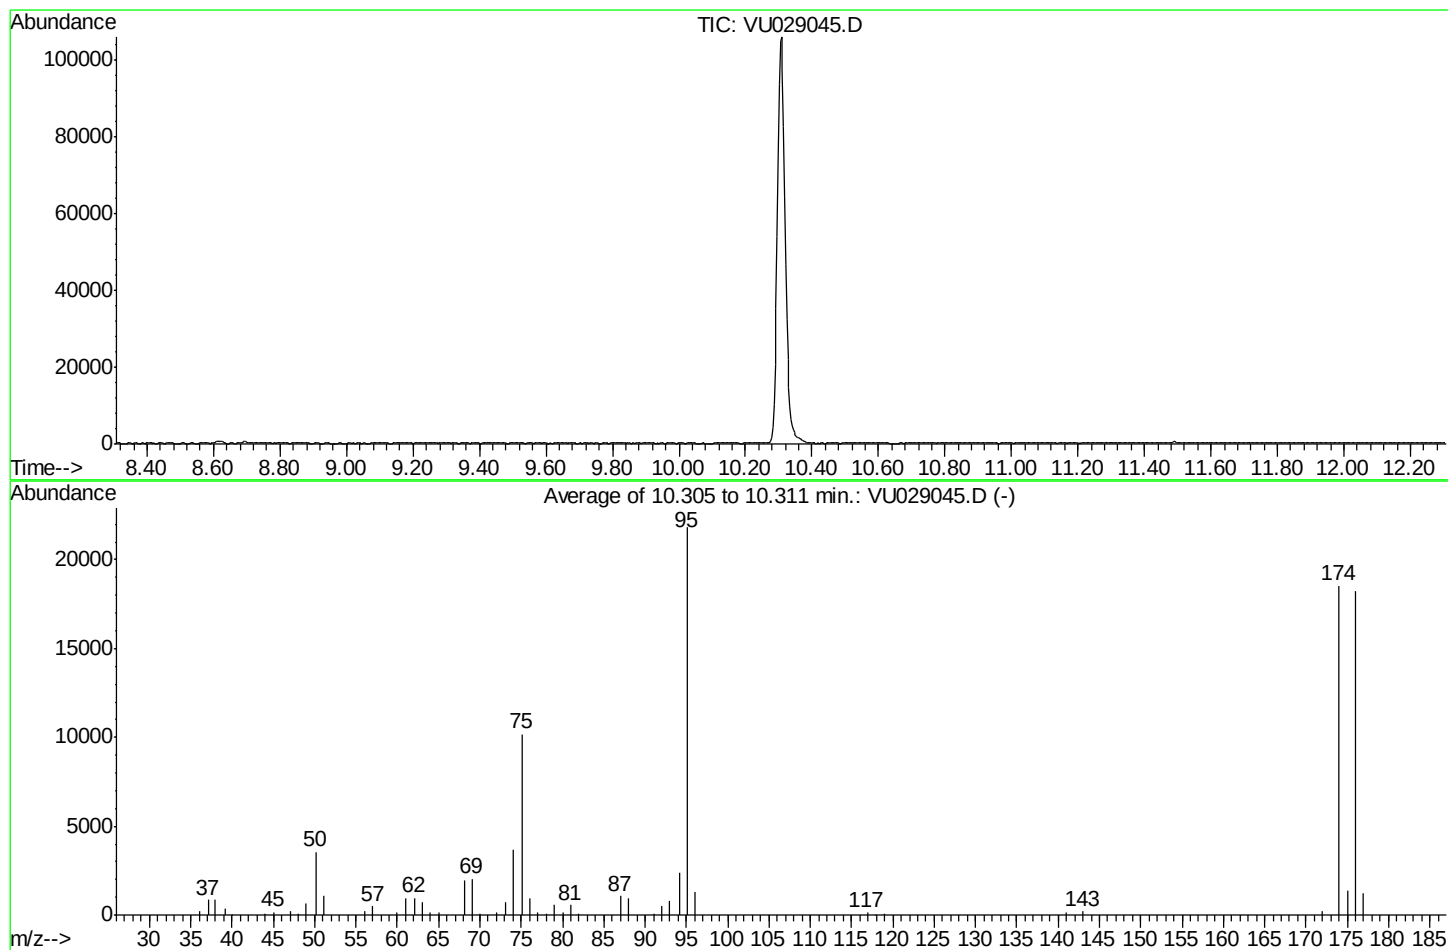

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	3568	PASS
75	95	30	80	46.7	10197	PASS
95	95	100	100	100.0	21824	PASS
96	95	5	9	5.9	1278	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.9	18520	PASS
175	174	5	9	7.3	1353	PASS
176	174	95	101	98.5	18248	PASS
177	176	5	9	6.8	1237	PASS

Scan 2829 (10.270 min): VU029045.D
BFB67

m/z	Abundance
40.00	115.0
44.00	229.0

Instrument :
MSVOA_U
ClientSampleId :
BFB67

m/z	Abundance
36.00	235.0
37.10	955.0
38.00	850.0
39.10	404.0
39.90	143.0
44.00	293.0
45.00	184.0
47.00	248.0
48.00	117.0
49.00	653.0
50.10	3711.0
51.10	1174.0
56.00	233.0
57.00	478.0
60.00	173.0
61.10	971.0
62.10	1003.0
63.10	716.0
64.00	106.0
65.10	140.0
68.10	1985.0
69.10	2157.0
70.00	130.0
72.00	118.0
73.10	736.0
74.10	3656.0
75.10	10617.0
76.00	968.0
77.00	127.0
79.00	557.0
80.00	126.0
81.00	505.0
81.90	124.0
87.00	1010.0
88.00	994.0
91.00	108.0
92.00	593.0
93.00	847.0
94.10	2525.0
95.10	22384.0
96.00	1380.0
117.00	144.0
117.90	102.0
119.00	110.0
140.90	151.0
143.10	212.0
172.00	215.0
174.00	18568.0
175.00	1335.0
176.00	18200.0
177.00	1271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB67

m/z	Abundance
36.00	223.0
37.10	857.0
38.00	873.0
39.10	410.0
40.00	134.0
44.00	304.0
45.00	175.0
47.10	233.0
48.00	105.0
49.00	670.0
50.10	3660.0
51.10	1106.0
56.00	254.0
57.00	499.0
60.00	158.0
61.00	964.0
62.10	993.0
63.10	734.0
64.00	134.0
65.10	168.0
68.10	2031.0
69.10	2090.0
70.00	114.0
72.00	144.0
73.00	749.0
74.10	3765.0
75.10	10470.0
76.00	957.0
77.00	128.0
78.00	110.0
79.00	584.0
80.00	140.0
80.90	571.0
81.90	106.0
87.00	1105.0
88.00	944.0
91.00	105.0
92.10	573.0
93.00	833.0
94.10	2421.0
95.10	22544.0
96.00	1283.0
117.00	138.0
118.90	110.0
140.90	150.0
143.10	215.0
172.00	212.0
174.00	19072.0
175.00	1374.0
176.00	18872.0
177.00	1271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB67

m/z	Abundance
36.00	164.0
37.10	718.0
38.00	798.0
39.10	371.0
40.00	147.0
44.00	271.0
45.00	174.0
47.10	219.0
49.00	669.0
50.10	3335.0
51.10	973.0
56.00	261.0
57.00	471.0
60.00	120.0
61.00	843.0
62.00	900.0
63.10	652.0
64.00	131.0
65.10	172.0
68.10	1885.0
69.00	1905.0
72.00	168.0
73.00	731.0
74.10	3523.0
75.10	9505.0
76.00	844.0
76.90	134.0
78.00	105.0
79.00	532.0
80.00	141.0
80.90	597.0
87.00	1104.0
88.00	899.0
92.00	460.0
93.00	777.0
94.10	2122.0
95.10	20544.0
96.10	1173.0
116.90	129.0
118.90	109.0
140.90	121.0
143.00	200.0
171.90	215.0
174.00	17920.0
175.00	1351.0
176.00	17672.0
177.00	1171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB67