

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU010720\
 Data File : VU036395.D
 Acq On : 07 Jan 2020 16:02
 Operator : JC/MD
 Sample : L1042-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFRA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.372	5	10	15	rBV2	12229	11949	0.50%	0.064%
2	1.613	78	85	99	rBV	291285	322989	13.39%	1.719%
3	1.932	176	184	199	rVB	253752	335325	13.90%	1.785%
4	2.594	376	390	404	rBV	482657	810972	33.62%	4.317%
5	2.793	442	452	462	rBV2	7417	16380	0.68%	0.087%
6	3.051	529	532	535	rBV2	962	723	0.03%	0.004%
7	3.073	535	539	540	rBV3	1558	1015	0.04%	0.005%
8	3.221	573	585	586	rBV3	13516	16729	0.69%	0.089%
9	3.391	635	638	639	rBV2	2047	1154	0.05%	0.006%
10	3.469	659	662	665	rVB3	1157	854	0.04%	0.005%
11	3.494	665	670	672	rBV4	764	767	0.03%	0.004%
12	3.568	690	693	697	rVB3	1004	766	0.03%	0.004%
13	3.613	703	707	715	rBV8	1339	1996	0.08%	0.011%
14	3.919	788	802	819	rVB3	19671	45934	1.90%	0.244%
15	4.044	837	841	845	rBV5	935	988	0.04%	0.005%
16	4.089	852	855	859	rVB3	1215	916	0.04%	0.005%
17	4.407	950	954	956	rVB4	1039	743	0.03%	0.004%
18	4.433	956	962	965	rBV4	1650	1461	0.06%	0.008%
19	4.459	965	970	973	rVB5	972	908	0.04%	0.005%
20	4.588	1004	1010	1013	rBV5	1311	1147	0.05%	0.006%
21	4.678	1021	1038	1059	rBV	208236	520868	21.59%	2.772%
22	5.108	1154	1172	1192	rBV	426154	970923	40.25%	5.168%
23	5.375	1252	1255	1261	rVB4	2362	2375	0.10%	0.013%
24	5.407	1261	1265	1267	rBV3	1987	1561	0.06%	0.008%
25	5.562	1311	1313	1317	rVB3	1177	721	0.03%	0.004%
26	5.584	1317	1320	1323	rBV3	1182	931	0.04%	0.005%
27	5.665	1339	1345	1349	rVB6	1100	1173	0.05%	0.006%
28	5.764	1353	1376	1400	rBV2	891067	2412270	100.00%	12.840%
29	6.144	1491	1494	1496	rBV4	1274	891	0.04%	0.005%
30	6.288	1522	1539	1560	rBV	726393	1391289	57.68%	7.405%
31	6.485	1597	1600	1602	rBV4	1376	946	0.04%	0.005%
32	6.581	1617	1630	1644	rVB6	19261	40039	1.66%	0.213%
33	6.729	1661	1676	1694	rBV	563162	1107431	45.91%	5.894%
34	6.925	1733	1737	1743	rBV6	1543	1353	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\U010720\
 Data File : VU036395.D
 Acq On : 07 Jan 2020 16:02
 Operator : JC/MD
 Sample : L1042-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFRA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
 Title : VOC Analysis

35	6.993	1756	1758	1761	rBV4	1273	847	0.04%	0.005%
36	7.214	1813	1827	1838	rBV7	8737	20958	0.87%	0.112%
37	7.288	1846	1850	1855	rVB4	955	779	0.03%	0.004%
38	7.337	1859	1865	1868	rBV4	1178	1328	0.06%	0.007%
39	7.530	1918	1925	1927	rBV4	889	974	0.04%	0.005%
40	7.600	1932	1947	1972	rBV	353180	646618	26.81%	3.442%
41	7.928	2034	2049	2069	rBV	1149892	2026665	84.01%	10.787%
42	8.211	2122	2137	2167	rBV	246112	450647	18.68%	2.399%
43	8.436	2202	2207	2212	rBV7	1372	1497	0.06%	0.008%
44	8.501	2218	2227	2239	rVB6	4232	8669	0.36%	0.046%
45	8.581	2241	2252	2265	rVB6	16391	29039	1.20%	0.155%
46	8.671	2265	2280	2323	rBV	482007	1239477	51.38%	6.597%
47	8.954	2365	2368	2371	rBV3	1103	751	0.03%	0.004%
48	9.179	2432	2438	2441	rBV5	979	1018	0.04%	0.005%
49	9.237	2454	2456	2459	rBV4	1140	804	0.03%	0.004%
50	9.279	2464	2469	2473	rBV5	953	894	0.04%	0.005%
51	9.349	2486	2491	2493	rBV3	864	723	0.03%	0.004%
52	9.366	2493	2496	2501	rVV6	1009	967	0.04%	0.005%
53	9.446	2507	2521	2556	rVB	1013651	1802698	74.73%	9.595%
54	9.591	2562	2566	2574	rBV6	2330	3382	0.14%	0.018%
55	9.716	2592	2605	2614	rVV2	15153	25635	1.06%	0.136%
56	10.028	2699	2702	2706	rBV4	1464	795	0.03%	0.004%
57	10.128	2723	2733	2738	rBV5	7592	12646	0.52%	0.067%
58	10.166	2743	2745	2747	rVV3	1741	919	0.04%	0.005%
59	10.301	2785	2787	2792	rVB3	1058	840	0.03%	0.004%
60	10.375	2807	2810	2812	rBV3	1352	1030	0.04%	0.005%
61	10.481	2837	2843	2844	rBV3	1190	1132	0.05%	0.006%
62	10.738	2919	2923	2924	rBV3	1032	716	0.03%	0.004%
63	10.783	2924	2937	2961	rVB	732023	1254440	52.00%	6.677%
64	10.915	2972	2978	2990	rVB7	6860	12411	0.51%	0.066%
65	11.105	3033	3037	3044	rVB8	2308	2879	0.12%	0.015%
66	11.195	3061	3065	3066	rVV3	1141	814	0.03%	0.004%
67	11.494	3153	3158	3163	rVV4	1833	2226	0.09%	0.012%
68	11.594	3185	3189	3191	rBV2	1672	1229	0.05%	0.007%
69	11.652	3204	3207	3212	rVB5	1283	1047	0.04%	0.006%
70	11.767	3238	3243	3245	rBV3	1911	1673	0.07%	0.009%
71	11.835	3251	3264	3283	rVB	852152	1498731	62.13%	7.977%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU010720\
 Data File : VU036395.D
 Acq On : 07 Jan 2020 16:02
 Operator : JC/MD
 Sample : L1042-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFRA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
 Title : VOC Analysis

72	11.906	3283	3286	3288	rBV2	1739	1191	0.05%	0.006%
73	12.041	3325	3328	3331	rBV3	937	759	0.03%	0.004%
74	12.086	3333	3342	3349	rBV4	4878	7854	0.33%	0.042%
75	12.163	3364	3366	3369	rBV3	1167	773	0.03%	0.004%
76	12.217	3370	3383	3401	rVB	917367	1566535	64.94%	8.338%
77	12.324	3414	3416	3421	rVB3	1292	862	0.04%	0.005%
78	12.349	3421	3424	3425	rBV2	1165	773	0.03%	0.004%
79	12.401	3434	3440	3446	rVB6	1809	2376	0.10%	0.013%
80	12.484	3462	3466	3467	rBV3	2233	1551	0.06%	0.008%
81	12.594	3491	3500	3508	rBV6	6802	9839	0.41%	0.052%
82	12.896	3589	3594	3602	rBV5	3976	5007	0.21%	0.027%
83	12.996	3614	3625	3633	rBV3	11209	18097	0.75%	0.096%
84	13.047	3633	3641	3655	rVB2	16685	26018	1.08%	0.138%
85	13.124	3662	3665	3669	rBV5	1382	887	0.04%	0.005%
86	13.156	3670	3675	3677	rBV5	2167	1910	0.08%	0.010%
87	13.182	3680	3683	3685	rBV3	1242	786	0.03%	0.004%
88	13.237	3694	3700	3706	rBV6	2722	3342	0.14%	0.018%
89	13.269	3706	3710	3713	rBV5	1325	895	0.04%	0.005%
90	13.314	3721	3724	3732	rVB8	3617	4243	0.18%	0.023%
91	13.475	3765	3774	3781	rBV5	12092	19084	0.79%	0.102%
92	13.661	3829	3832	3834	rBV3	1359	876	0.04%	0.005%
93	13.812	3871	3879	3883	rBV9	1736	2876	0.12%	0.015%
94	13.854	3886	3892	3894	rBV5	5960	5983	0.25%	0.032%
95	14.108	3961	3971	3977	rBV2	7417	11797	0.49%	0.063%
96	14.346	4041	4045	4049	rBV7	2362	2349	0.10%	0.013%
97	14.725	4160	4163	4166	rBV3	1990	1204	0.05%	0.006%
98	14.790	4180	4183	4185	rBV3	1833	1110	0.05%	0.006%
99	15.237	4319	4322	4326	rBV6	2472	1778	0.07%	0.009%
100	15.414	4372	4377	4379	rBV4	2365	2462	0.10%	0.013%


Sum of corrected areas: 18787602

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU010720\
Data File : VU036395.D
Acq On : 07 Jan 2020 16:02
Operator : JC/MD
Sample : L1042-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BFRA0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

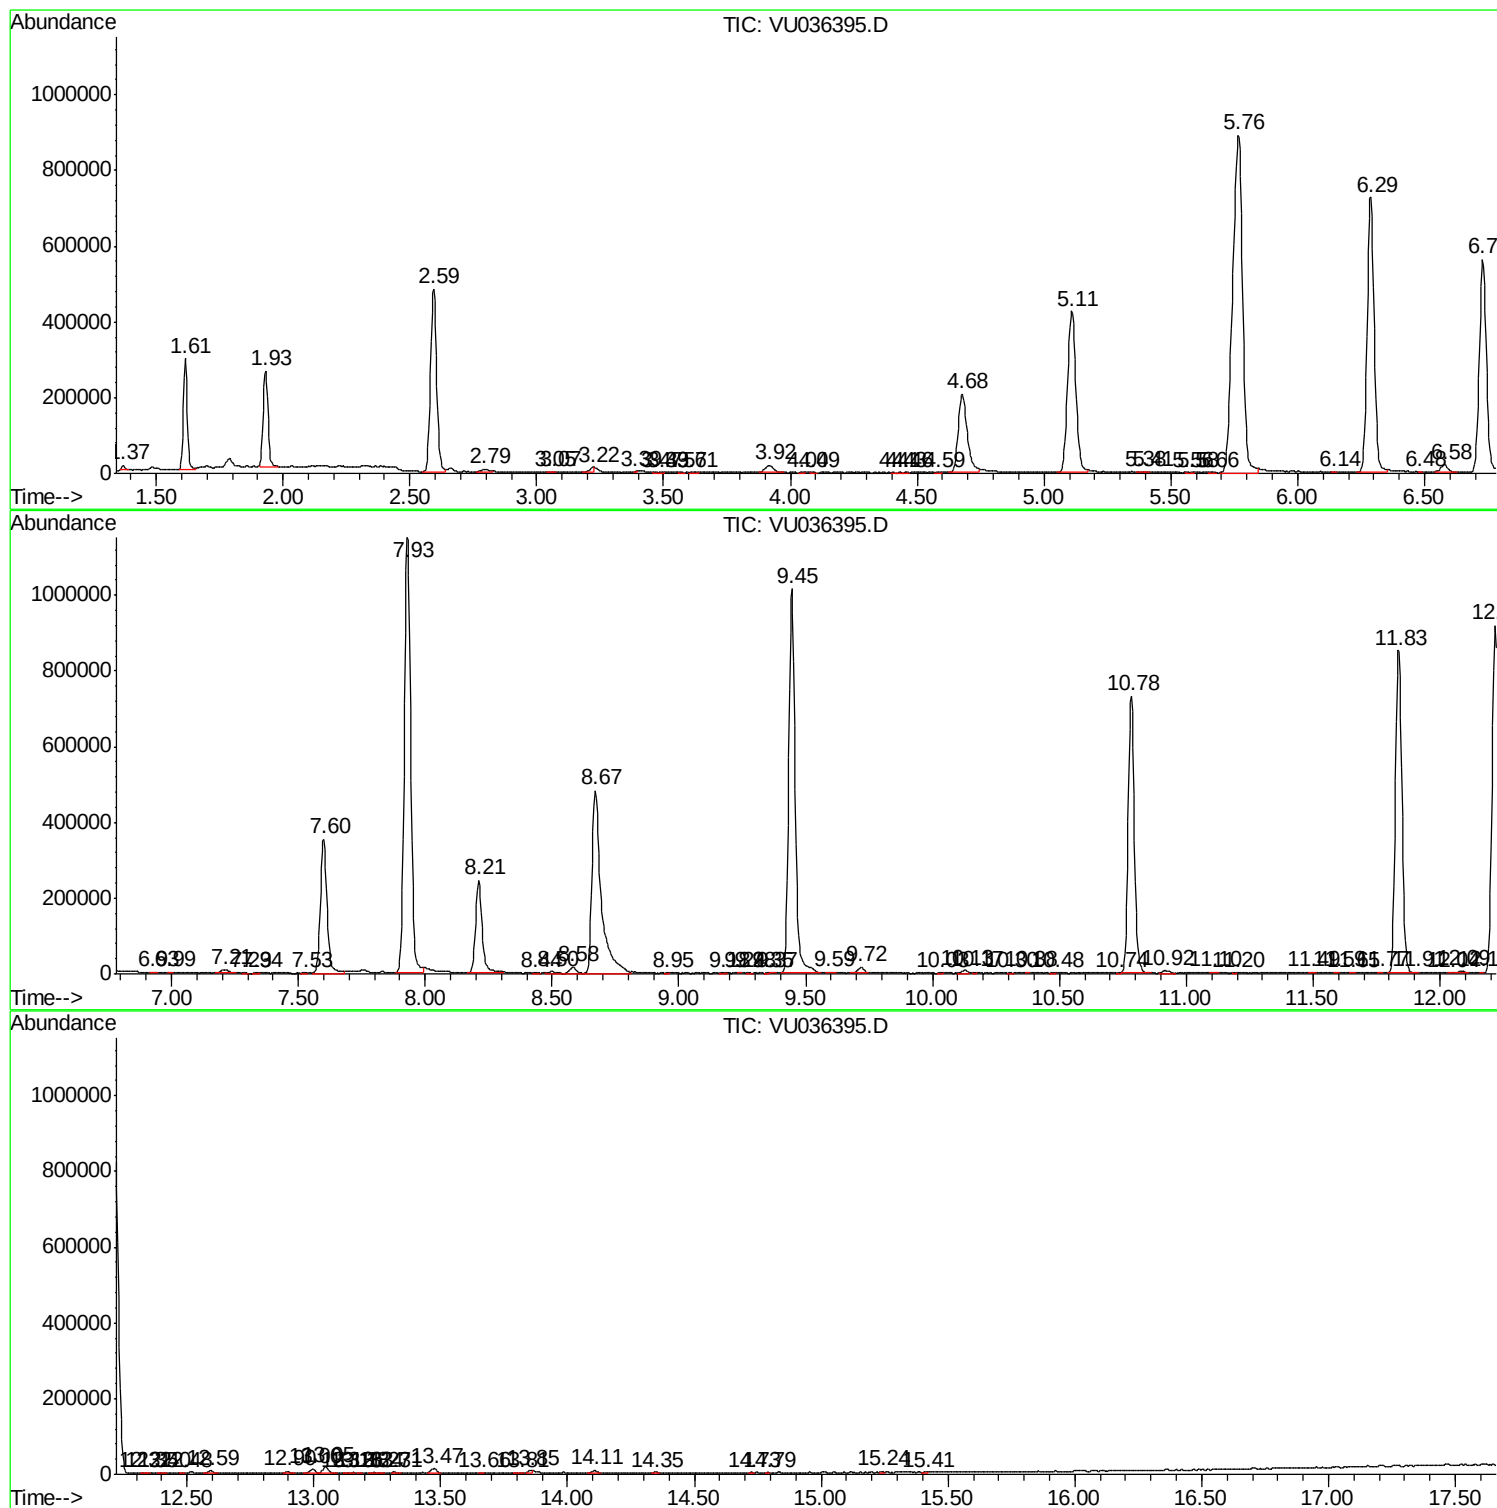

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU010720\
Data File : VU036395.D
Acq On : 07 Jan 2020 16:02
Operator : JC/MD
Sample : L1042-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFRA0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU010720\
Data File : VU036395.D
Acq On : 07 Jan 2020 16:02
Operator : JC/MD
Sample : L1042-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFRA0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc