


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010720\
 Data File : VU036392.D
 Acq On : 07 Jan 2020 11:48
 Operator : JC/MD
 Sample : BFB34
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB34

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
 Title : VOC Analysis
 Last Update : Wed Jan 08 03:56:17 2020

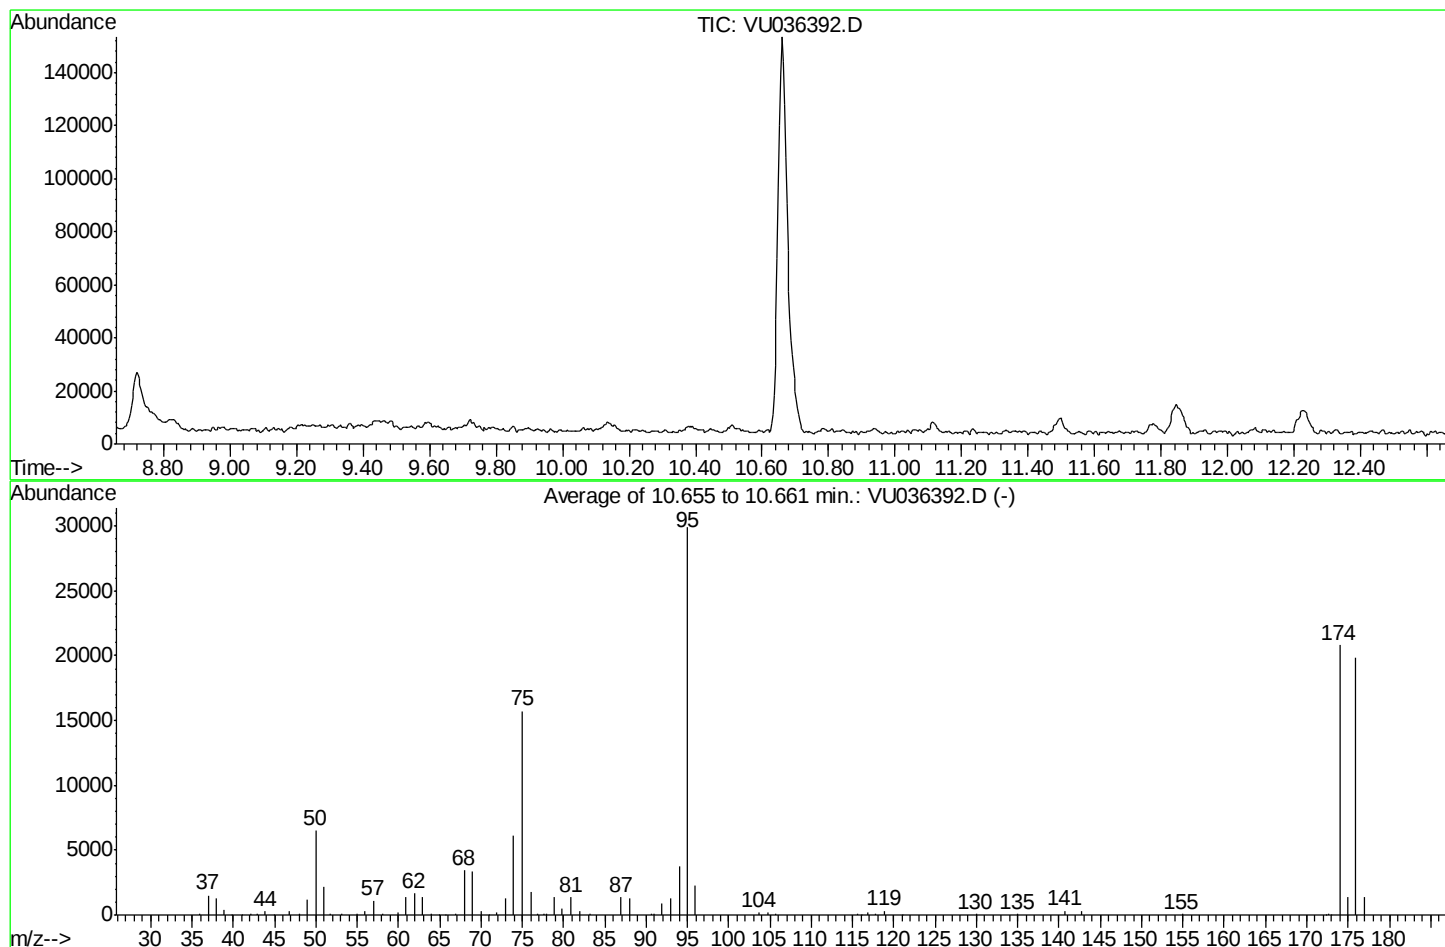

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	6511	PASS
75	95	30	80	52.6	15734	PASS
95	95	100	100	100.0	29898	PASS
96	95	5	9	7.7	2291	PASS
173	174	0.00	2	0.5	98	PASS
174	95	50	120	69.6	20810	PASS
175	174	5	9	6.7	1398	PASS
176	174	95	101	95.2	19808	PASS
177	176	5	9	7.0	1383	PASS

m/z	Abundance
35.90	907.0
37.00	1386.0
38.00	1435.0
38.90	556.0
39.80	630.0
41.00	365.0
42.10	121.0
43.00	325.0
43.90	797.0
44.90	181.0
46.80	293.0
48.90	1077.0
49.90	6127.0
51.00	1955.0
51.80	116.0
53.10	154.0
54.80	243.0
55.90	548.0
57.00	992.0
58.10	171.0
59.90	197.0
60.90	1252.0
61.90	1631.0
62.90	1348.0
63.90	156.0
64.90	111.0
65.70	134.0
66.90	112.0
67.90	3321.0
69.00	3196.0
70.00	327.0
71.90	176.0
73.00	1383.0
73.90	5733.0
75.00	14888.0
76.00	1532.0
76.80	119.0
77.90	173.0
78.90	1270.0
79.80	420.0
80.90	1402.0
81.90	223.0
83.10	169.0
86.90	1278.0
88.00	1295.0
90.60	134.0
91.00	114.0
91.90	861.0
93.00	1213.0
94.00	3499.0
95.00	28344.0
95.90	2342.0
103.70	166.0
104.70	150.0
105.70	142.0
115.70	103.0
116.80	196.0
117.80	135.0
118.90	275.0
121.00	102.0
140.80	322.0
142.80	222.0
172.70	173.0
174.00	19784.0
175.00	1312.0
175.90	18104.0
176.90	1470.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
35.90	918.0
37.00	1554.0
37.90	1765.0
38.90	647.0
39.80	702.0
41.00	345.0
42.10	128.0
42.90	402.0
43.90	760.0
45.00	178.0
46.80	347.0
47.90	174.0
48.90	1187.0
50.00	6742.0
51.00	2297.0
51.80	102.0
53.10	134.0
55.00	329.0
56.00	555.0
57.00	1178.0
60.00	251.0
60.80	1396.0
62.00	1700.0
62.90	1434.0
63.90	162.0
67.00	104.0
68.00	3515.0
68.90	3333.0
69.90	339.0
71.00	140.0
71.80	233.0
73.00	1498.0
73.90	6361.0
75.00	15804.0
76.00	1774.0
76.80	146.0
77.60	152.0
78.00	133.0
78.90	1452.0
79.80	506.0
80.90	1508.0
81.90	279.0
83.20	102.0
86.90	1376.0
88.00	1339.0
90.60	107.0
91.00	150.0
91.80	864.0
93.00	1313.0
94.00	3833.0
95.00	30712.0
96.00	2346.0
103.70	186.0
104.70	173.0
105.70	159.0
115.70	104.0
116.80	171.0
117.80	149.0
118.90	331.0
130.00	105.0
135.00	100.0
140.80	334.0
142.80	282.0
154.90	147.0
172.70	123.0
174.00	21384.0
174.90	1404.0
176.00	20264.0
176.90	1410.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
35.90	1032.0
37.00	1568.0
37.90	1983.0
38.90	676.0
39.80	693.0
41.00	310.0
41.80	153.0
42.90	395.0
43.90	925.0
45.00	139.0
46.80	370.0
48.00	217.0
48.90	1179.0
50.00	6666.0
51.00	2316.0
53.00	143.0
55.00	439.0
56.00	602.0
57.00	1177.0
60.00	258.0
60.90	1499.0
62.00	1584.0
62.90	1450.0
63.90	130.0
67.00	133.0
68.00	3465.0
68.90	3598.0
69.90	353.0
71.00	228.0
71.80	322.0
73.00	1549.0
74.00	6141.0
75.00	16512.0
76.00	1902.0
76.80	150.0
77.60	167.0
78.00	148.0
78.90	1390.0
79.80	467.0
80.90	1539.0
81.90	364.0
87.00	1355.0
87.90	1196.0
91.00	110.0
91.90	877.0
92.90	1293.0
94.00	3826.0
95.00	30640.0
96.00	2185.0
103.70	159.0
104.70	148.0
105.80	143.0
115.60	110.0
116.10	110.0
116.80	165.0
117.80	171.0
118.90	322.0
129.90	161.0
135.00	103.0
140.70	258.0
142.70	331.0
154.90	139.0
172.30	103.0
173.00	116.0
174.00	21264.0
174.90	1480.0
176.00	21056.0
176.90	1270.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

Scan 2886 (10.619 min): VU036392.D
BFB34

m/z	Abundance
35.10	148.0
35.90	844.0
37.80	405.0
38.90	269.0
39.80	655.0
41.00	288.0
41.90	277.0
42.90	226.0
44.00	537.0
44.90	116.0
54.80	203.0
55.20	196.0
55.80	232.0
69.20	171.0
71.00	107.0
73.10	149.0
81.00	125.0
82.30	108.0
82.90	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34