


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU010721\
 Data File : VU041858.D
 Acq On : 06 Jan 2021 12:27
 Operator : SY/MD
 Sample : BFB37
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB37

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR122820WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Jan 07 13:48:48 2021

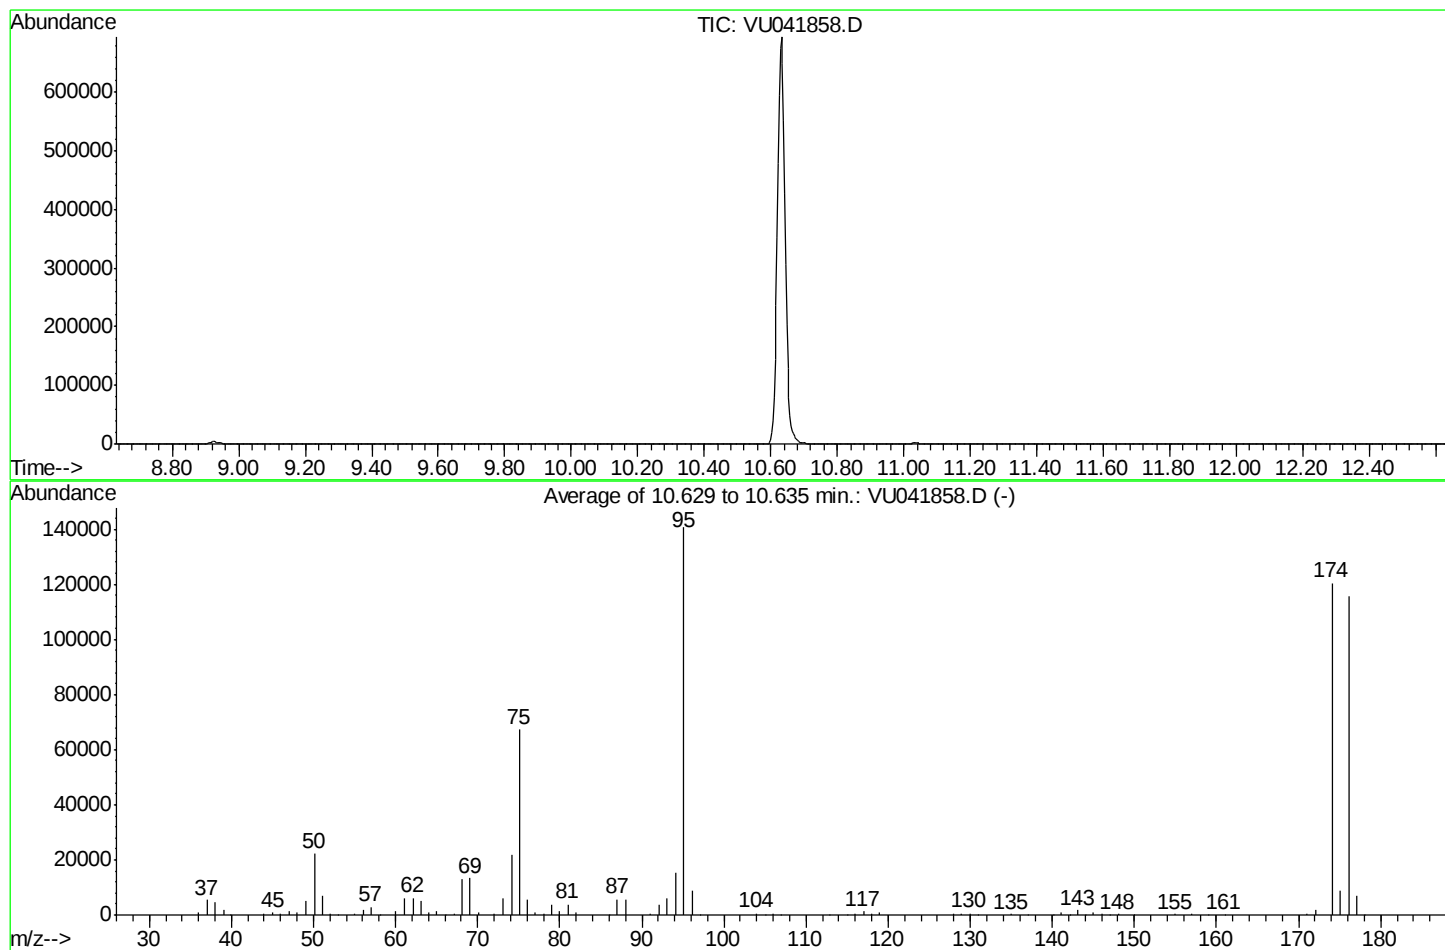

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	22162	PASS
75	95	30	80	47.8	67253	PASS
95	95	100	100	100.0	140650	PASS
96	95	5	9	6.2	8788	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.5	120293	PASS
175	174	5	9	7.5	8991	PASS
176	174	95	101	96.2	115685	PASS
177	176	5	9	6.1	7077	PASS