




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010722\
Data File : VU046697.D
Acq On : 07 Jan 2022 16:29
Operator : SY/MD
Sample : N1074-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGLK3

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/11/2022
Supervised By :Mahesh Dadoda 01/11/2022

Quant Time: Jan 07 23:27:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 07 23:26:33 2022
Response via : Initial Calibration

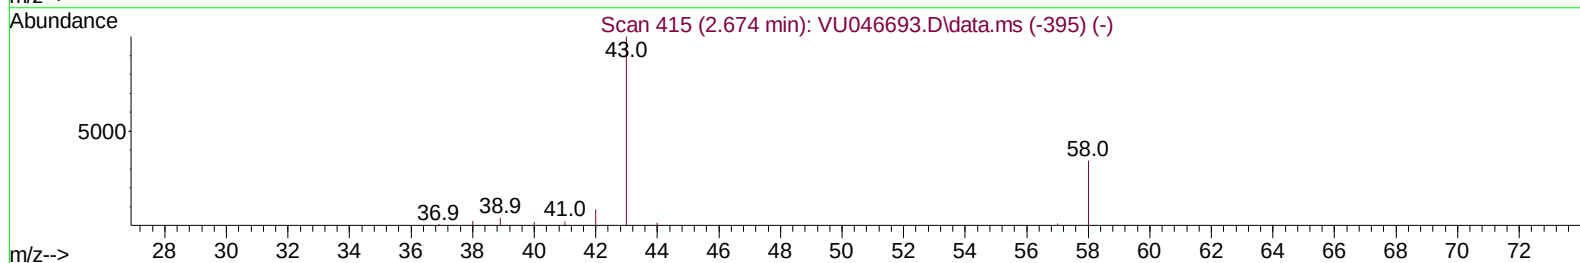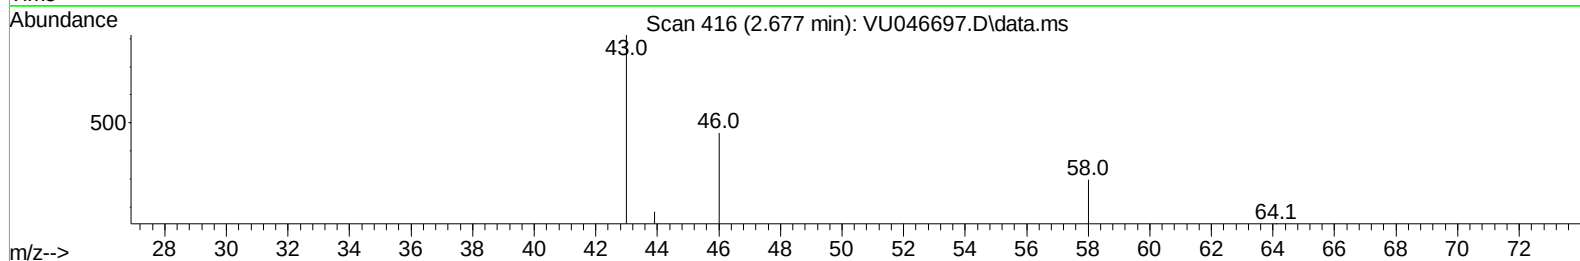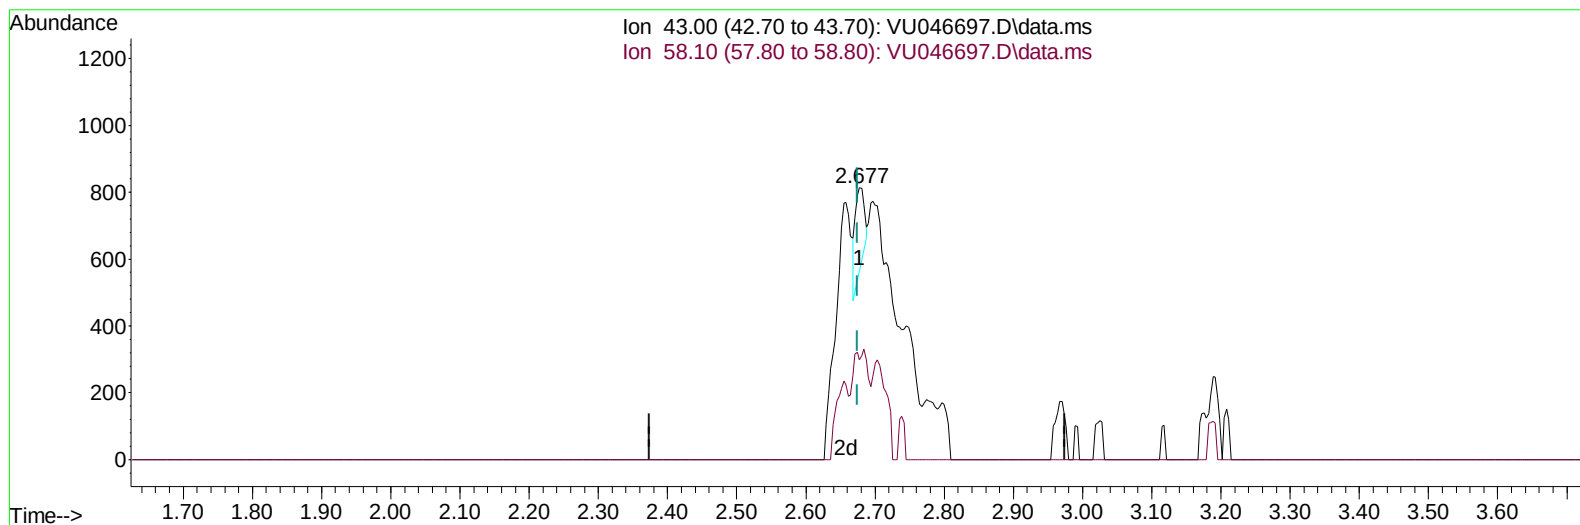

TIC: VU046697.D\data.ms

(13) Acetone (T)

2.677min (+ 0.003) 0.20 ug/L

response 229

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	35.50	37.99
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010722\
Data File : VU046697.D
Acq On : 07 Jan 2022 16:29
Operator : SY/MD
Sample : N1074-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGLK3

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/11/2022
Supervised By :Mahesh Dadoda 01/11/2022

Quant Time: Jan 07 23:27:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 07 23:26:33 2022
Response via : Initial Calibration

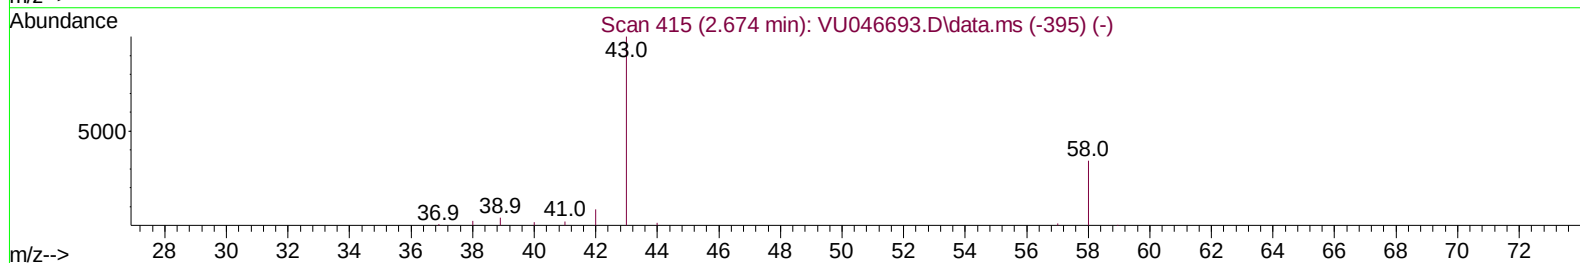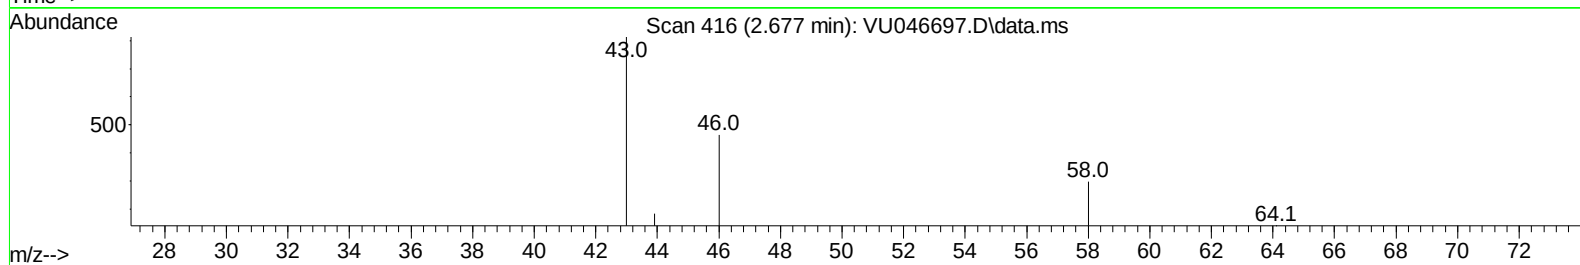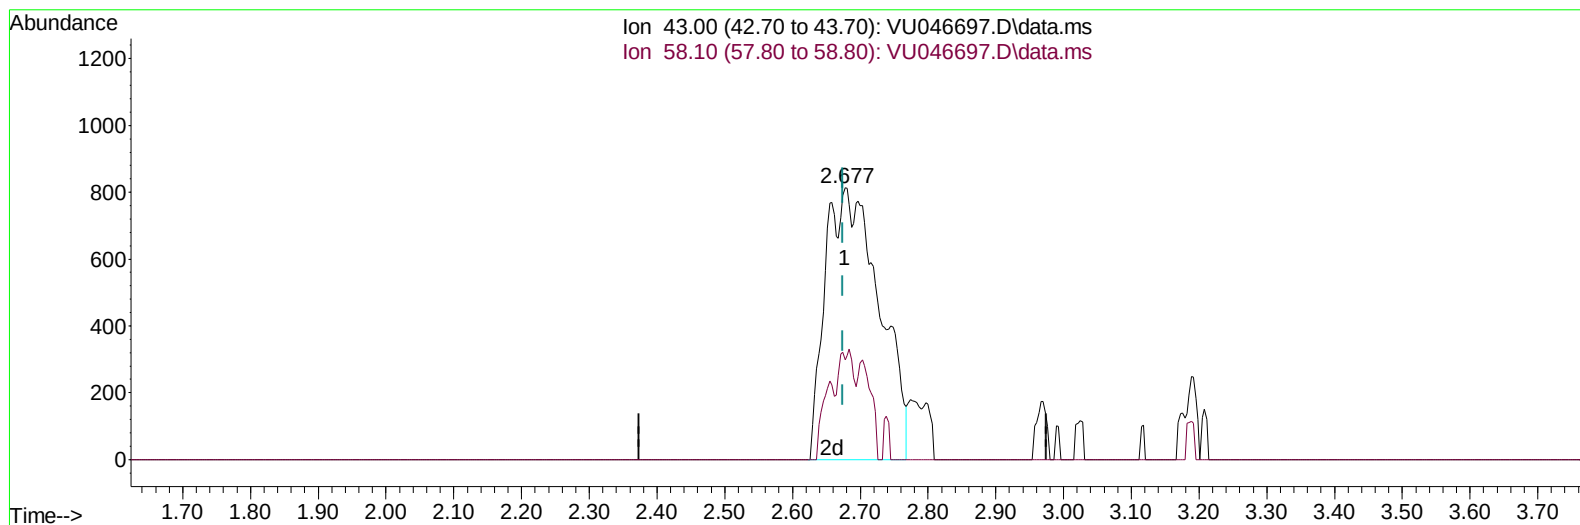

TIC: VU046697.D\data.ms

(13) Acetone (T)

2.677min (+ 0.003) 3.96 ug/L m

response 4495

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	35.50	1.94
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010722\
 Data File : VU046697.D
 Acq On : 07 Jan 2022 16:29
 Operator : SY/MD
 Sample : N1074-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGLK3

Manual IntegrationsAPPROVED

Quant Time: Jan 07 23:27:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 07 23:26:33 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 01/11/2022
 Supervised By :Mahesh Dadoda 01/11/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	186715	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	184606	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	93148	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	49651	30.473	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	60.940%	
7) Chloroethane-d5	1.919	69	41827	34.557	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	69.120%#	
11) 1,1-Dichloroethene-d2	2.571	63	70009	25.263	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	50.520%#	
21) 2-Butanone-d5	4.652	46	107884	90.470	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	90.470%	
24) Chloroform-d	5.066	84	103598	36.068	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	72.140%	
26) 1,2-Dichloroethane-d4	5.706	65	69147	37.959	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	75.920%	
32) Benzene-d6	5.732	84	203829	35.380	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	70.760%	
36) 1,2-Dichloropropane-d6	6.693	67	64682	36.797	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	73.600%	
41) Toluene-d8	7.902	98	179421	34.837	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	69.680%#	
43) trans-1,3-Dichloroprop...	8.182	79	31100	36.724	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	73.440%	
47) 2-Hexanone-d5	8.639	63	84444	90.426	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	90.430%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	108252	39.763	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	79.520%	
66) 1,2-Dichlorobenzene-d4	12.195	152	79340	41.163	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	82.320%	
Target Compounds						
13) Acetone	2.677	43	4495m	3.961	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010722\
Data File : VU046697.D
Acq On : 07 Jan 2022 16:29
Operator : SY/MD
Sample : N1074-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGLK3

Manual IntegrationsAPPROVED

Quant Time: Jan 07 23:27:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 07 23:26:33 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/11/2022
Supervised By :Mahesh Dadoda 01/11/2022

