


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010722\
 Data File : VU046692.D
 Acq On : 07 Jan 2022 10:11
 Operator : SY/MD
 Sample : BFB039
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB039

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis
 Last Update : Wed Jan 12 04:49:52 2022

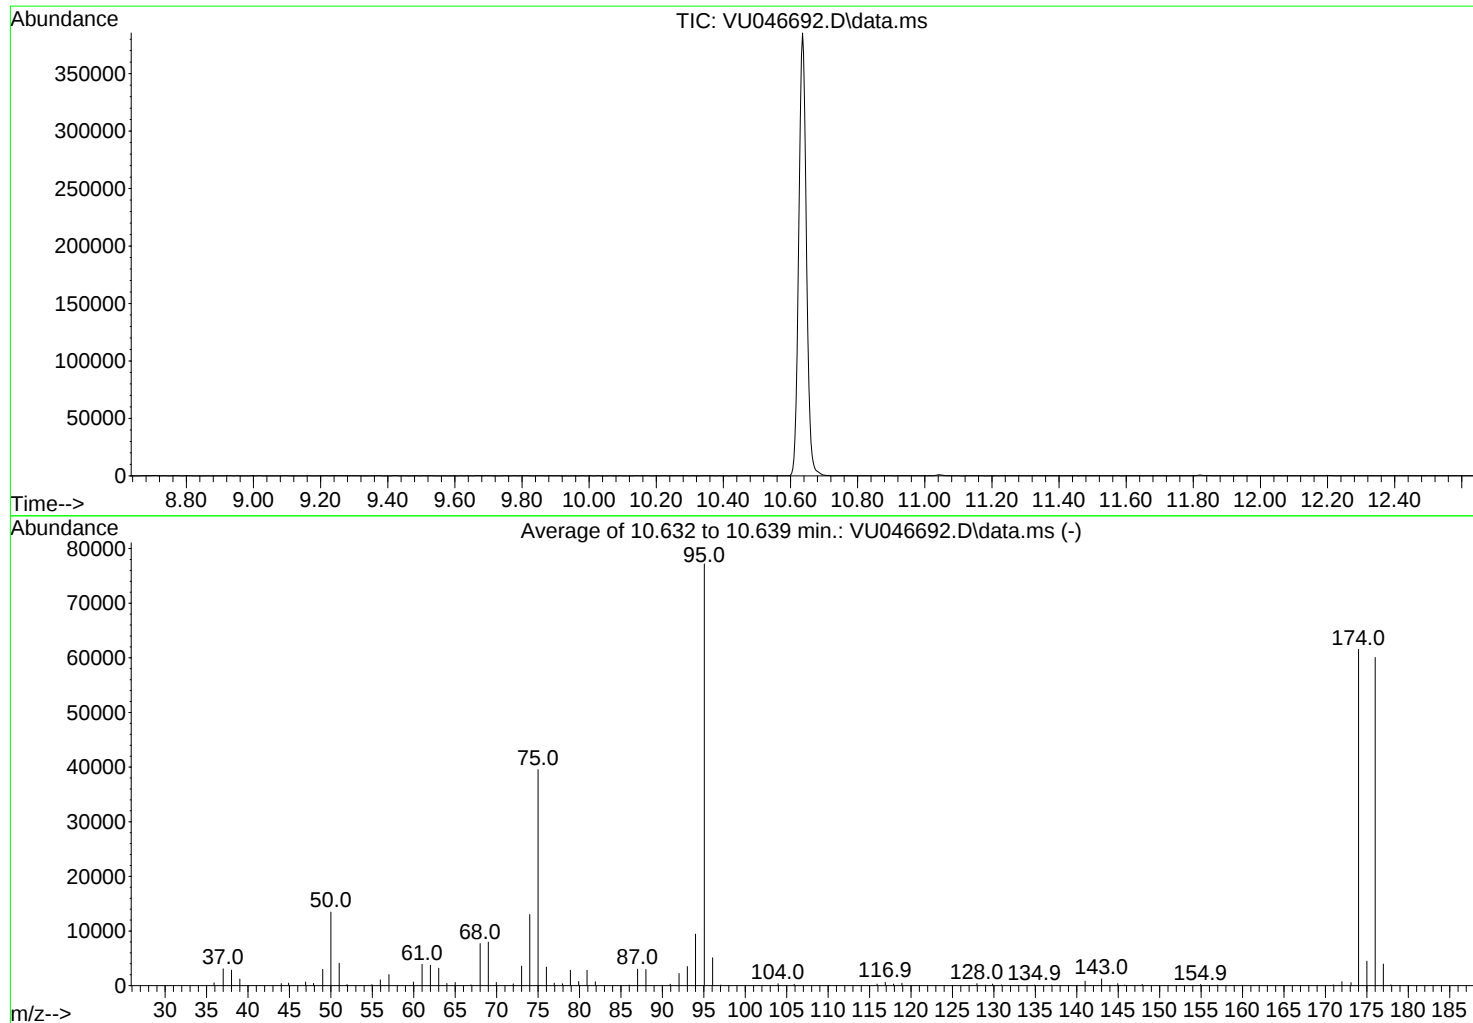

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	13486	PASS
75	95	30	80	51.2	39541	PASS
95	95	100	100	100.0	77203	PASS
96	95	5	9	6.6	5107	PASS
173	174	0.00	2	0.9	565	PASS
174	95	50	120	79.7	61544	PASS
175	174	5	9	7.3	4479	PASS
176	174	95	101	97.6	60067	PASS
177	176	5	9	6.6	3948	PASS

m/z	Abundance
44.00	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	552.0
37.00	3003.0
38.00	2971.0
39.00	1223.0
44.00	427.0
44.90	437.0
47.00	635.0
47.90	424.0
49.00	3025.0
50.00	13442.0
51.00	3963.0
52.00	220.0
54.90	211.0
56.00	1095.0
57.00	1995.0
60.00	674.0
61.00	3806.0
62.00	3633.0
63.00	3142.0
64.00	471.0
65.00	588.0
66.90	117.0
68.00	7549.0
69.00	7917.0
70.00	613.0
72.00	315.0
73.00	3312.0
74.00	12821.0
75.00	38872.0
76.00	3400.0
76.90	470.0
78.00	368.0
78.90	2795.0
79.90	767.0
80.90	2873.0
81.90	741.0
86.00	111.0
87.00	2965.0
88.00	2984.0
90.90	271.0
92.00	2150.0
93.00	3643.0
94.00	9416.0
95.10	75912.0
96.10	5060.0
97.10	133.0
104.00	313.0
104.90	112.0
105.90	228.0
114.80	109.0
115.90	260.0
116.90	583.0
117.90	311.0
118.90	420.0
127.90	355.0
129.00	122.0
129.80	277.0
130.90	123.0
134.90	107.0
137.00	114.0
141.00	784.0
143.00	1256.0
144.90	416.0
145.80	109.0
147.90	200.0
154.90	189.0
157.00	105.0
170.90	157.0
172.00	668.0
173.10	579.0
174.00	59040.0
175.00	4342.0
176.00	57568.0
177.00	3957.0
177.90	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	562.0
37.00	3202.0
38.00	2922.0
39.00	1246.0
44.00	483.0
44.90	494.0
47.00	667.0
47.90	421.0
49.00	3110.0
50.00	14056.0
51.00	4262.0
52.00	231.0
54.90	226.0
55.90	1080.0
57.00	2113.0
60.00	689.0
61.00	4020.0
62.00	3847.0
63.00	3339.0
64.00	414.0
65.00	605.0
66.90	150.0
68.00	7950.0
69.00	8229.0
70.00	606.0
72.00	343.0
73.00	3729.0
74.00	13488.0
75.00	40864.0
76.00	3536.0
76.90	481.0
78.00	357.0
78.90	2884.0
79.90	787.0
80.90	2883.0
81.90	751.0
86.00	114.0
87.00	3118.0
88.00	3052.0
91.00	278.0
92.00	2285.0
93.00	3570.0
94.00	9777.0
95.10	79752.0
96.00	5242.0
97.00	132.0
104.00	370.0
104.90	107.0
105.90	255.0
115.90	279.0
116.90	623.0
117.90	315.0
118.90	456.0
127.90	394.0
129.00	127.0
129.90	280.0
130.90	157.0
134.90	110.0
137.00	136.0
141.00	857.0
143.00	1293.0
145.00	388.0
145.80	140.0
147.90	195.0
154.90	197.0
156.90	121.0
170.90	143.0
172.00	738.0
173.10	570.0
174.00	63552.0
175.00	4641.0
176.00	62304.0
177.00	4090.0
177.90	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	508.0
37.00	3026.0
38.00	2629.0
39.00	1180.0
44.00	512.0
44.90	523.0
46.90	713.0
47.90	400.0
49.00	2802.0
50.00	12961.0
51.00	4087.0
51.90	200.0
55.00	224.0
55.90	995.0
57.00	1946.0
59.90	654.0
61.00	3831.0
62.00	3710.0
63.00	3105.0
64.00	344.0
65.00	573.0
66.90	164.0
68.00	7641.0
69.00	7756.0
69.90	510.0
72.00	349.0
73.00	3638.0
74.00	12669.0
75.00	38888.0
76.00	3286.0
77.00	461.0
77.90	303.0
78.90	2730.0
79.90	771.0
80.90	2643.0
81.90	662.0
86.00	106.0
87.00	2954.0
88.00	2869.0
91.00	262.0
92.00	2278.0
93.00	3207.0
94.00	9145.0
95.00	75944.0
96.00	5019.0
97.00	138.0
103.90	352.0
105.90	286.0
115.90	323.0
116.90	607.0
117.90	293.0
118.90	455.0
128.00	390.0
129.00	119.0
129.90	282.0
130.90	160.0
134.90	118.0
136.90	149.0
141.00	848.0
143.00	1175.0
145.00	342.0
145.80	148.0
147.90	183.0
155.00	191.0
156.90	130.0
158.90	119.0
171.00	114.0
172.00	768.0
173.10	545.0
174.00	62040.0
175.00	4455.0
176.00	60328.0
177.00	3796.0
177.90	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039