

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010820\
 Data File : VU036407.D
 Acq On : 08 Jan 2020 15:05
 Operator : JC/MD
 Sample : L1042-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFRA4

Manual Integrations
 APPROVED

apatel
 1/9/2020 3:45:14 PM

Quant Time: Jan 09 03:53:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 09 03:50:28 2020
 Response via : Initial Calibration

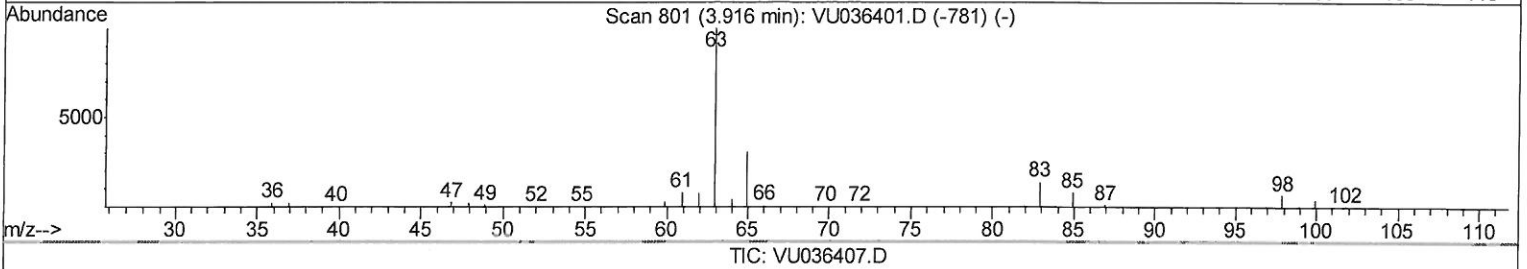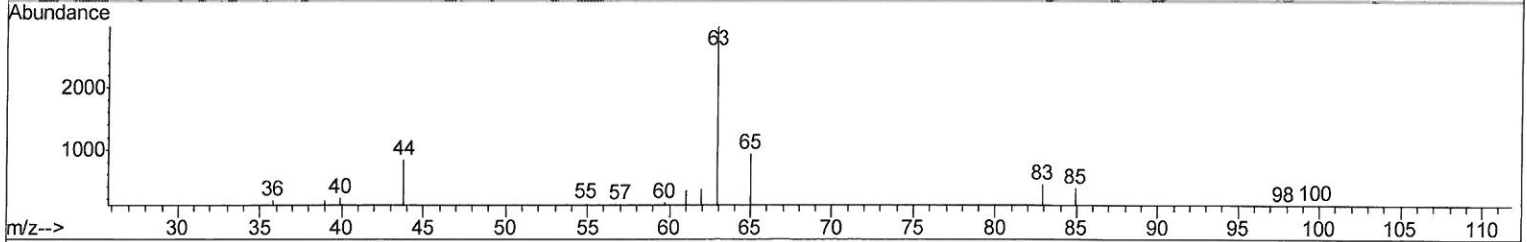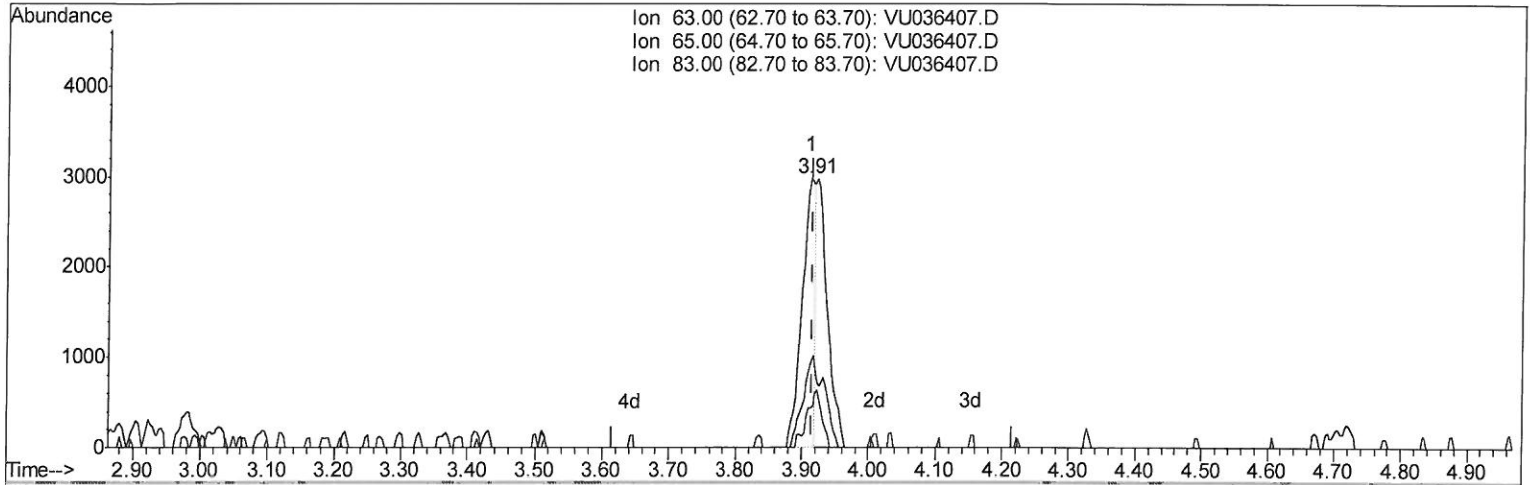

(19) 1,1-Dichloroethane (T)

3.912min (-0.003) 0.71ug/L

response 4118

Ion	Exp%	Act%
63.00	100	100
65.00	28.60	31.16
83.00	13.70	14.73
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010820\
Data File : VU036407.D
Acq On : 08 Jan 2020 15:05
Operator : JC/MD
Sample : L1042-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BFRA4

Manual Integrations
APPROVED

apatel
1/9/2020 3:45:14 PM

Quant Time: Jan 09 03:53:11 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 09 03:50:28 2020
Response via : Initial Calibration

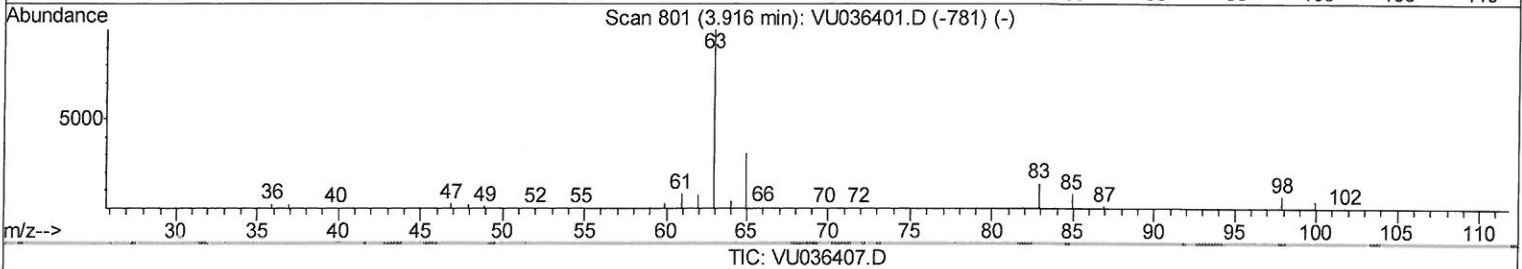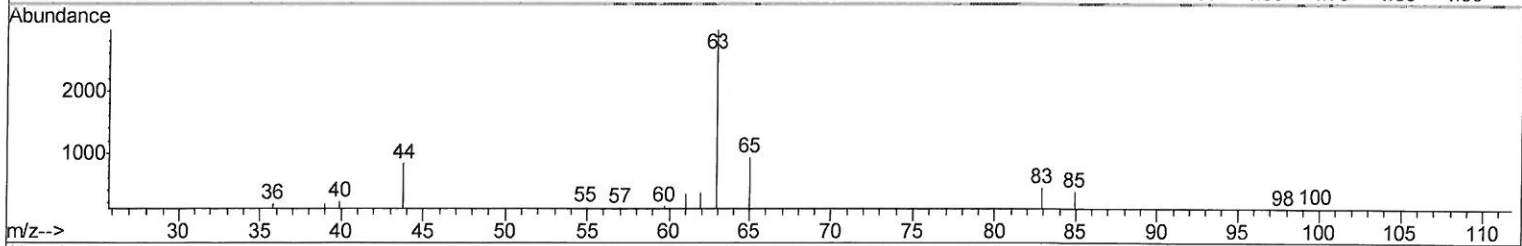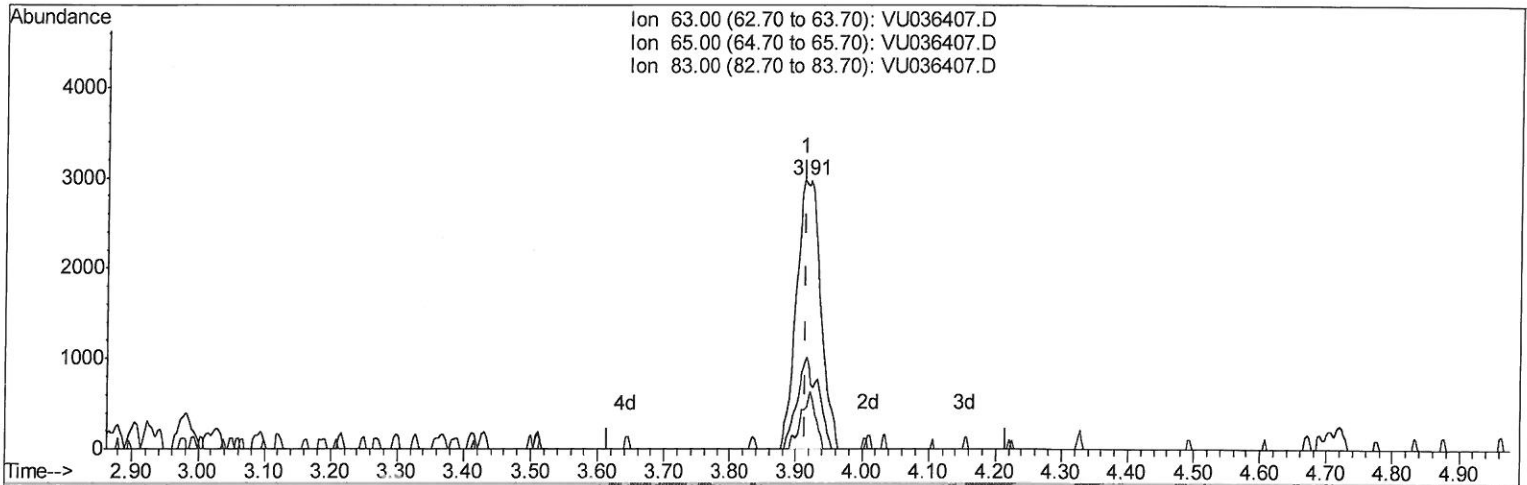

(19) 1,1-Dichloroethane (T)

3.912min (-0.003) 1.29ug/L m

response 7498

Ion	Exp%	Act%
63.00	100	100
65.00	28.60	31.16
83.00	13.70	14.73
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010820\
Quantitation Report (LSC Reviewed)

Data File : VU036407.D
Acq On : 08 Jan 2020 15:05
Operator : JC/MD
Sample : L1042-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFRA4

Manual Integrations
APPROVED

apatel
1/9/2020 3:45:14 PM

Quant Time: Jan 09 11:50:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 09 03:50:28 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	464900	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	430954	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	173661	50.00	ug/L	0.00

System Monitoring Compounds						
4) Vinyl Chloride-d3	1.61	65	142194	39.25	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.50%
7) Chloroethane-d5	1.93	69	130062	42.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.12%
11) 1,1-Dichloroethene-d2	2.59	63	225172	36.49	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.98%
21) 2-Butanone-d5	4.68	46	271574	100.67	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.67%
24) Chloroform-d	5.11	84	312201	49.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.76%
26) 1,2-Dichloroethane-d4	5.75	65	217324	51.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.68%
32) Benzene-d6	5.77	84	629292	52.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.90%
36) 1,2-Dichloropropane-d6	6.73	67	207966	51.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.38%
41) Toluene-d8	7.93	98	584355	50.74	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.48%
43) trans-1,3-Dichloropropene-	8.21	79	105471	48.31	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.62%
47) 2-Hexanone-d5	8.67	63	209486	100.94	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.94%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	299793	49.12	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.24%
64) 1,2-Dichlorobenzene-d4	12.22	152	183371	50.34	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.68%

Target Compounds					Qvalue
13) Acetone	2.66	43	8183	2.925 ug/L	89
19) 1,1-Dichloroethane	3.91	63	7498m	1.288 ug/L	91
34) Trichloroethene	6.58	95	6370	1.952 ug/L	95
46) Tetrachloroethene	8.58	164	9286	3.954 ug/L	92

01/09/20 84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU036407.D
Acq On : 08 Jan 2020 15:05
Operator : JC/MD
Sample : L1042-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFRA4

Manual Integrations
APPROVED

apatel
1/9/2020 3:45:14 PM

Quant Time: Jan 09 11:50:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 09 03:50:28 2020
Response via : Initial Calibration

