


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010820\
 Data File : VU036400.D
 Acq On : 08 Jan 2020 10:40
 Operator : JC/MD
 Sample : BFB35
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB35

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
 Title : VOC Analysis
 Last Update : Thu Jan 09 03:50:28 2020

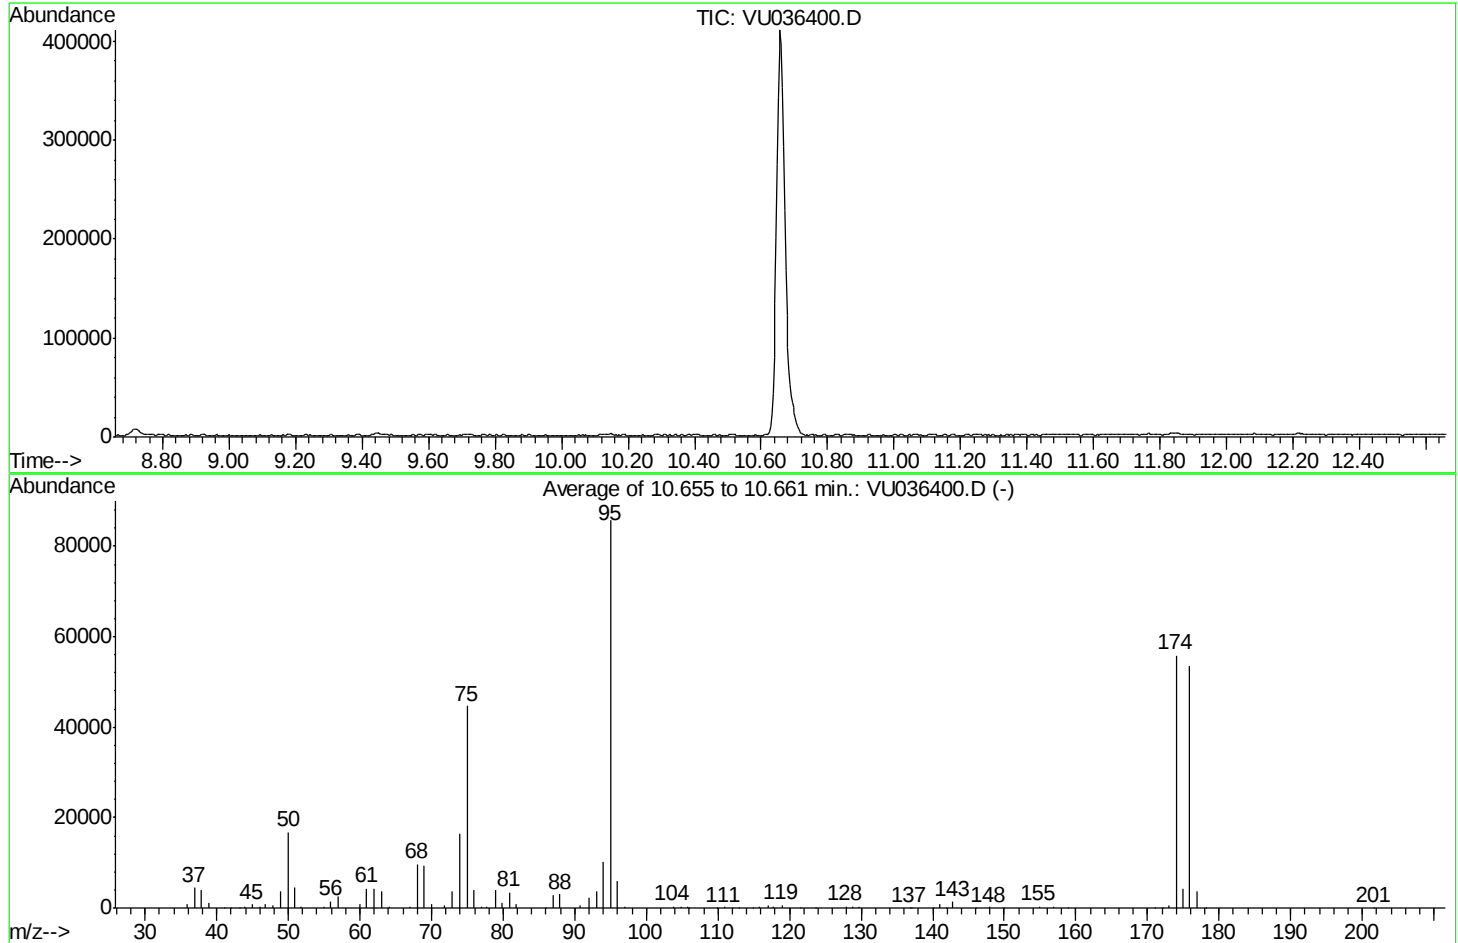

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	16831	PASS
75	95	30	80	52.1	44690	PASS
95	95	100	100	100.0	85741	PASS
96	95	5	9	6.9	5876	PASS
173	174	0.00	2	1.1	628	PASS
174	95	50	120	65.1	55813	PASS
175	174	5	9	7.8	4341	PASS
176	174	95	101	96.0	53554	PASS
177	176	5	9	6.9	3721	PASS

m/z	Abundance
35.90	842.0
36.90	4548.0
37.90	3881.0
38.90	1472.0
39.80	142.0
40.90	222.0
42.10	122.0
42.90	149.0
43.90	1475.0
44.90	780.0
46.00	150.0
46.80	793.0
47.80	627.0
48.90	3602.0
50.00	16976.0
50.90	4645.0
51.80	394.0
54.90	528.0
55.90	1668.0
57.00	2736.0
60.00	807.0
60.90	4564.0
62.00	4561.0
63.00	3341.0
64.10	428.0
67.00	297.0
68.00	9105.0
69.00	9550.0
70.00	900.0
71.90	417.0
73.00	3909.0
73.90	16063.0
75.00	43864.0
75.90	4056.0
76.90	483.0
77.70	238.0
78.90	3896.0
79.80	1348.0
80.90	3378.0
81.80	713.0
85.90	110.0
86.90	2814.0
88.00	3205.0
90.80	416.0
92.00	2376.0
93.00	4122.0
94.00	9944.0
95.00	85072.0
96.00	6132.0
97.00	335.0
103.70	380.0
104.80	197.0
105.70	369.0
109.90	107.0
110.80	236.0
114.90	118.0
115.70	344.0
117.00	416.0
117.70	257.0
118.90	435.0
121.50	123.0
127.90	398.0
128.90	196.0
129.60	288.0
136.80	126.0
140.90	952.0
142.90	1214.0
145.90	128.0
147.90	184.0
154.80	262.0
156.90	109.0
171.00	116.0
172.00	246.0
173.00	638.0
174.00	52896.0
174.90	3954.0
175.90	51576.0
176.90	3553.0
178.10	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
35.90	891.0
36.90	4714.0
37.90	4156.0
38.90	1427.0
39.80	246.0
41.00	300.0
42.00	143.0
43.10	121.0
43.90	1469.0
44.90	809.0
46.00	217.0
46.80	832.0
47.70	605.0
48.90	3728.0
50.00	17264.0
51.00	4688.0
51.80	482.0
54.90	621.0
55.90	1751.0
57.00	2709.0
59.90	731.0
60.90	4494.0
62.00	4378.0
63.00	3745.0
64.00	339.0
67.00	322.0
68.00	10056.0
69.00	9503.0
70.00	785.0
71.90	488.0
73.00	3749.0
74.00	16840.0
75.00	45976.0
75.90	4241.0
76.90	410.0
77.80	253.0
78.90	4160.0
79.80	1274.0
80.90	3578.0
81.80	801.0
85.90	145.0
86.90	2973.0
88.00	3164.0
90.70	458.0
92.00	2461.0
93.00	3796.0
94.00	10570.0
95.00	88168.0
96.00	6102.0
97.00	376.0
103.80	391.0
104.80	207.0
105.70	401.0
109.90	120.0
110.90	174.0
112.00	135.0
112.90	102.0
114.90	125.0
115.80	386.0
116.90	529.0
117.70	169.0
118.90	606.0
121.50	132.0
127.90	459.0
128.80	278.0
129.70	329.0
136.80	130.0
140.90	1015.0
141.90	132.0
142.80	1429.0
147.90	221.0
149.90	104.0
154.80	323.0
157.00	209.0
171.10	117.0
173.00	650.0
174.00	57256.0
174.90	4557.0
175.90	55240.0
176.90	3756.0
178.10	132.0
201.60	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
35.90	862.0
36.90	4240.0
37.90	3786.0
38.90	1295.0
39.80	286.0
41.00	294.0
41.90	166.0
43.10	185.0
43.90	1499.0
44.90	839.0
46.00	172.0
46.90	881.0
47.70	534.0
48.90	3625.0
50.00	16255.0
51.00	4829.0
51.90	407.0
54.90	621.0
55.90	1581.0
56.90	2769.0
59.90	694.0
60.90	4083.0
61.90	4012.0
62.90	3797.0
64.00	257.0
67.00	303.0
68.00	10044.0
68.90	8950.0
69.90	617.0
71.80	484.0
72.90	3539.0
74.00	16760.0
75.00	44232.0
75.90	3782.0
77.00	345.0
77.80	226.0
78.90	3995.0
79.90	1137.0
80.90	3504.0
81.90	845.0
85.90	178.0
86.90	2927.0
87.90	2959.0
90.80	499.0
92.00	2239.0
93.00	3269.0
94.00	10136.0
95.00	83984.0
96.00	5395.0
97.10	351.0
103.80	463.0
104.80	168.0
105.90	443.0
111.00	188.0
112.00	172.0
112.80	157.0
115.80	390.0
116.90	585.0
117.70	138.0
118.90	683.0
123.70	117.0
127.90	425.0
128.80	309.0
129.80	372.0
137.00	173.0
140.00	111.0
140.90	870.0
141.80	154.0
142.80	1312.0
147.90	179.0
149.90	107.0
154.90	352.0
157.00	226.0
158.80	112.0
172.90	596.0
174.00	57288.0
174.90	4512.0
175.90	53848.0
176.90	3854.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

Scan 2884 (10.613 min): VU036400.D
BFB35

m/z	Abundance
39.00	273.0
39.80	282.0
41.10	226.0
43.00	178.0
43.90	1230.0
50.80	115.0
55.00	163.0
56.10	138.0
56.80	107.0
61.50	106.0
73.00	184.0
76.90	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35