

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010821\
 Data File : VU041866.D
 Acq On : 07 Jan 2021 11:04
 Operator : SY/MD
 Sample : L5214-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 08 00:31:01 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUSIM120820.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 08 00:30:19 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.23	114	6093	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.36	117	5660	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.74	152	2787	0.50	ug/L	0.00

System Monitoring Compounds

2) Vinyl Chloride-d3	1.61	65	3071	0.50	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	100.00%
4) 1,2-Dichloroethane-d4	5.68	65	3410	0.41	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	82.00%
7) 1,2-Dichloropropane-d6	6.64	67	3751	0.55	ug/L	-0.02
Spiked Amount	0.500	Range	60 - 140	Recovery	=	110.00%
8) Toluene-d8	7.85	98	6406	0.51	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.00%
10) 1,1,2,2-Tetrachloroethane-	10.68	84	4139	0.59	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	118.00%

Target Compounds


					Qvalue
3) Vinyl chloride	1.61	62	277	0.032	ug/L # 67
6) Trichloroethene	6.51	95	187	0.026	ug/L 92
9) 1,2-Dibromoethane	8.87	107	136	0.027	ug/L # 88
12) 1,2,3-Trichloropropane	10.75	75	137	0.031	ug/L # 87
13) 1,2-Dibromo-3-chloropropan	12.91	75	21	0.023	ug/L 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010821\
Data File : VU041866.D
Acq On : 07 Jan 2021 11:04
Operator : SY/MD
Sample : L5214-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jan 08 00:31:01 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUSIM120820.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 08 00:30:19 2021
Response via : Initial Calibration

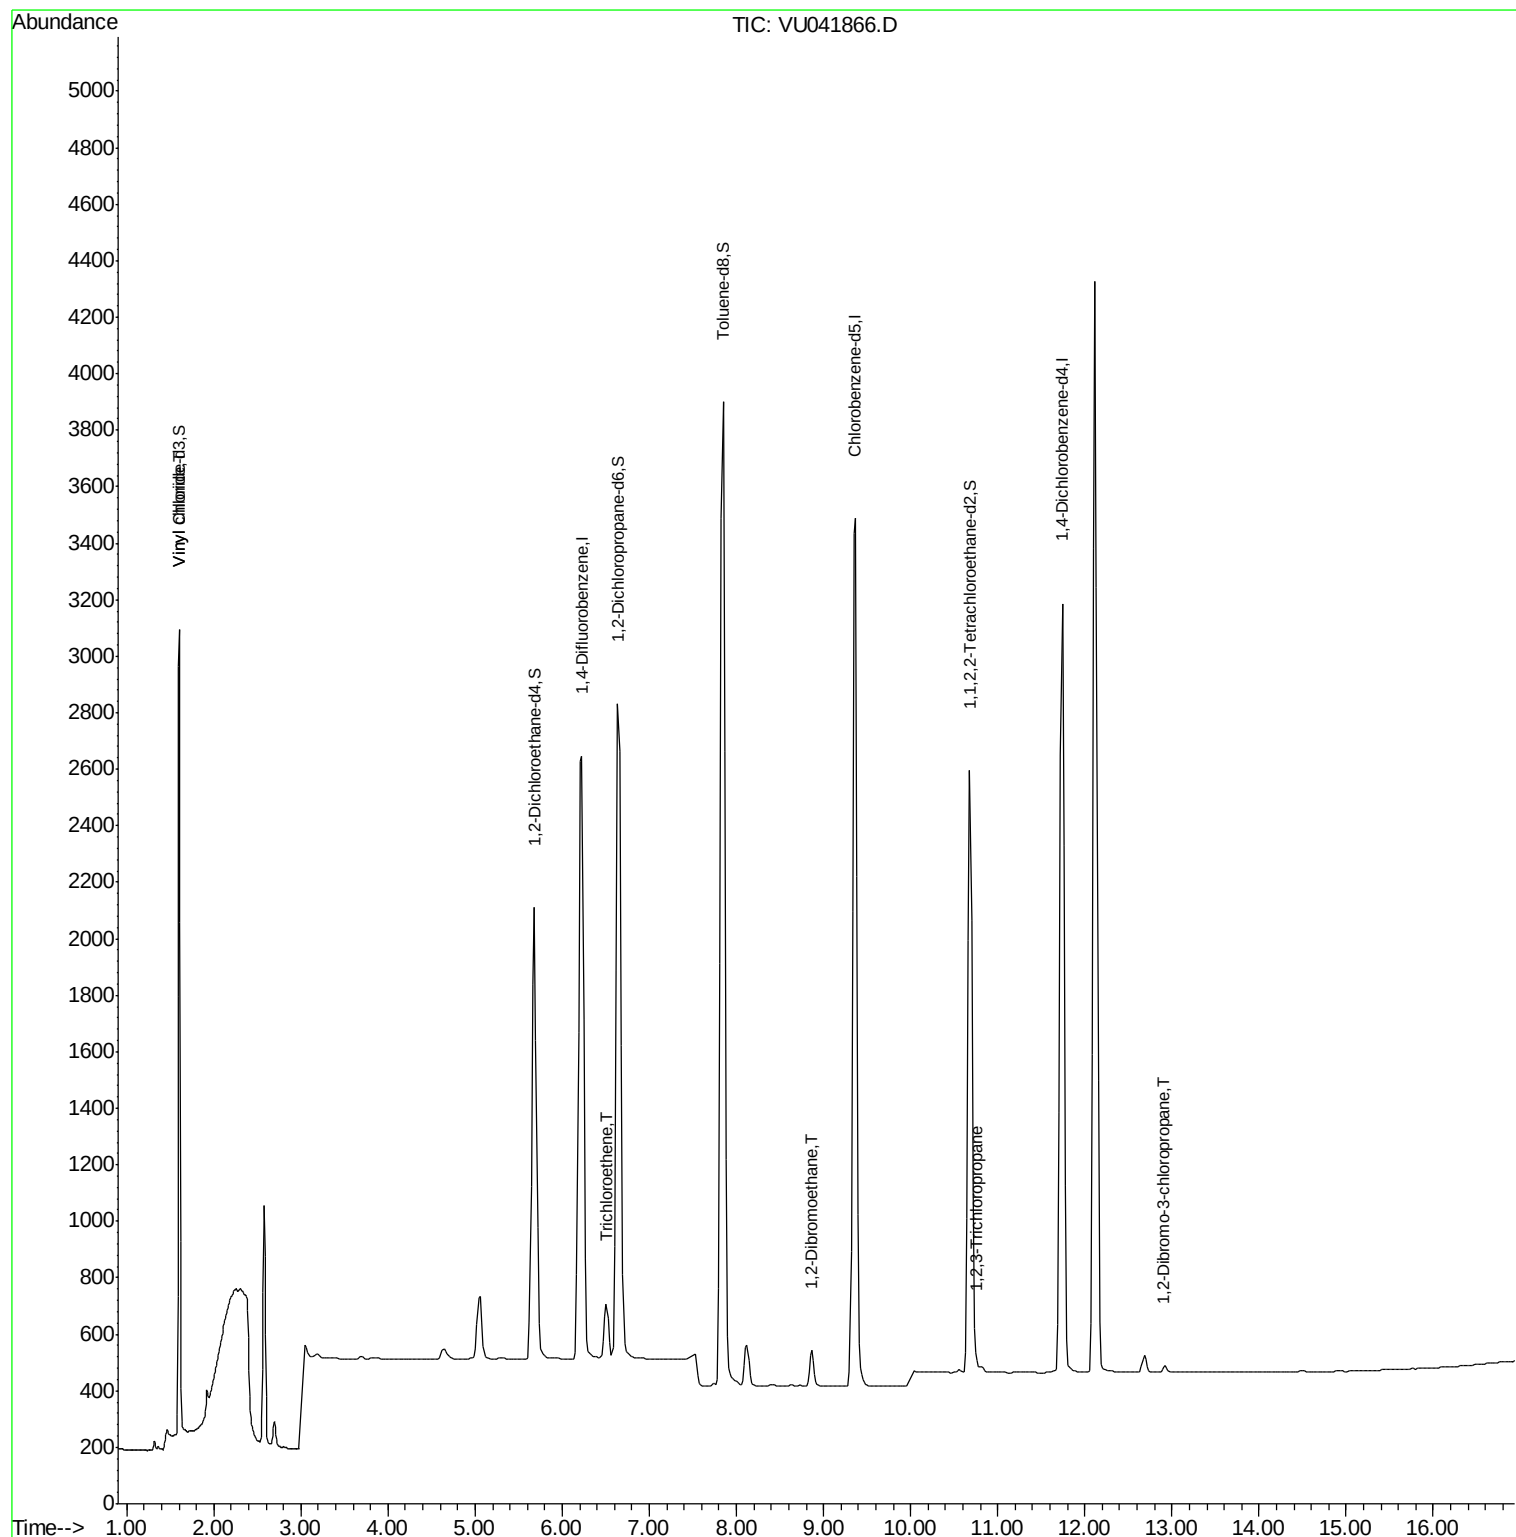

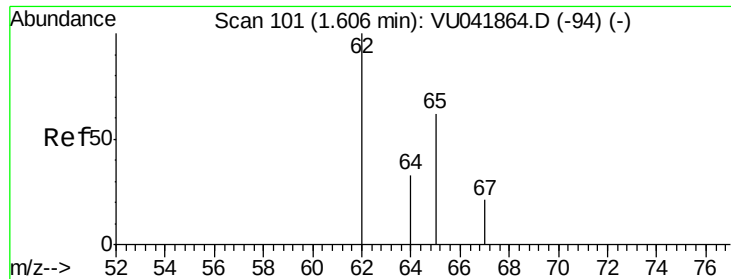

#3

Vinyl chloride

Concen: 0.032 ug/L

RT: 1.61 min Scan# 101

Delta R.T. -0.00 min

Lab File: VU041866.D

Acq: 07 Jan 2021 11:04

Instrument :

MSVOA_U





ClientSampled :

Tot Ion: 62 Resp: 277

Ion Ratio Lower Upper

62 100

64 76.8 78.3 145.3#

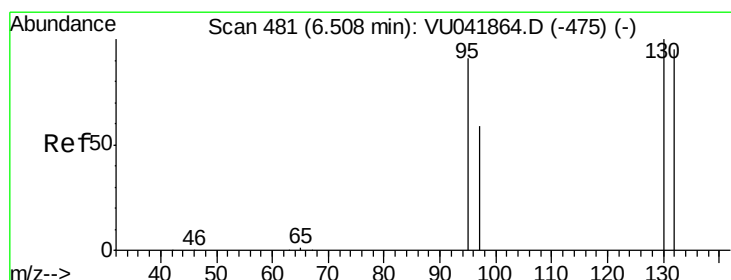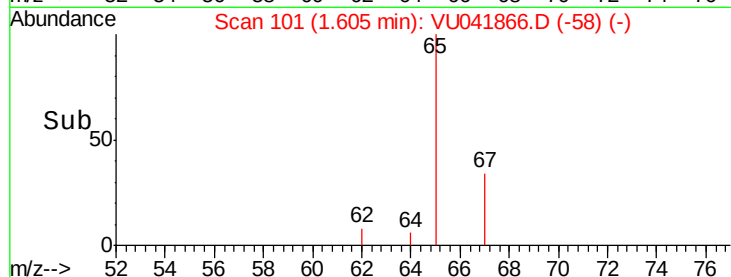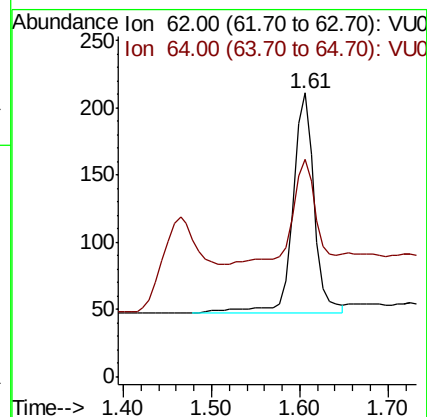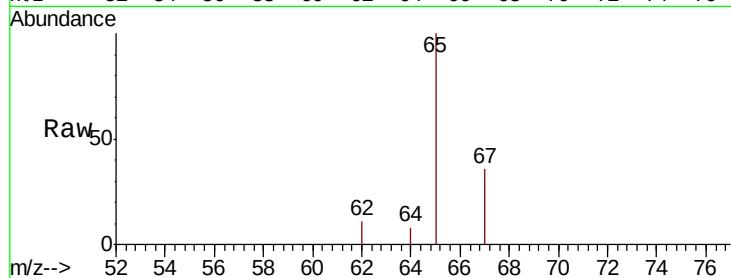

#6

Trichloroethene

Concen: 0.026 ug/L

RT: 6.51 min Scan# 481

Delta R.T. -0.00 min

Lab File: VU041866.D

Acq: 07 Jan 2021 11:04

Tgt Ion: 95 Resp: 187




Ion Ratio Lower Upper


95 100

97 79.6 49.2 91.4

132 99.0 74.5 138.3

130 102.0 77.1 143.3

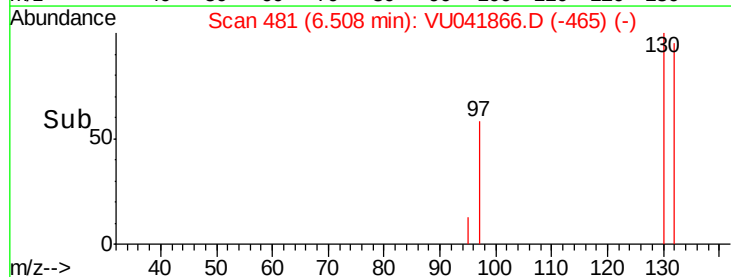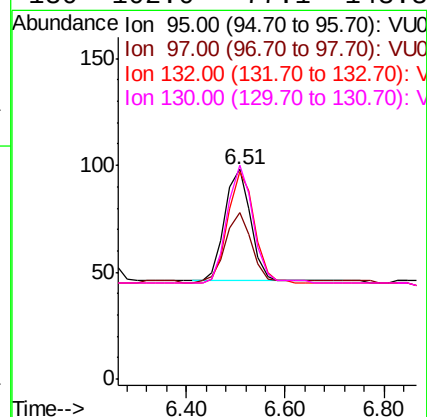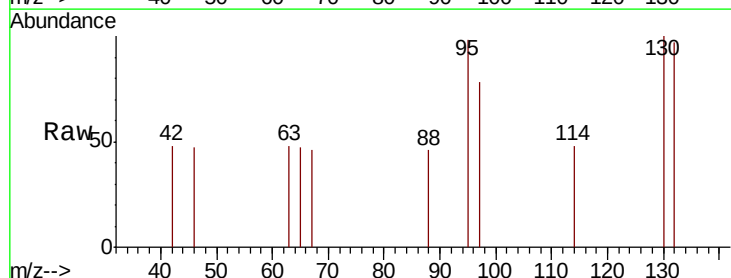

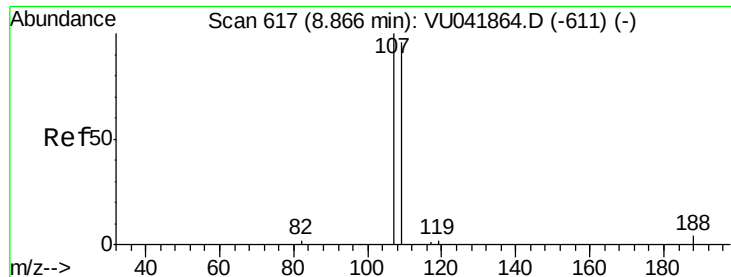

#9

1,2-Dibromoethane

Concen: 0.027 ug/L

RT: 8.87 min Scan# 617

Delta R.T. -0.00 min

Lab File: VU041866.D

Acq: 07 Jan 2021 11:04

Instrument :

MSVOA_U

ClientSampleId :


Tot Ion:107 Resp: 136

Ion Ratio Lower Upper

107 100

109 95.4 66.8 124.2




188 54.0 18.7 28.1#

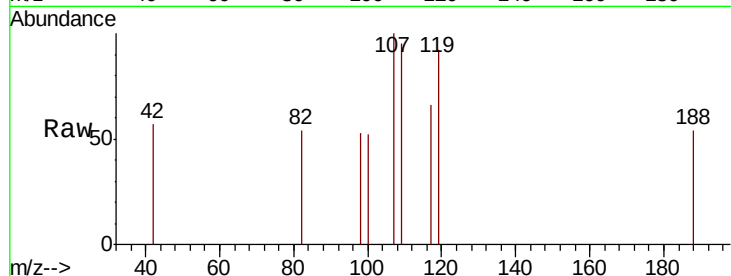

Abundance Ion 107.00 (106.70 to 107.70): V

Ion 109.00 (108.70 to 109.70): V

Ion 188.00 (187.70 to 188.70): V

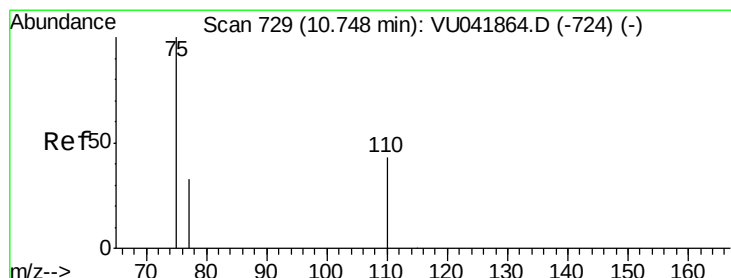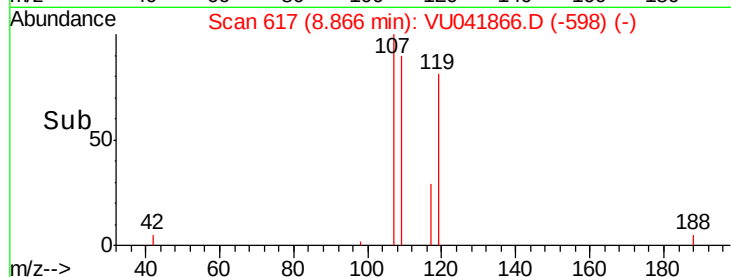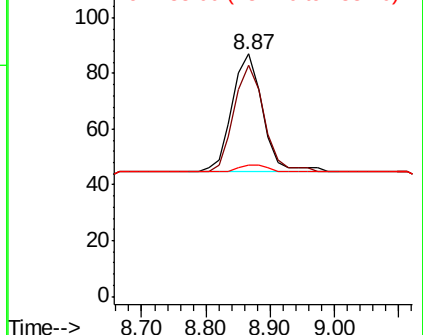

#12

1,2,3-Trichloropropane

Concen: 0.031 ug/L

RT: 10.75 min Scan# 729

Delta R.T. -0.00 min

Lab File: VU041866.D

Acq: 07 Jan 2021 11:04


Tgt Ion: 75 Resp: 137

Ion Ratio Lower Upper

75 100

110 47.4 34.0 51.0



77 24.1 28.6 42.8#

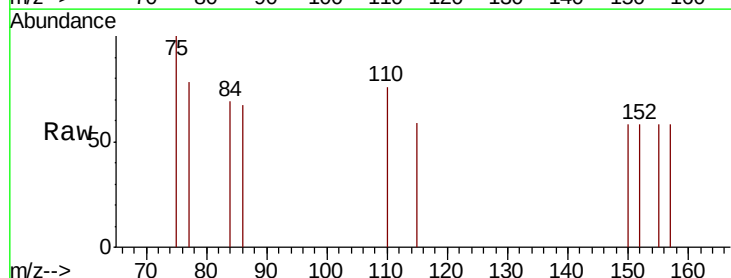


Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 110.00 (109.70 to 110.70): V

Ion 77.00 (76.70 to 77.70): VU0

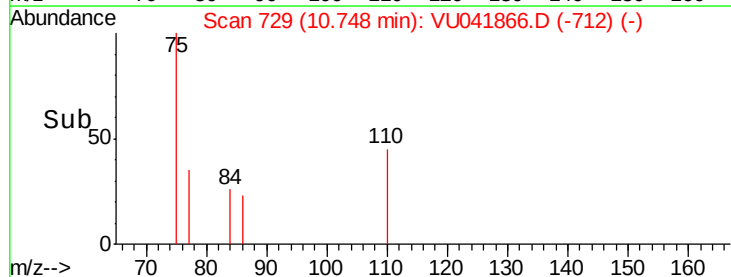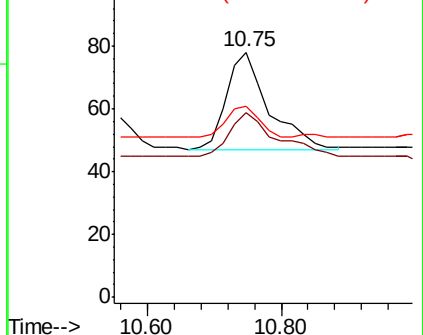

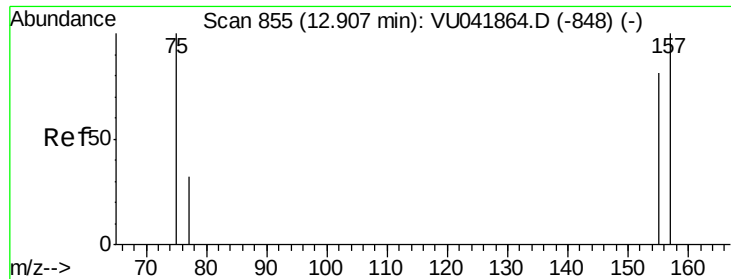

#13

1,2-Dibromo-3-chloropropane

Concen: 0.023 ug/L

RT: 12.91 min Scan# 855

Delta R.T. -0.00 min

Lab File: VU041866.D

Acq: 07 Jan 2021 11:04

Instrument :

MSVOA_U

ClientSampleId :


Tot Ion: 75 Resp: 21

Ion Ratio Lower Upper

75 100

157 94.4 72.2 108.2

155 92.6 68.3 102.5

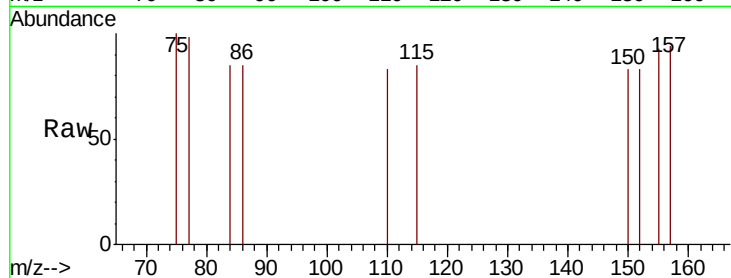

Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 157.00 (156.70 to 157.70): V

Ion 155.00 (154.70 to 155.70): V

