

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010821\
 Data File : VU041865.D
 Acq On : 07 Jan 2021 10:37
 Operator : SY/MD
 Sample : VU0108WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 08 00:30:58 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUSIM120820.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 08 00:30:19 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.23	114	6173	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.36	117	5695	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.74	152	2809	0.50	ug/L	0.00

System Monitoring Compounds

2) Vinyl Chloride-d3	1.60	65	3027	0.49	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	98.00%
4) 1,2-Dichloroethane-d4	5.68	65	3328	0.39	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	78.00%
7) 1,2-Dichloropropane-d6	6.64	67	3677	0.54	ug/L	-0.02
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.00%
8) Toluene-d8	7.85	98	6235	0.49	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.00%
10) 1,1,2,2-Tetrachloroethane-	10.68	84	4112	0.59	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	118.00%

Target Compounds


					Qvalue
13) 1,2-Dibromo-3-chloropropan	12.91	75	12	0.013	ug/L 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010821\
Data File : VU041865.D
Acq On : 07 Jan 2021 10:37
Operator : SY/MD
Sample : VU0108WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jan 08 00:30:58 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUSIM120820.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 08 00:30:19 2021
Response via : Initial Calibration

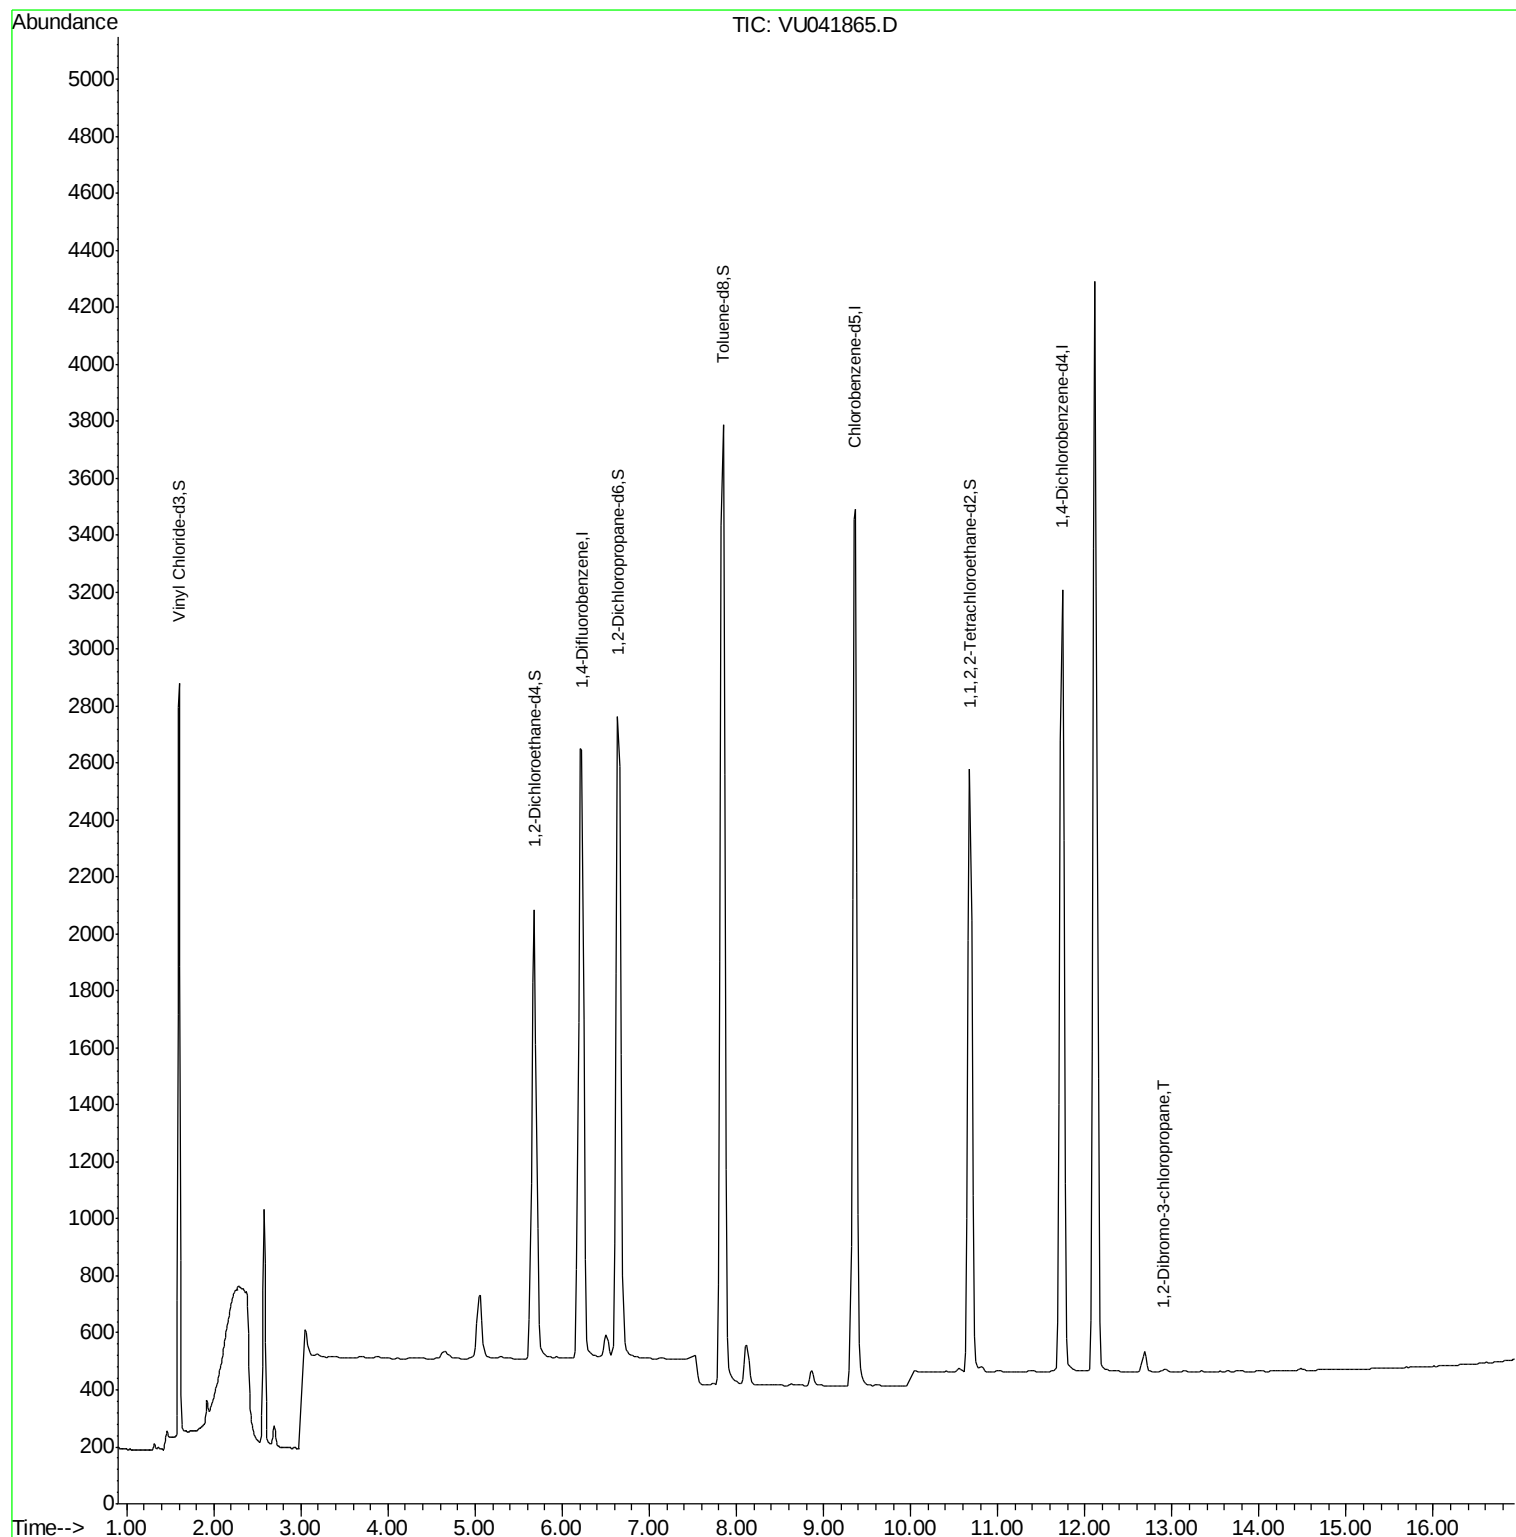

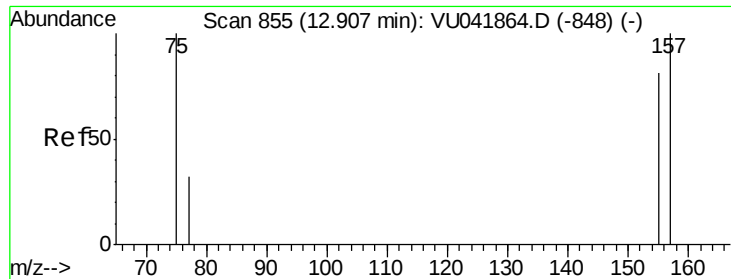

#13

1,2-Dibromo-3-chloropropane

Concen: 0.013 ug/L

RT: 12.91 min Scan# 855

Delta R.T. -0.00 min


Lab File: VU041865.D

Acq: 07 Jan 2021 10:37

Instrument :

MSVOA_U

ClientSampleId :

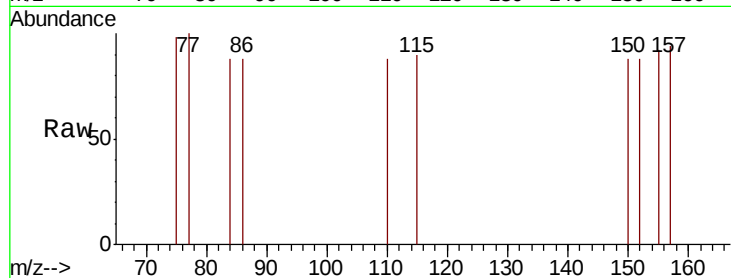

Tot Ion: 75 Resp: 12

Ion Ratio Lower Upper

75 100

157 96.0 72.2 108.2

155 94.0 68.3 102.5

