


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010822\
Data File : VU046703.D
Acq On : 08 Jan 2022 14:01
Operator : SY/MD
Sample : N1077-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXT8

Manual IntegrationsAPPROVED

Quant Time: Jan 10 00:40:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jan 10 00:25:50 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/10/2022
Supervised By :Mahesh Dadoda 01/10/2022

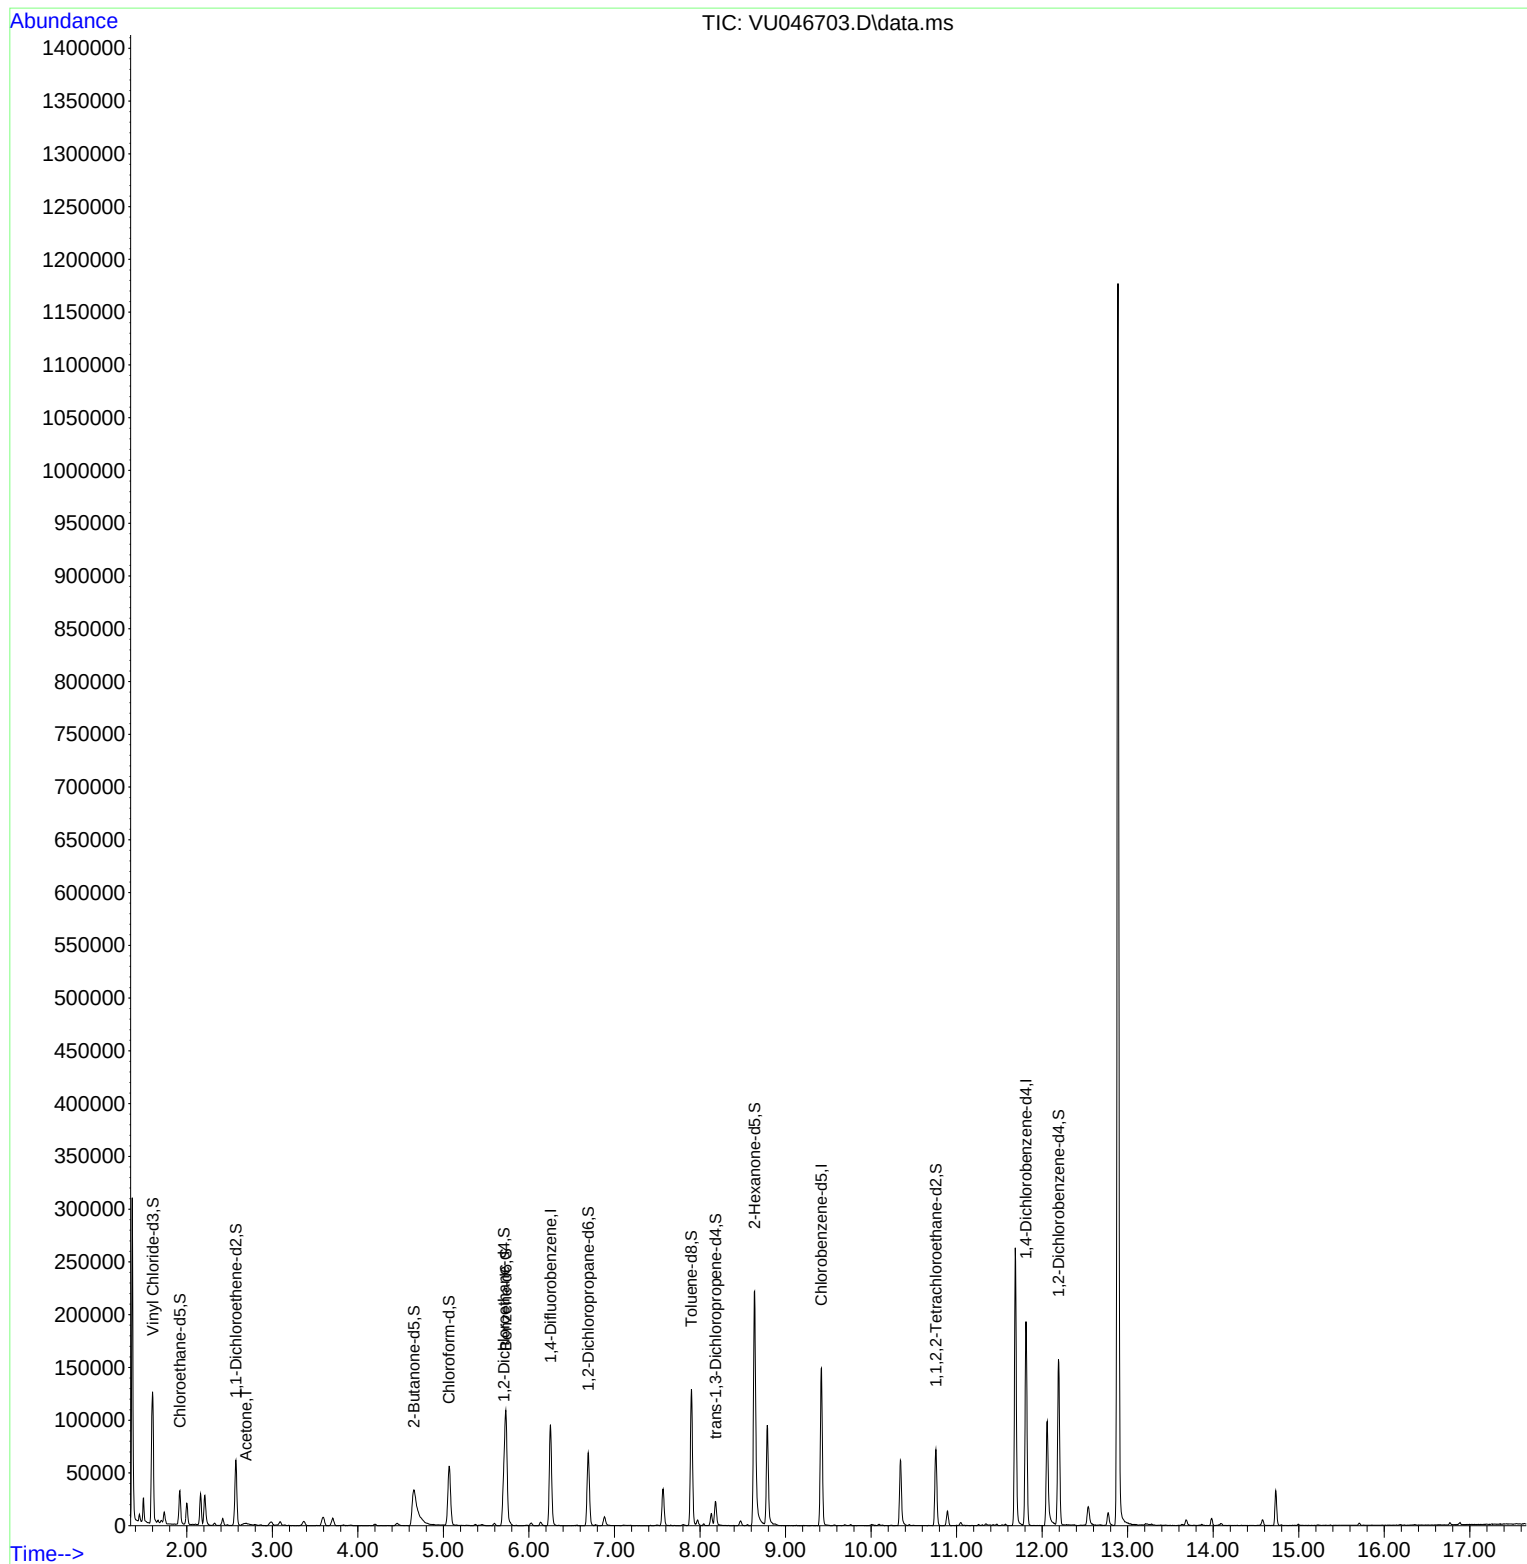




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010822\
 Data File : VU046703.D
 Acq On : 08 Jan 2022 14:01
 Operator : SY/MD
 Sample : N1077-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXT8

Manual IntegrationsAPPROVED

Quant Time: Jan 10 00:40:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 10 00:25:50 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

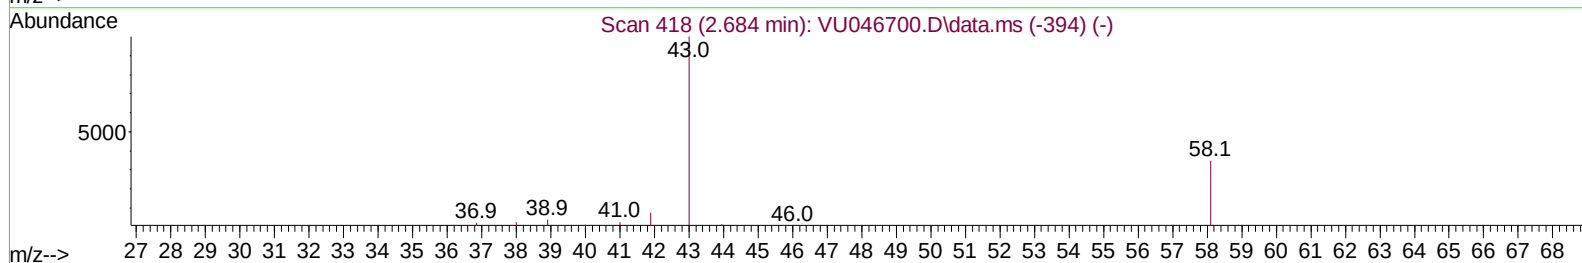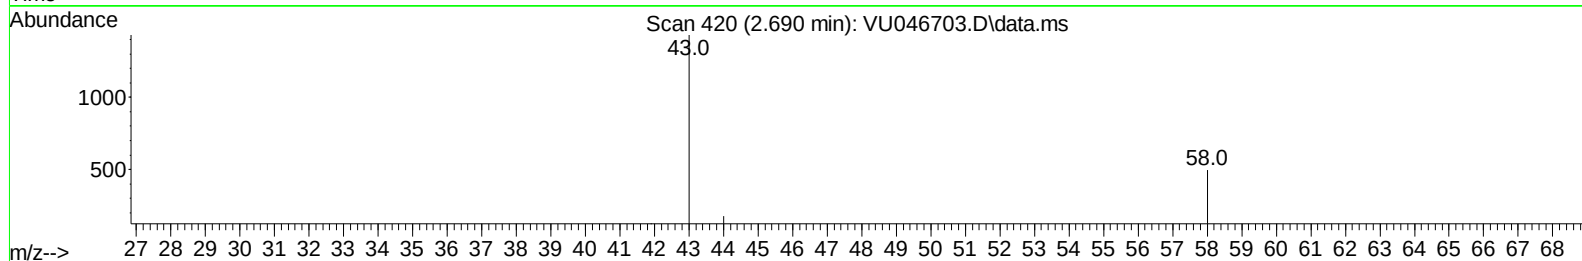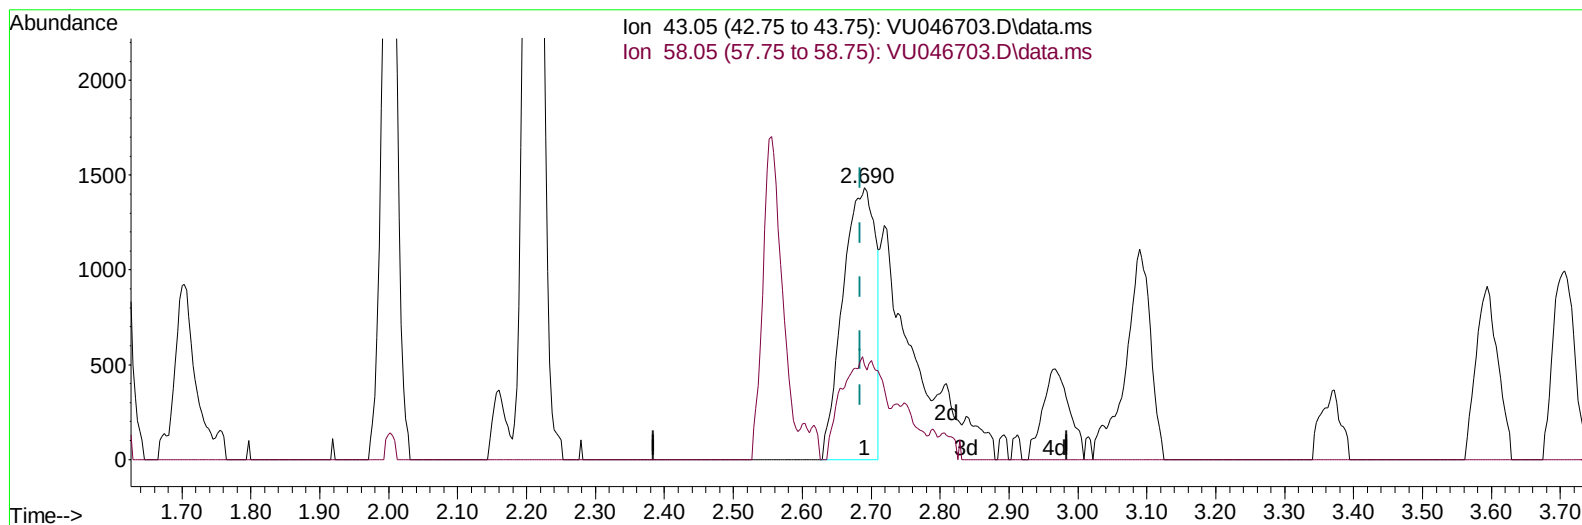

TIC: VU046703.D\data.ms

(13) Acetone (T)

2.690min (+ 0.006) 2.77 ug/L

response 4677

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	28.91
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010822\
 Data File : VU046703.D
 Acq On : 08 Jan 2022 14:01
 Operator : SY/MD
 Sample : N1077-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXT8

Manual IntegrationsAPPROVED

Quant Time: Jan 10 00:40:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 10 00:25:50 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

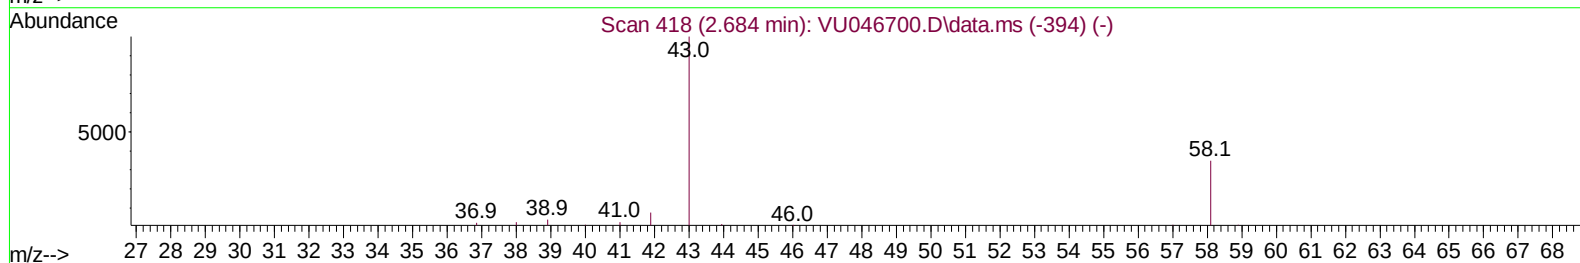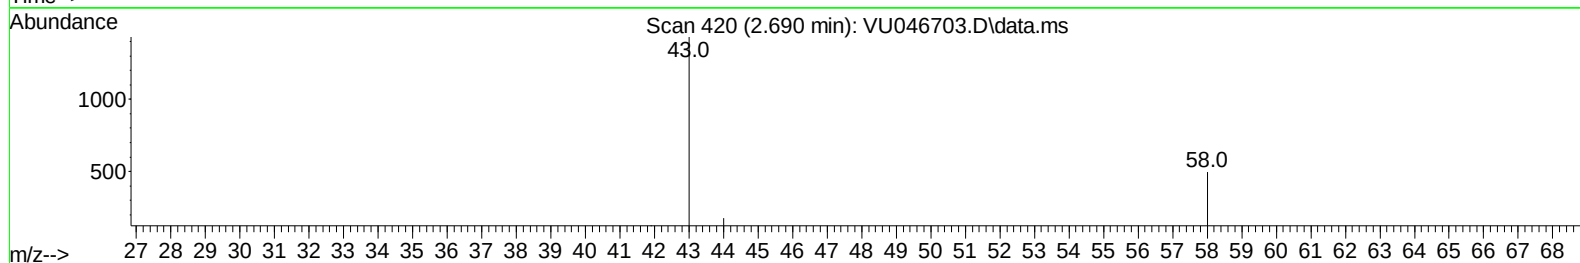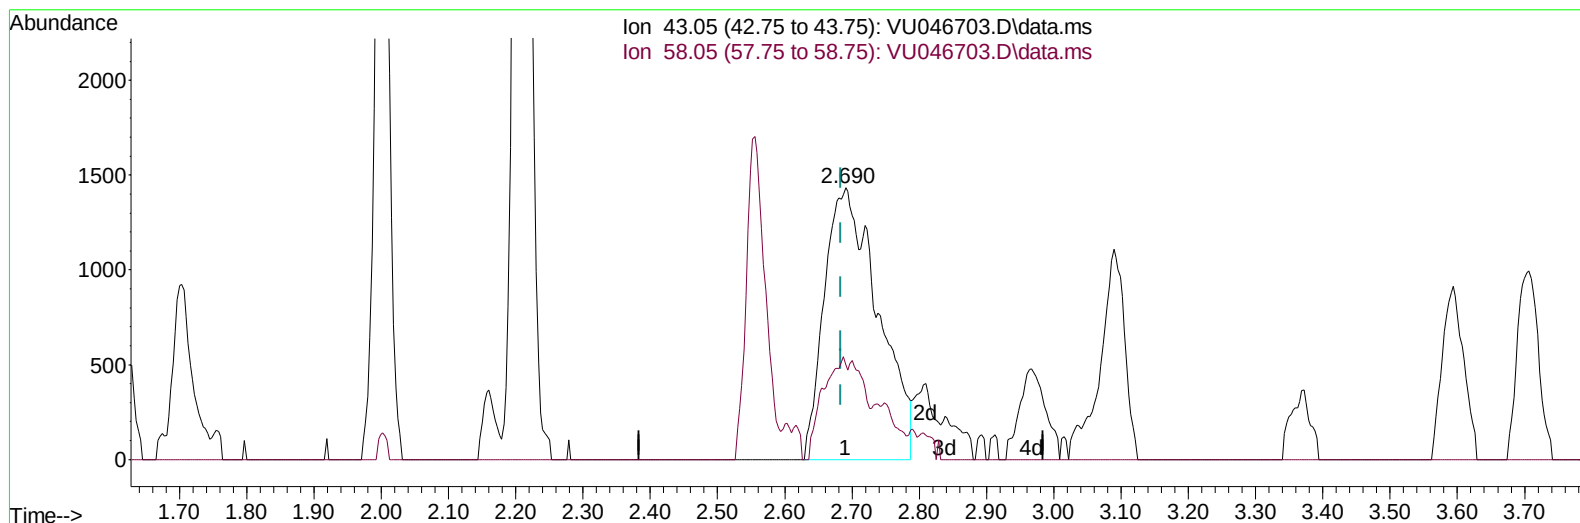

TIC: VU046703.D\data.ms

(13) Acetone (T)

2.690min (+ 0.006) 4.71 ug/L m

response 7934

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	17.04
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010822\
 Data File : VU046703.D
 Acq On : 08 Jan 2022 14:01
 Operator : SY/MD
 Sample : N1077-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXT8

Manual IntegrationsAPPROVED

Quant Time: Jan 10 00:40:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 10 00:25:50 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	78702	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	85328	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	51496	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	25592	4.128	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.600%
7) Chloroethane-d5	1.919	69	21472	4.399	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.000%
11) 1,1-Dichloroethene-d2	2.575	65	11508	4.402	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.000%
20) 2-Butanone-d5	4.655	46	96339	53.577	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.160%
24) Chloroform-d	5.066	84	54226	4.774	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.400%
26) 1,2-Dichloroethane-d4	5.706	65	32286	4.972	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%
32) Benzene-d6	5.732	84	103696	4.360	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%
36) 1,2-Dichloropropane-d6	6.693	67	33040	4.623	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.400%
41) Toluene-d8	7.899	98	87984	4.076	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.600%
43) trans-1,3-Dichloroprop...	8.182	79	14343	4.339	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.800%
46) 2-Hexanone-d5	8.639	63	92399	47.608	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.220%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	36380	4.959	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	40988	4.321	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.400%
Target Compounds					Qvalue	
13) Acetone	2.690	43	7934m	4.706	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed