


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010822\
 Data File : VU046699.D
 Acq On : 08 Jan 2022 10:18
 Operator : SY/MD
 Sample : BFB040
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB040

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jan 10 00:25:50 2022

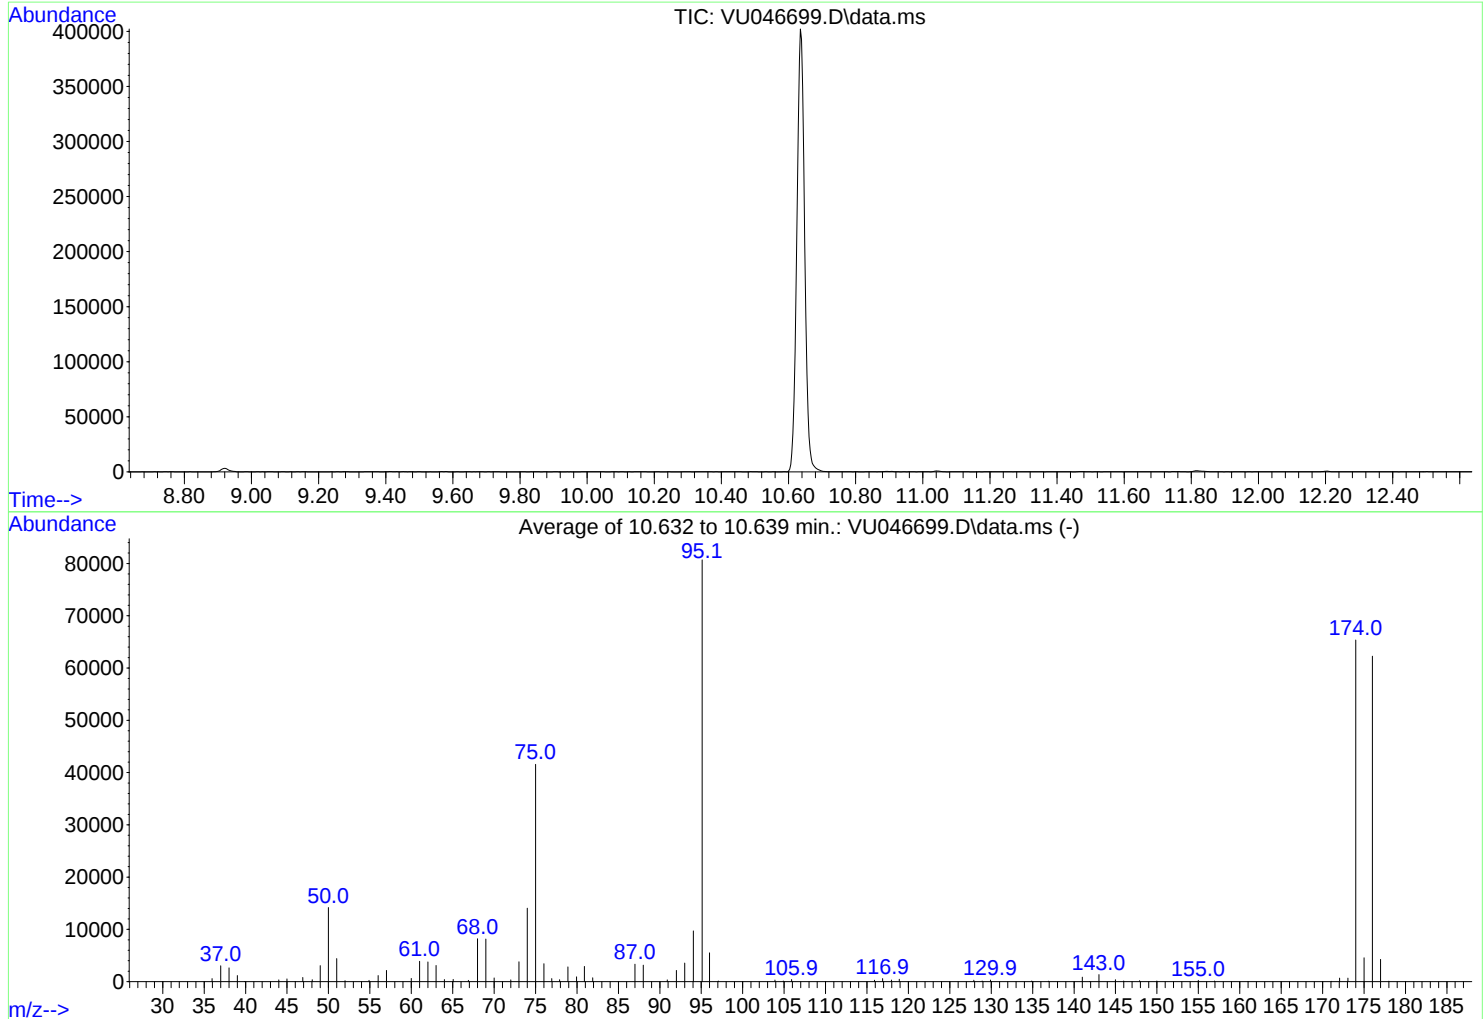

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	14174	PASS
75	95	30	80	51.5	41589	PASS
95	95	100	100	100.0	80701	PASS
96	95	5	9	6.8	5501	PASS
173	174	0.00	2	1.0	666	PASS
174	95	50	120	81.0	65352	PASS
175	174	5	9	7.0	4567	PASS
176	174	95	101	95.3	62256	PASS
177	176	5	9	6.9	4268	PASS

m/z	Abundance
36.00	552.0
37.00	3069.0
38.00	2567.0
39.00	1092.0
39.90	102.0
44.00	380.0
45.00	510.0
46.90	765.0
48.10	383.0
49.00	3080.0
50.00	13962.0
51.00	4401.0
52.00	188.0
54.90	256.0
56.00	1099.0
57.00	2055.0
60.00	651.0
61.00	3859.0
62.00	3765.0
63.00	3114.0
64.00	399.0
65.10	443.0
66.90	257.0
68.00	8134.0
69.00	8216.0
70.00	669.0
72.00	323.0
73.00	3872.0
74.00	14053.0
75.00	41576.0
76.00	3240.0
76.90	638.0
77.90	363.0
78.90	2843.0
80.00	944.0
80.90	2893.0
81.90	690.0
87.00	3441.0
88.00	3122.0
90.90	315.0
92.00	2162.0
93.00	3524.0
94.10	9899.0
95.10	80800.0
96.00	5441.0
97.00	122.0
103.90	316.0
104.90	136.0
105.90	415.0
115.90	279.0
116.90	647.0
118.00	303.0
118.90	448.0
127.90	283.0
128.90	134.0
129.90	298.0
134.90	124.0
136.90	157.0
141.00	838.0
143.00	1462.0
145.00	348.0
146.00	117.0
147.90	175.0
150.00	136.0
155.00	280.0
157.00	135.0
172.00	681.0
173.10	709.0
174.00	66848.0
175.00	4697.0
176.00	64216.0
177.00	4191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
36.00	609.0
37.00	3114.0
38.00	2758.0
39.00	1186.0
44.00	467.0
45.00	544.0
46.90	820.0
48.00	382.0
49.00	3180.0
50.00	14713.0
51.00	4602.0
52.00	181.0
54.90	241.0
56.00	1194.0
57.00	2210.0
60.00	629.0
61.00	4055.0
62.00	3950.0
63.00	3203.0
64.00	423.0
65.00	448.0
66.90	262.0
68.00	8526.0
69.00	8364.0
70.00	719.0
72.00	318.0
73.00	3955.0
74.00	14500.0
75.00	42896.0
76.00	3524.0
77.00	608.0
77.90	387.0
78.90	2896.0
80.00	961.0
80.90	2979.0
81.90	753.0
87.00	3404.0
88.00	3225.0
90.90	355.0
92.00	2192.0
93.00	3674.0
94.00	10002.0
95.10	83168.0
96.00	5696.0
97.00	127.0
103.90	320.0
104.90	139.0
105.90	413.0
115.90	302.0
116.90	585.0
118.00	320.0
118.90	468.0
127.90	293.0
128.90	125.0
129.90	302.0
134.90	121.0
136.90	114.0
141.00	917.0
141.90	105.0
143.00	1406.0
145.00	348.0
146.00	115.0
147.90	179.0
150.00	132.0
155.00	246.0
156.90	137.0
161.00	103.0
171.00	105.0
172.00	690.0
173.10	684.0
174.00	67512.0
175.00	4655.0
176.00	64336.0
177.00	4422.0
178.00	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
35.90	583.0
37.00	2885.0
38.00	2613.0
39.00	1217.0
44.00	497.0
45.00	546.0
46.00	107.0
46.90	807.0
48.00	346.0
49.00	2953.0
50.00	13848.0
51.00	4265.0
52.00	172.0
54.90	225.0
56.00	1172.0
57.00	2170.0
60.00	579.0
61.00	3787.0
62.00	3614.0
63.00	3009.0
64.00	420.0
65.00	450.0
66.90	211.0
68.00	7968.0
69.00	7819.0
70.00	690.0
72.00	335.0
73.00	3574.0
74.00	13628.0
75.00	40296.0
76.00	3484.0
77.00	511.0
77.90	354.0
78.90	2719.0
79.90	861.0
80.90	2820.0
81.90	745.0
87.00	3196.0
88.00	3078.0
90.90	345.0
92.00	2104.0
93.00	3435.0
94.00	9197.0
95.10	78136.0
96.00	5367.0
97.10	136.0
103.90	321.0
104.90	130.0
105.90	390.0
115.90	292.0
116.90	508.0
117.90	297.0
118.90	495.0
127.90	278.0
128.90	108.0
129.90	306.0
134.90	115.0
141.00	860.0
143.00	1176.0
145.00	374.0
146.00	105.0
147.90	180.0
150.00	106.0
155.00	177.0
156.90	141.0
171.10	104.0
172.10	660.0
173.00	605.0
174.00	61696.0
175.00	4349.0
176.00	58216.0
177.00	4190.0
178.00	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
44.00	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040