

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057396.D
 Acq On : 08 Jan 2024 20:44
 Operator : MD/SY
 Sample : 05787-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 09 05:07:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 09 00:42:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	282945	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	274734	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	112341	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	77227	39.656	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	79.320%		
7) Chloroethane-d5	1.914	69	61753	40.977	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.960%		
11) 1,1-Dichloroethene-d2	2.560	63	124611	30.189	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	60.380%		
21) 2-Butanone-d5	4.634	46	85769	90.892	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.890%		
24) Chloroform-d	5.055	84	183697	39.889	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	79.780%		
26) 1,2-Dichloroethane-d4	5.692	65	127698	41.975	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.940%		
32) Benzene-d6	5.721	84	320411	43.447	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.900%		
36) 1,2-Dichloropropane-d6	6.682	67	91046	43.741	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	87.480%		
41) Toluene-d8	7.891	98	283605	41.037	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.080%		
43) trans-1,3-Dichloroprop...	8.177	79	51754	41.657	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.320%		
47) 2-Hexanone-d5	8.640	63	63447	93.244	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.240%		
56) 1,1,2,2-Tetrachloroeth...	10.753	84	131517	42.281	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.560%		
66) 1,2-Dichlorobenzene-d4	12.190	152	100552	45.763	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.520%		
Target Compounds						
					Qvalue	
60) 1,2,3-Trichloropropane	11.807	75	12240	5.752	ug/L	# 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057396.D
Acq On : 08 Jan 2024 20:44
Operator : MD/SY
Sample : 05787-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jan 09 05:07:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 09 00:42:22 2024
Response via : Initial Calibration

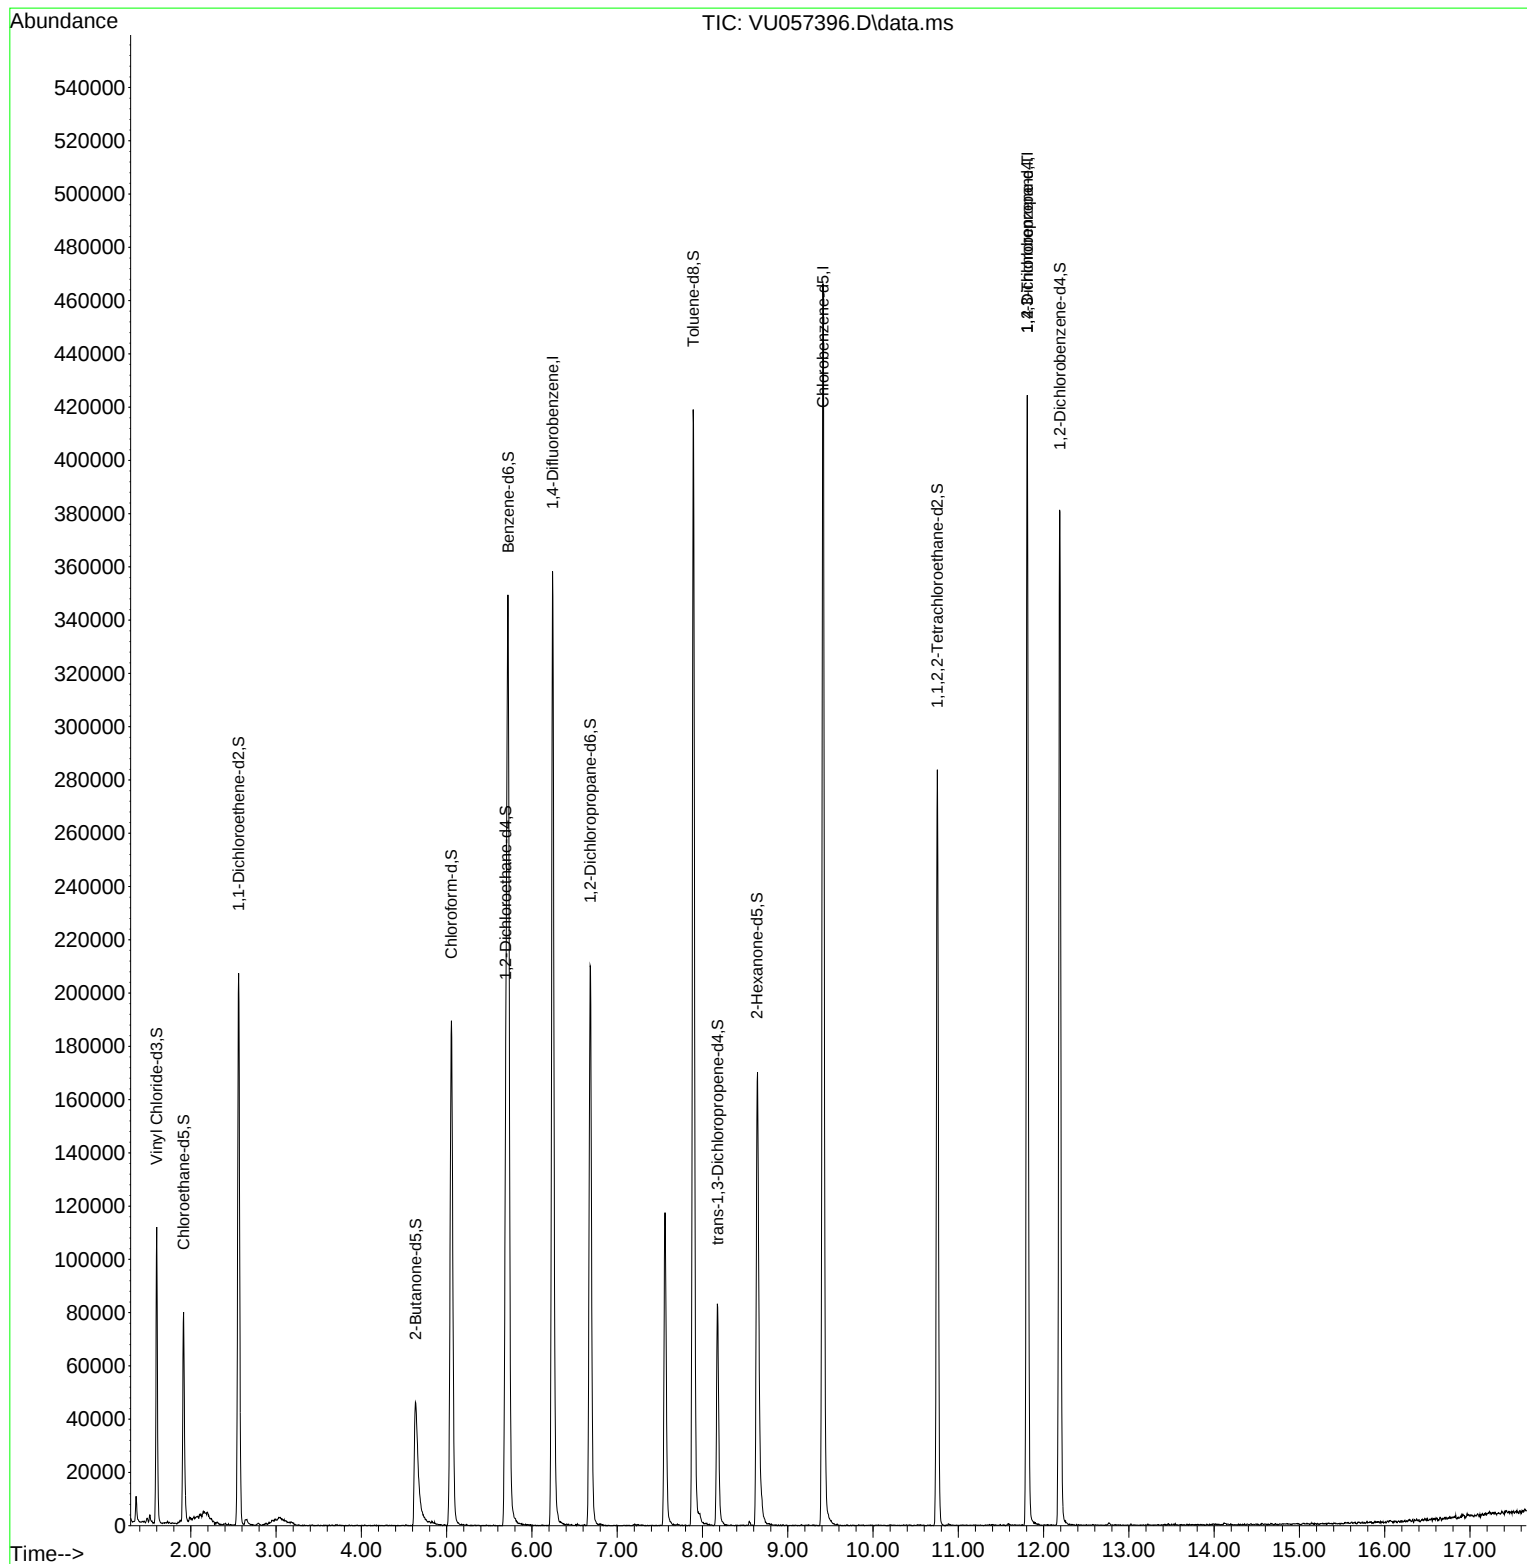

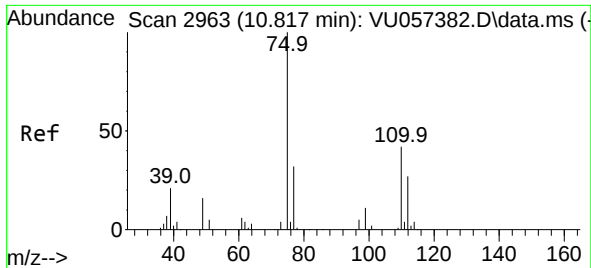

#60
 1,2,3-Trichloropropane
 Concen: 5.752 ug/L
 RT: 11.807 min Scan# 31
 Delta R.T. 0.990 min
 Lab File: VU057396.D
 Acq: 08 Jan 2024 20:44

Instrument :
 MSVOA_U
 ClientSampleId :

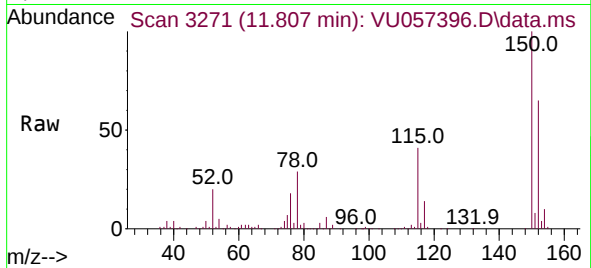

Tgt Ion:	75	Resp:	12240
Ion	Ratio	Lower	Upper
75	100		
77	34.4	26.0	39.0
110	2.2	33.6	50.4#

