




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057389.D
Acq On : 08 Jan 2024 17:55
Operator : MD/SY
Sample : 05787-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME6

Manual IntegrationsAPPROVED

Quant Time: Jan 09 05:05:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 09 00:42:22 2024
Response via : Initial Calibration

Reviewed By :John Carlone 01/09/2024
Supervised By :Mahesh Dadoda 01/09/2024

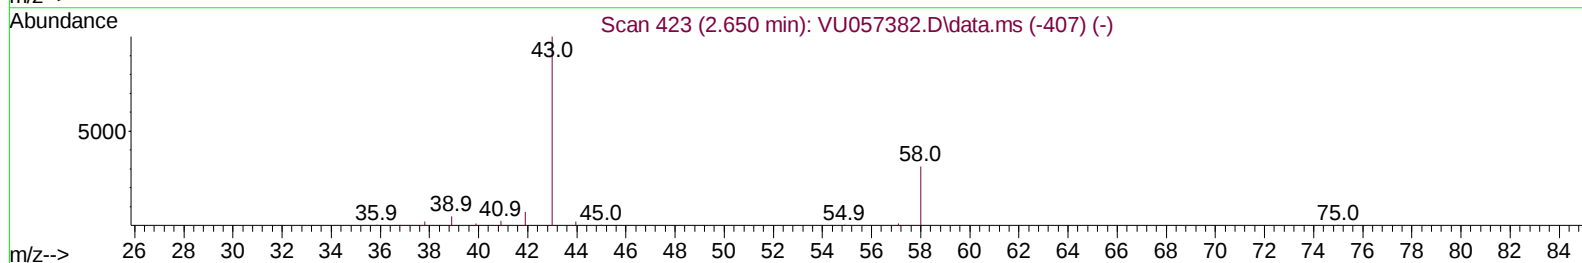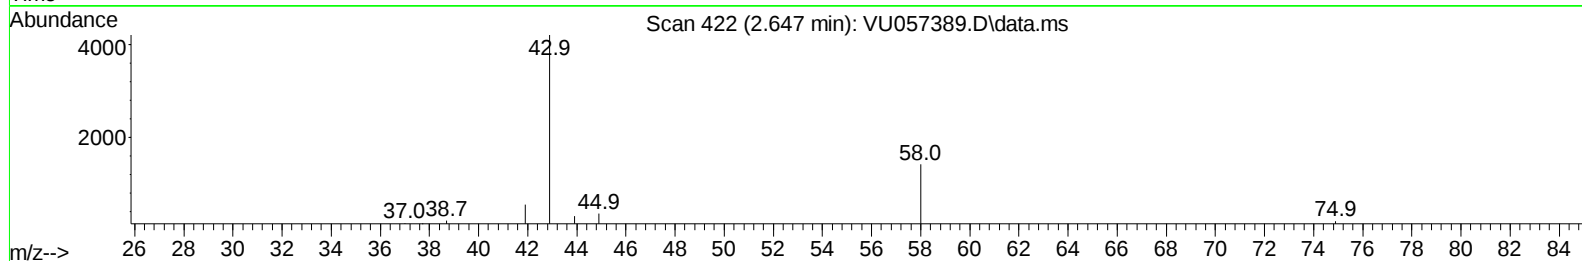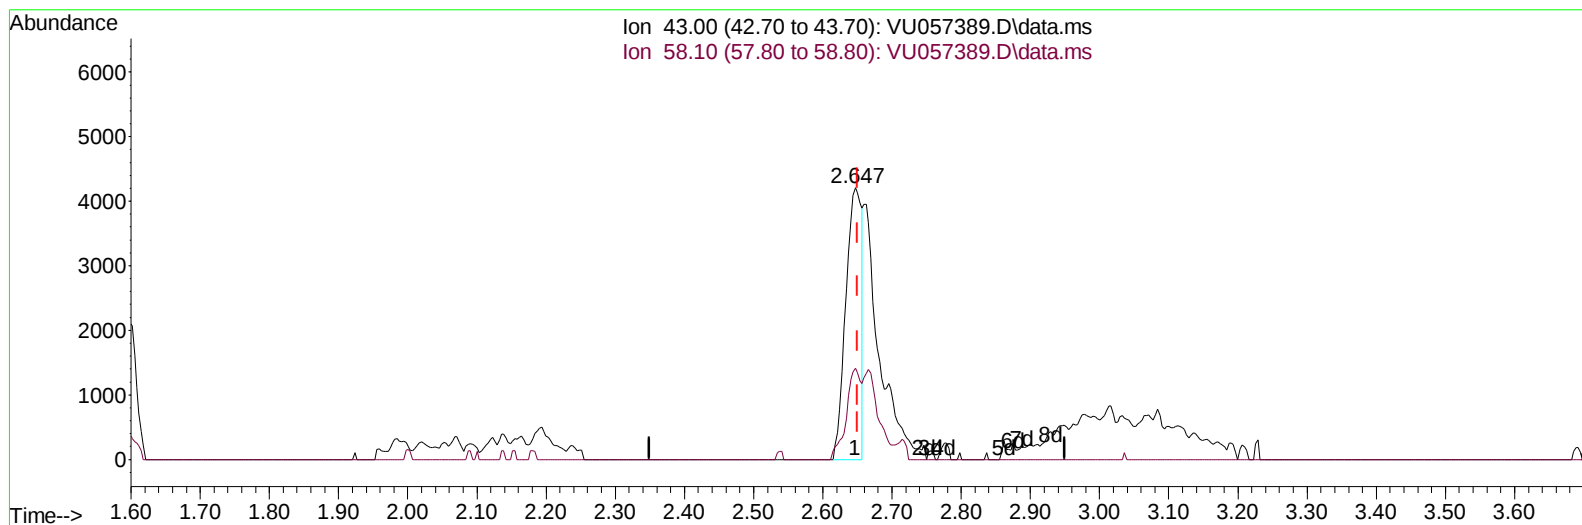

TIC: VU057389.D\data.ms

(13) Acetone (T)

2.647min (-0.003) 6.41 ug/L

response 6684

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	32.60	31.63
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057389.D
 Acq On : 08 Jan 2024 17:55
 Operator : MD/SY
 Sample : 05787-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME6

Manual IntegrationsAPPROVED

Quant Time: Jan 09 05:05:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 09 00:42:22 2024
 Response via : Initial Calibration

Reviewed By :John Carlone 01/09/2024
 Supervised By :Mahesh Dadoda 01/09/2024

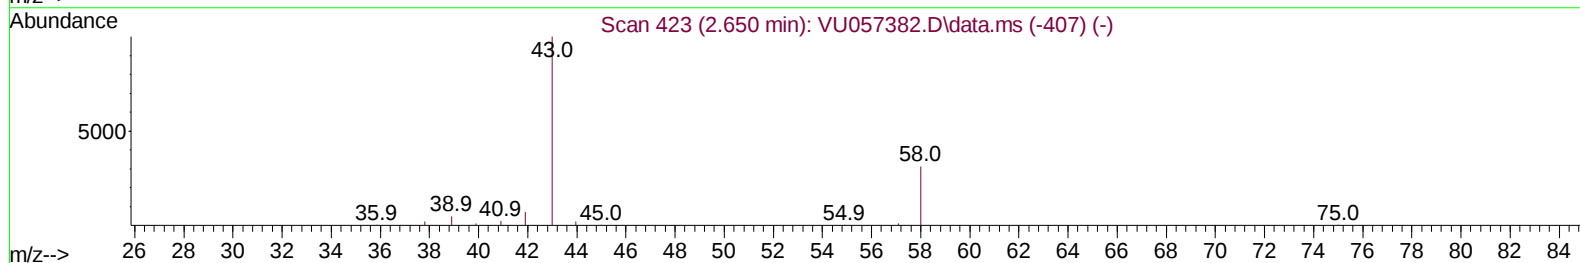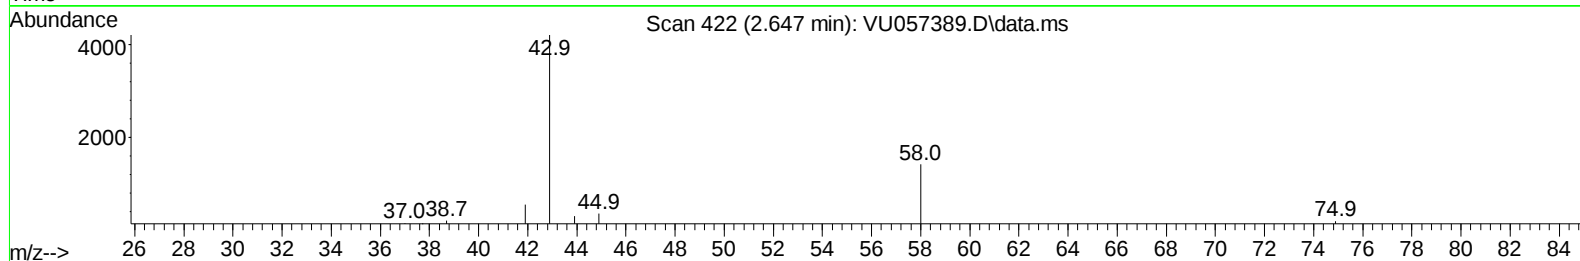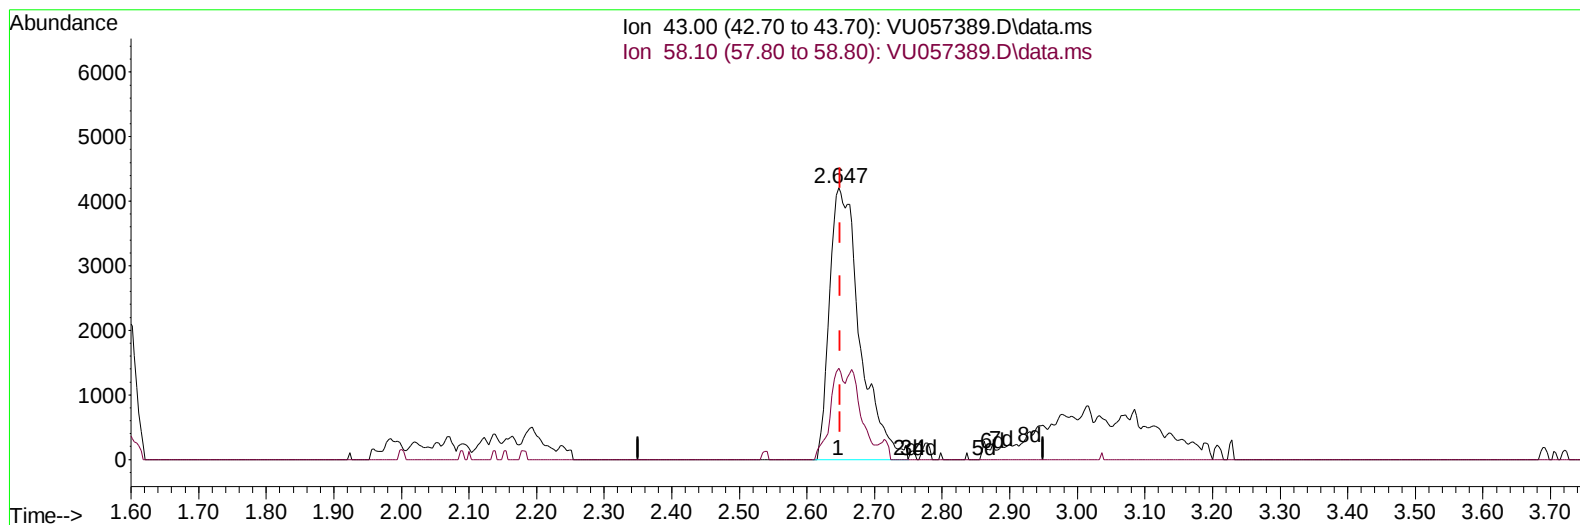

TIC: VU057389.D\data.ms

(13) Acetone (T)

2.647min (-0.003) 12.61 ug/L m

response 13145

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	32.60	16.08
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057389.D
 Acq On : 08 Jan 2024 17:55
 Operator : MD/SY
 Sample : 05787-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME6

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/09/2024
 Supervised By :Mahesh Dadoda 01/09/2024

Quant Time: Jan 09 05:05:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 09 00:42:22 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		256578	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117		253691	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		105794	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.599	65		80563	45.620	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	91.240%	
7) Chloroethane-d5	1.914	69		63038	46.128	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	92.260%	
11) 1,1-Dichloroethene-d2	2.560	63		129132	34.499	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	69.000%	
21) 2-Butanone-d5	4.634	46		90498	105.759	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	105.760%	
24) Chloroform-d	5.055	84		184620	44.210	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	88.420%	
26) 1,2-Dichloroethane-d4	5.692	65		129989	47.119	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	94.240%	
32) Benzene-d6	5.721	84		332167	48.777	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	97.560%	
36) 1,2-Dichloropropane-d6	6.685	67		91877	47.802	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	95.600%	
41) Toluene-d8	7.891	98		296095	46.398	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	92.800%	
43) trans-1,3-Dichloroprop...	8.174	79		54318	47.347	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	94.700%	
47) 2-Hexanone-d5	8.643	63		67057	106.723	ug/L	0.01
Spiked Amount 100.000	Range 45	- 130		Recovery	=	106.720%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84		134979	46.993	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	93.980%	
66) 1,2-Dichlorobenzene-d4	12.190	152		106070	51.262	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	102.520%	
Target Compounds							
13) Acetone	2.647	43		13145m	12.615	ug/L	
20) cis-1,2-Dichloroethene	4.666	96		5777	3.036	ug/L	88
34) Trichloroethene	6.541	95		4328	2.079	ug/L	90
46) Tetrachloroethene	8.547	164		188448	119.685	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057389.D
Acq On : 08 Jan 2024 17:55
Operator : MD/SY
Sample : 05787-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 3

Instrument :
MSVOA_U
ClientSampleId :
DCME6

Manual IntegrationsAPPROVED

Quant Time: Jan 09 05:05:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 09 00:42:22 2024
Response via : Initial Calibration

Reviewed By :John Carlone 01/09/2024
Supervised By :Mahesh Dadoda 01/09/2024

