




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057410.D
 Acq On : 09 Jan 2024 02:45
 Operator : MD/SY
 Sample : P1058-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YCHA3

Manual IntegrationsAPPROVED

Quant Time: Jan 09 06:28:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 09 06:09:25 2024
 Response via : Initial Calibration

Reviewed By :John Carlone 01/09/2024
 Supervised By :Mahesh Dadoda 01/09/2024

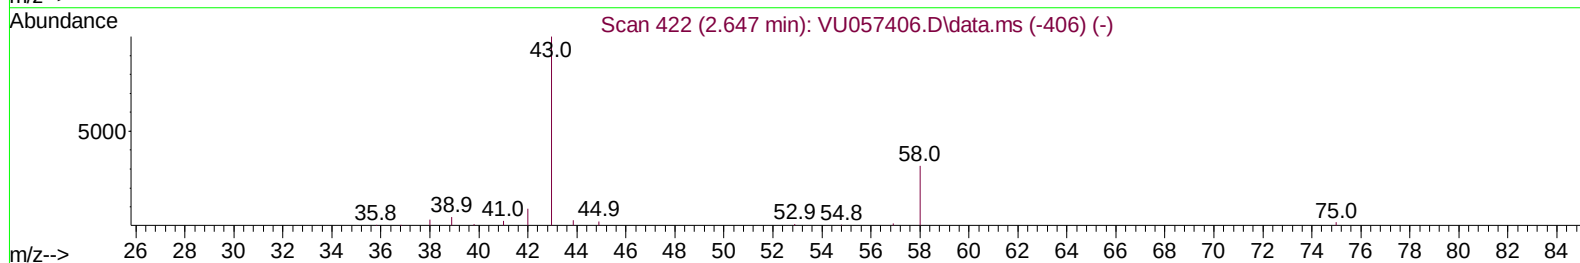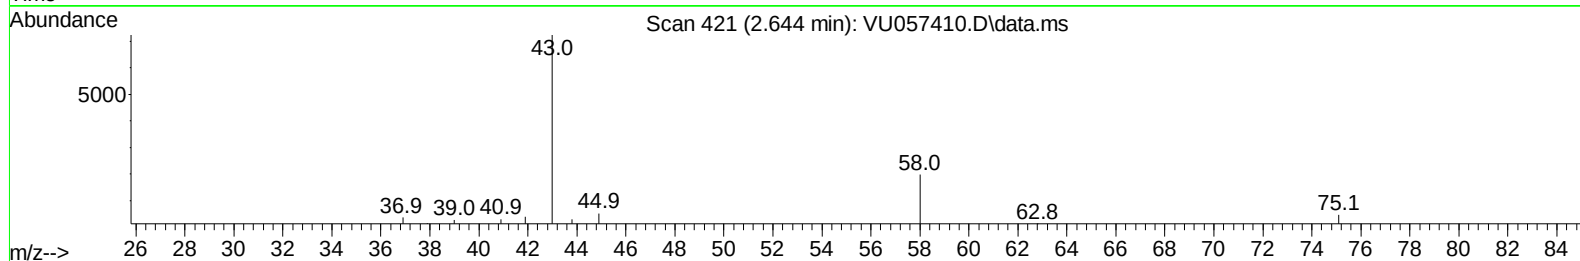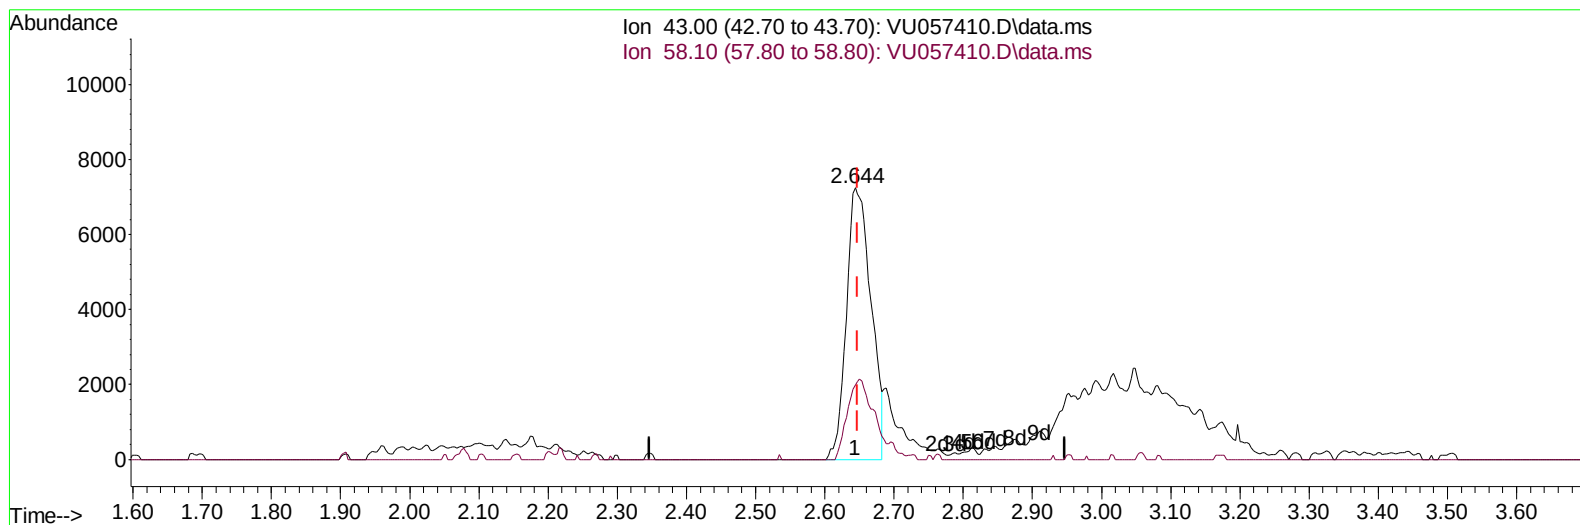

TIC: VU057410.D\data.ms

(13) Acetone (T)

2.644min (-0.003) 16.98 ug/L

response 17973

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	32.60	30.95
0.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057410.D
Acq On : 09 Jan 2024 02:45
Operator : MD/SY
Sample : P1058-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YCHA3

Manual IntegrationsAPPROVED

Quant Time: Jan 09 06:28:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 09 06:09:25 2024
Response via : Initial Calibration

Reviewed By :John Carlone 01/09/2024
Supervised By :Mahesh Dadoda 01/09/2024

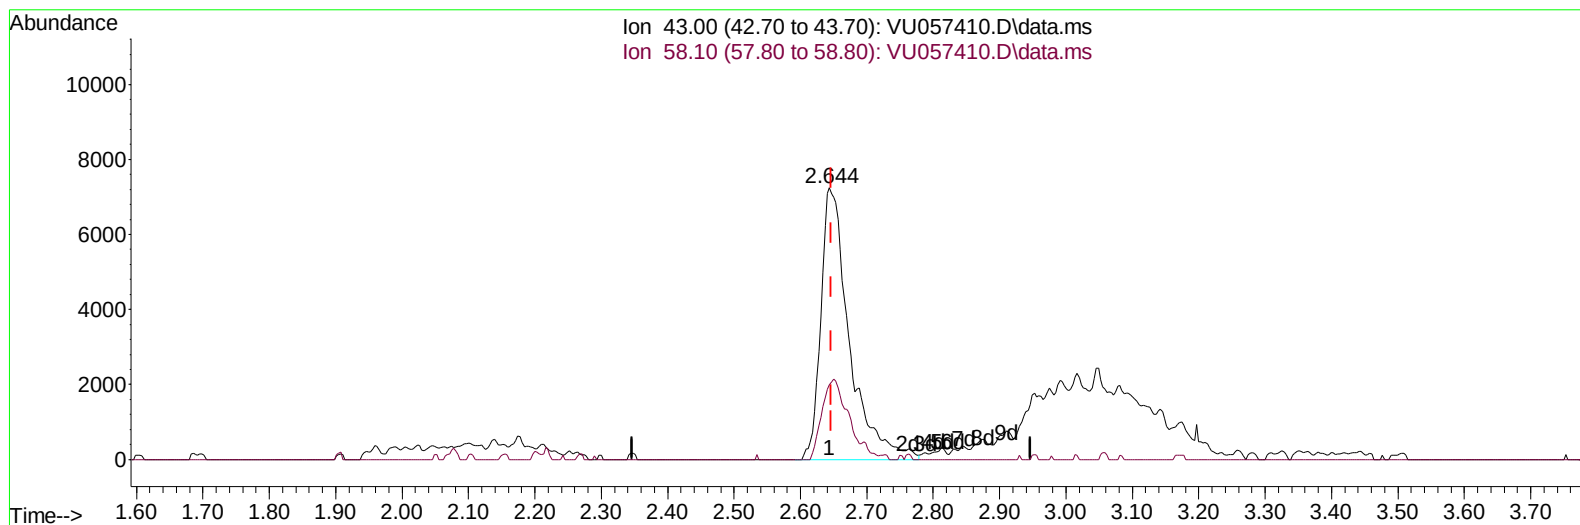




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057410.D
 Acq On : 09 Jan 2024 02:45
 Operator : MD/SY
 Sample : P1058-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YCHA3

Manual IntegrationsAPPROVED

Quant Time: Jan 09 06:28:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 09 06:09:25 2024
 Response via : Initial Calibration

Reviewed By :John Carlone 01/09/2024
 Supervised By :Mahesh Dadoda 01/09/2024

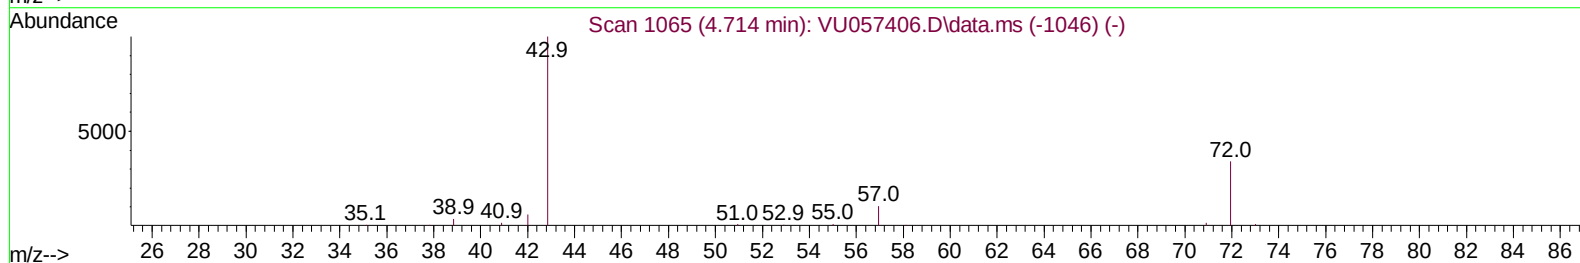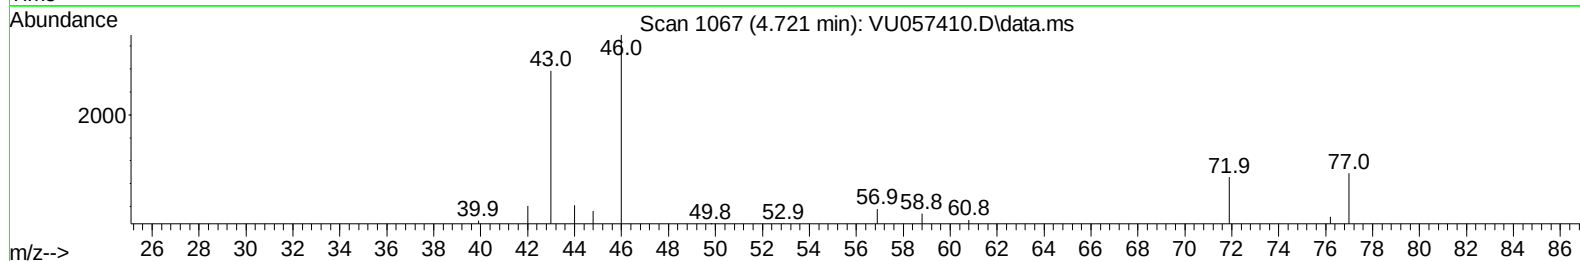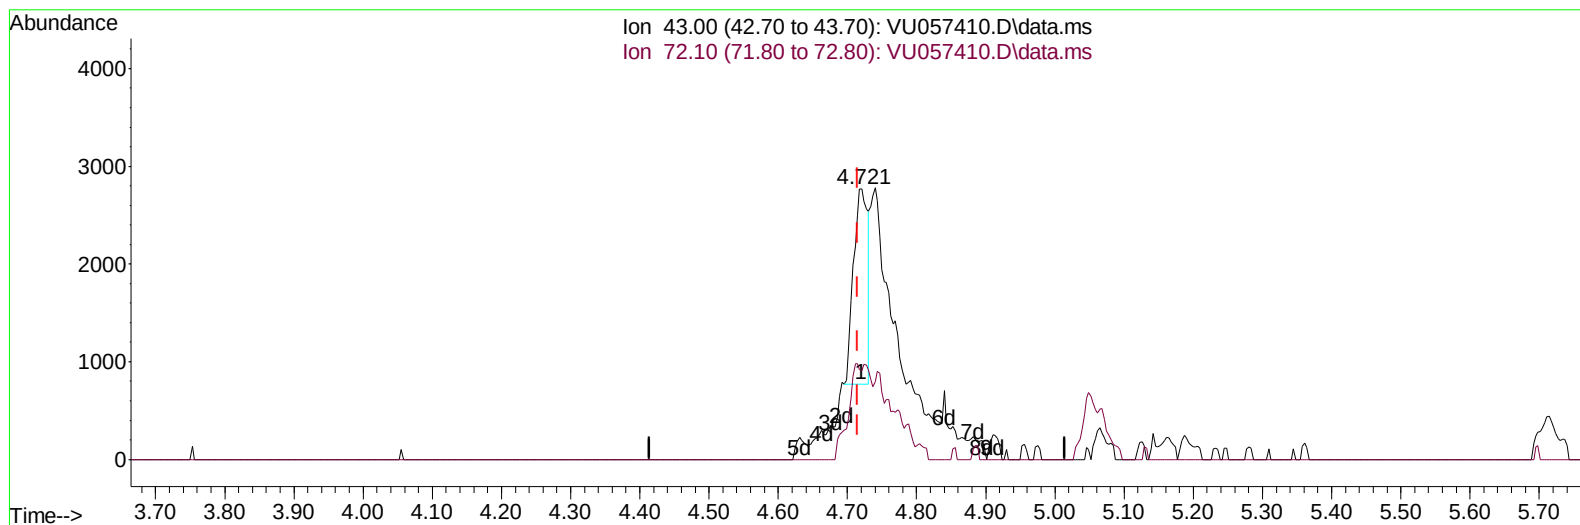

TIC: VU057410.D\data.ms

(22) 2-Butanone (T)

4.721min (+ 0.006) 2.78 ug/L

response 2897

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	30.40	46.84#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057410.D
Acq On : 09 Jan 2024 02:45
Operator : MD/SY
Sample : P1058-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YCHA3

Manual IntegrationsAPPROVED

Quant Time: Jan 09 06:28:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 09 06:09:25 2024
Response via : Initial Calibration

Reviewed By :John Carlone 01/09/2024
Supervised By :Mahesh Dadoda 01/09/2024

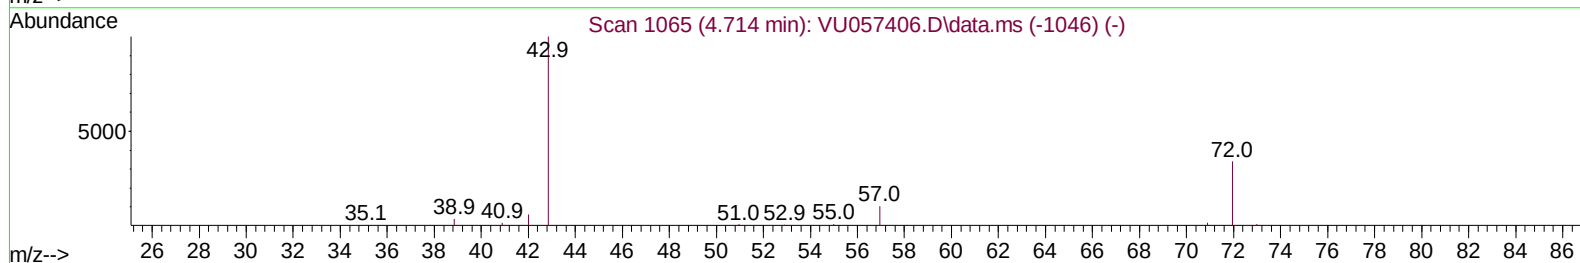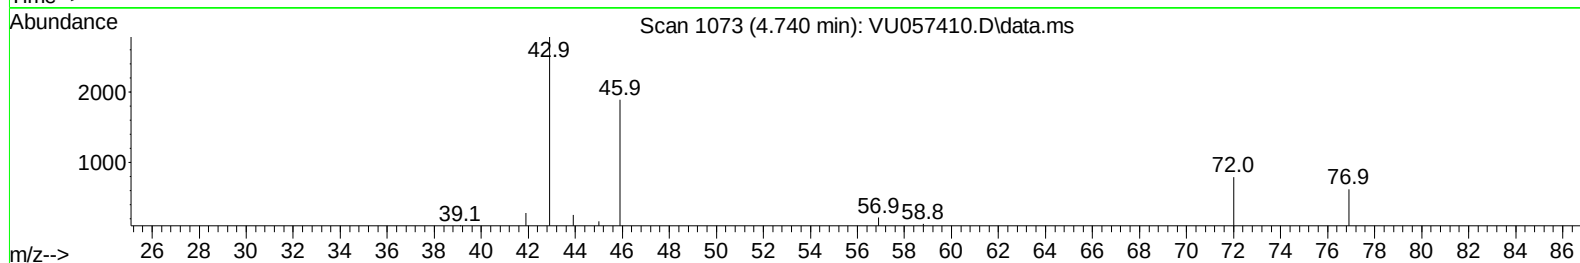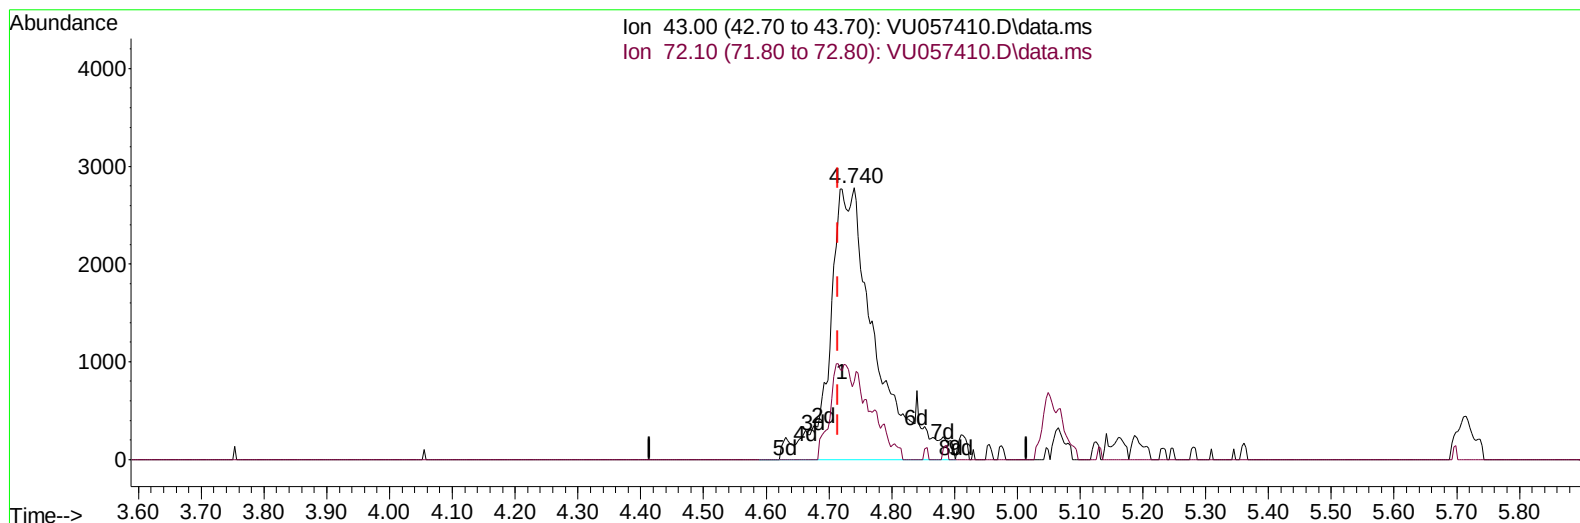

TIC: VU057410.D\data.ms

(22) 2-Butanone (T)

4.740min (+ 0.026) 13.60 ug/L m

response 14182

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	30.40	9.57#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057410.D
 Acq On : 09 Jan 2024 02:45
 Operator : MD/SY
 Sample : P1058-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YCHA3

Manual IntegrationsAPPROVED

Quant Time: Jan 09 06:28:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 09 06:09:25 2024
 Response via : Initial Calibration

Reviewed By : John Carlone 01/09/2024
 Supervised By : Mahesh Dadoda 01/09/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	260566	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	252492	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	106112	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	76335	42.565	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	85.120%	
7) Chloroethane-d5	1.911	69	60065	43.280	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	86.560%	
11) 1,1-Dichloroethene-d2	2.557	63	136026	35.785	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	71.560%	
21) 2-Butanone-d5	4.634	46	86709	99.780	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	99.780%	
24) Chloroform-d	5.052	84	182418	43.014	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	86.020%	
26) 1,2-Dichloroethane-d4	5.692	65	130613	46.620	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	93.240%	
32) Benzene-d6	5.718	84	325066	47.961	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.920%	
36) 1,2-Dichloropropane-d6	6.682	67	93603	48.931	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	97.860%	
41) Toluene-d8	7.891	98	294095	46.304	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	92.600%	
43) trans-1,3-Dichloroprop...	8.174	79	53564	46.912	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	93.820%	
47) 2-Hexanone-d5	8.647	63	66164	105.802	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	105.800%	
56) 1,1,2,2-Tetrachloroeth...	10.756	84	132985	46.519	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	93.040%	
66) 1,2-Dichlorobenzene-d4	12.190	152	103165	49.708	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	99.420%	
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.570	96	24700	13.990	ug/L #	34
13) Acetone	2.644	43	21568m	20.381	ug/L	
19) 1,1-Dichloroethane	3.859	63	12858	3.845	ug/L	99
20) cis-1,2-Dichloroethene	4.660	96	5983	3.097	ug/L	92
22) 2-Butanone	4.740	43	14182m	13.601	ug/L	
30) 1,1,1-Trichloroethane	5.306	97	5174	1.332	ug/L #	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057410.D
Acq On : 09 Jan 2024 02:45
Operator : MD/SY
Sample : P1058-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YCHA3

Manual IntegrationsAPPROVED

Quant Time: Jan 09 06:28:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 09 06:09:25 2024
Response via : Initial Calibration

Reviewed By :John Carlone 01/09/2024
Supervised By :Mahesh Dadoda 01/09/2024

