




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057411.D
Acq On : 09 Jan 2024 03:10
Operator : MD/SY
Sample : P1058-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YCHA4

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/09/2024
Supervised By :Mahesh Dadoda 01/09/2024

Quant Time: Jan 09 06:28:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 09 06:09:25 2024
Response via : Initial Calibration

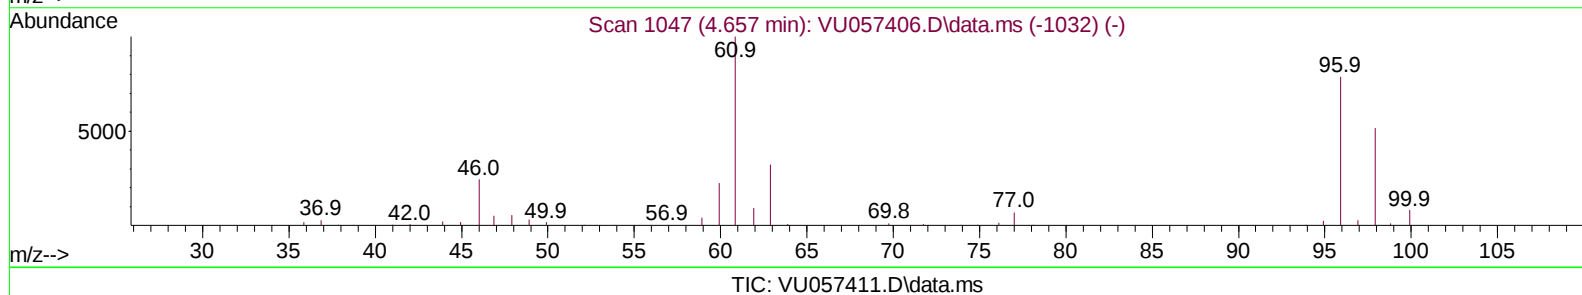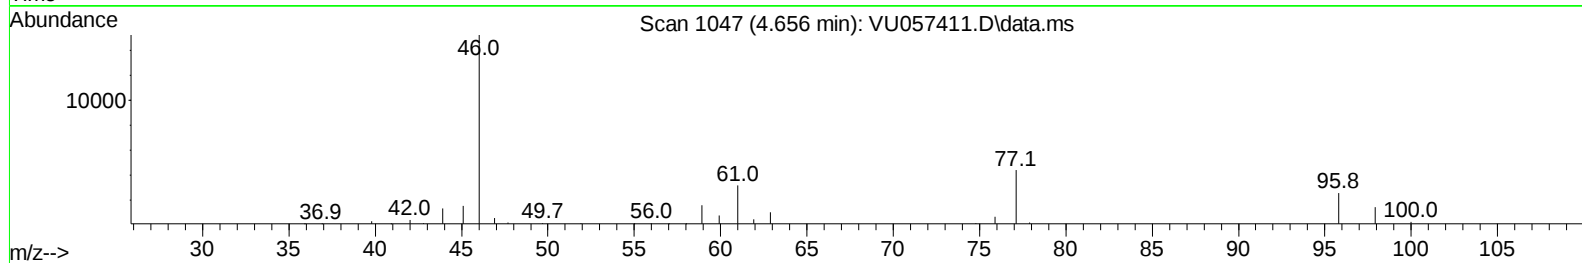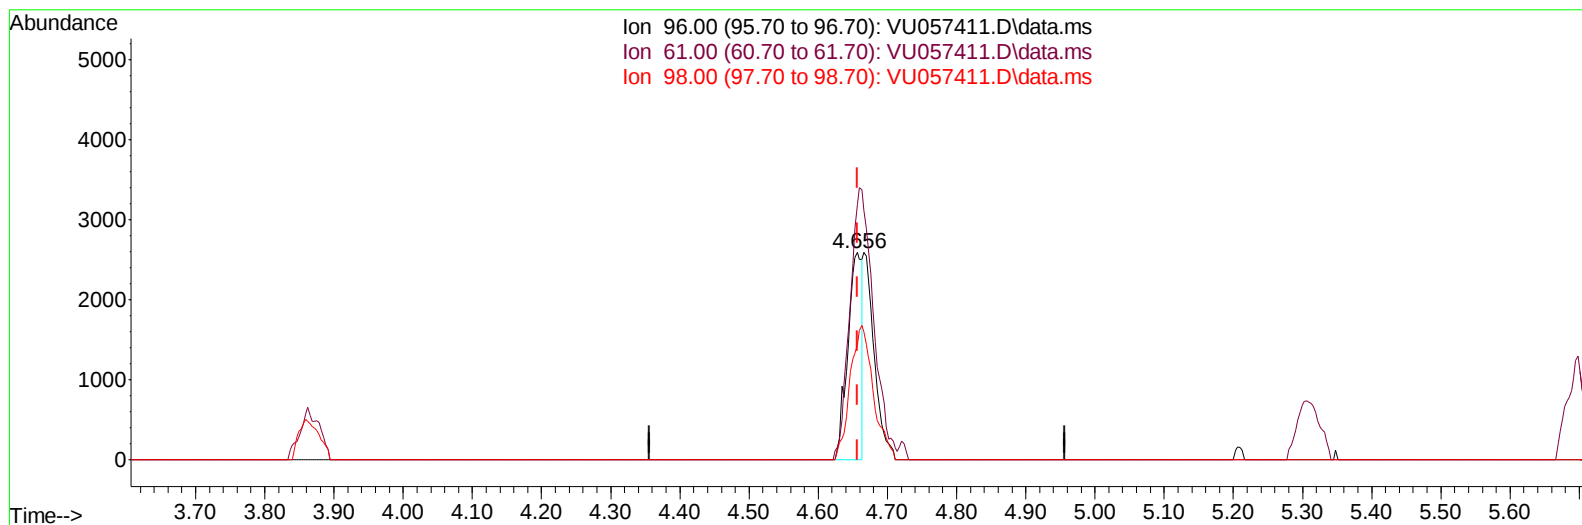**(20) cis-1,2-Dichloroethene (T)**

4.656min (-0.000) 1.84 ug/L

response 3669

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	125.70	123.09
98.00	62.00	55.64
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057411.D
Acq On : 09 Jan 2024 03:10
Operator : MD/SY
Sample : P1058-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YCHA4

Manual IntegrationsAPPROVED

Quant Time: Jan 09 06:28:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 09 06:09:25 2024
Response via : Initial Calibration

Reviewed By :John Carlone 01/09/2024
Supervised By :Mahesh Dadoda 01/09/2024

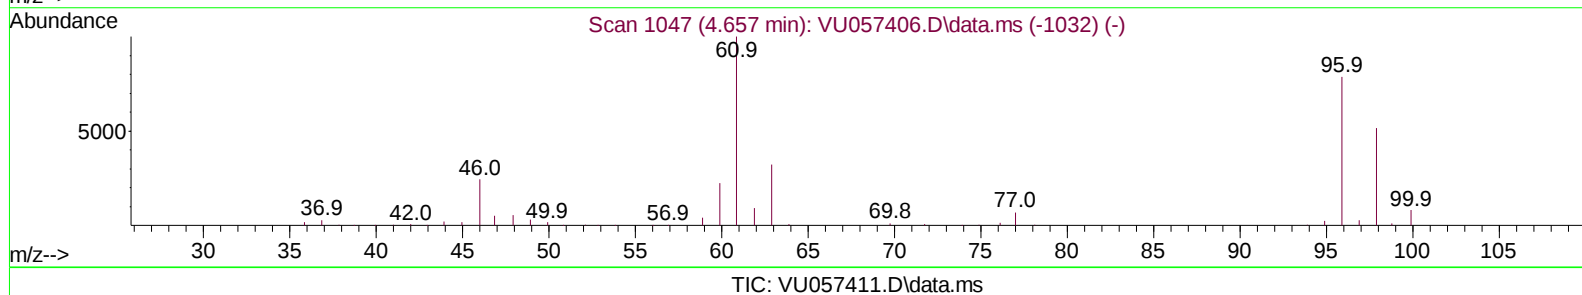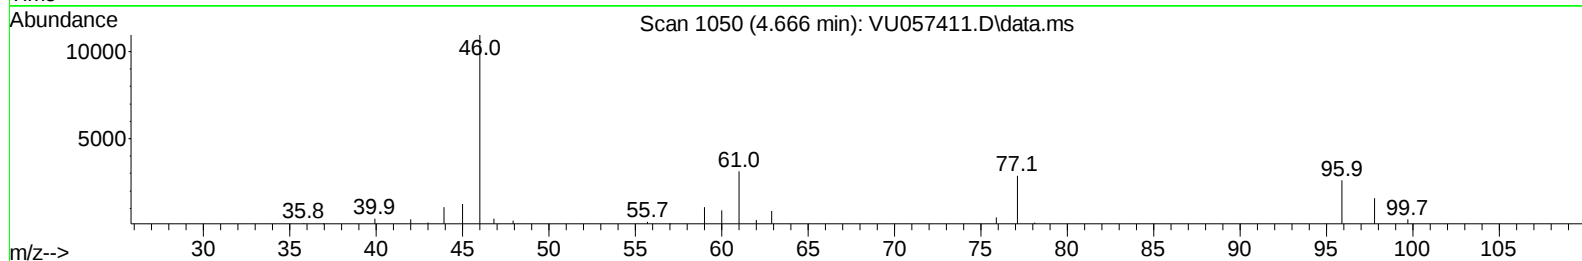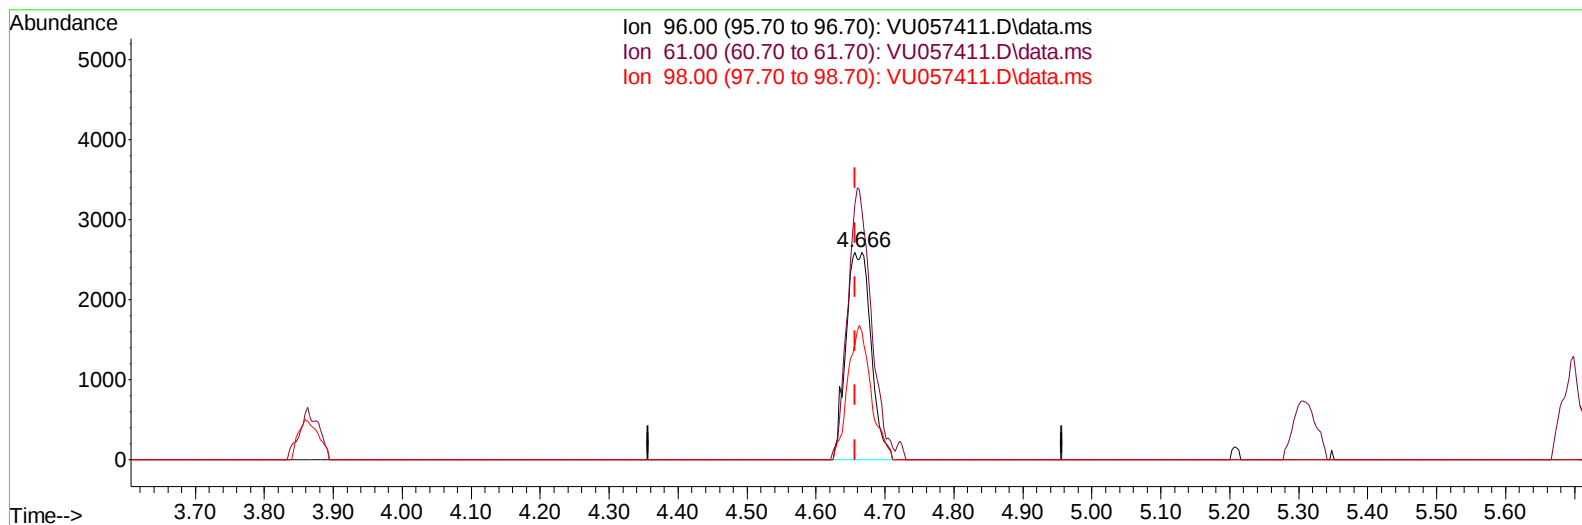

(20) cis-1,2-Dichloroethene (T)

4.666min (+ 0.010) 3.28 ug/L m

response 6544

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	125.70	120.22
98.00	62.00	61.54
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057411.D
 Acq On : 09 Jan 2024 03:10
 Operator : MD/SY
 Sample : P1058-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YCHA4

Manual IntegrationsAPPROVED

Quant Time: Jan 09 06:28:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 09 06:09:25 2024
 Response via : Initial Calibration

Reviewed By :John Carlone 01/09/2024
 Supervised By :Mahesh Dadoda 01/09/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	269359	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	253463	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	104886	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	78472	42.328	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	84.660%	
7) Chloroethane-d5	1.914	69	63754	44.438	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	88.880%	
11) 1,1-Dichloroethene-d2	2.560	63	140654	35.794	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	71.580%	
21) 2-Butanone-d5	4.634	46	87522	97.428	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	97.430%	
24) Chloroform-d	5.055	84	188668	43.035	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	86.080%	
26) 1,2-Dichloroethane-d4	5.692	65	132498	45.749	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.500%	
32) Benzene-d6	5.721	84	331024	48.653	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.300%	
36) 1,2-Dichloropropane-d6	6.682	67	93625	48.755	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	97.520%	
41) Toluene-d8	7.891	98	293674	46.060	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	92.120%	
43) trans-1,3-Dichloroprop...	8.174	79	51952	45.325	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	90.660%	
47) 2-Hexanone-d5	8.637	63	63063	100.457	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	100.460%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	133390	46.482	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	92.960%	
66) 1,2-Dichlorobenzene-d4	12.190	152	103064	50.240	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	100.480%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.605	62	6610	3.202	ug/L #	80
12) 1,1-Dichloroethene	2.573	96	24372	13.354	ug/L #	14
13) Acetone	2.644	43	44603	40.772	ug/L	91
19) 1,1-Dichloroethane	3.859	63	15218	4.402	ug/L	94
20) cis-1,2-Dichloroethene	4.666	96	6544m	3.276	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057411.D
Acq On : 09 Jan 2024 03:10
Operator : MD/SY
Sample : P1058-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YCHA4

Manual IntegrationsAPPROVED

Quant Time: Jan 09 06:28:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 09 06:09:25 2024
Response via : Initial Calibration

Reviewed By :John Carlone 01/09/2024
Supervised By :Mahesh Dadoda 01/09/2024

