

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057384.D
 Acq On : 08 Jan 2024 15:55
 Operator : MD/SY
 Sample : 05787-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

Signal : TIC: VU057384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	109	rVB	109213	128907	13.72%	1.813%
2	1.914	185	194	207	rBV	79941	112278	11.95%	1.579%
3	2.264	301	303	305	rBV2	500	234	0.02%	0.003%
4	2.563	384	396	414	rBV	202776	336826	35.85%	4.736%
5	2.917	503	506	508	rBV	278	188	0.02%	0.003%
6	2.956	513	518	522	rVB2	334	306	0.03%	0.004%
7	2.988	525	528	531	rBV2	521	387	0.04%	0.005%
8	3.046	539	546	551	rVB2	1255	1579	0.17%	0.022%
9	3.087	555	559	562	rBV	333	290	0.03%	0.004%
10	3.174	575	586	592	rBV5	2302	4713	0.50%	0.066%
11	3.338	634	637	639	rVV2	290	198	0.02%	0.003%
12	3.425	659	664	667	rBB2	299	241	0.03%	0.003%
13	3.444	667	670	673	rBB	221	168	0.02%	0.002%
14	3.611	718	722	727	rBB	175	221	0.02%	0.003%
15	3.714	751	754	759	rBB2	338	289	0.03%	0.004%
16	3.743	760	763	765	rBV	253	162	0.02%	0.002%
17	3.875	801	804	808	rBB2	324	187	0.02%	0.003%
18	4.065	860	863	869	rBB	215	219	0.02%	0.003%
19	4.348	949	951	956	rVB2	284	254	0.03%	0.004%
20	4.563	1014	1018	1021	rBB	221	194	0.02%	0.003%
21	4.637	1030	1041	1072	rBV	47810	148748	15.83%	2.091%
22	5.055	1152	1171	1199	rBV	180169	410747	43.72%	5.775%
23	5.245	1227	1230	1232	rBV	386	205	0.02%	0.003%
24	5.328	1253	1256	1262	rBB2	410	345	0.04%	0.005%
25	5.354	1262	1264	1268	rBB	281	168	0.02%	0.002%
26	5.409	1277	1281	1283	rBB2	312	203	0.02%	0.003%
27	5.521	1313	1316	1318	rVB	305	180	0.02%	0.003%
28	5.537	1318	1321	1323	rBB	266	164	0.02%	0.002%
29	5.717	1357	1377	1401	rBV2	341804	939558	100.00%	13.211%
30	5.920	1437	1440	1442	rBV2	302	209	0.02%	0.003%
31	5.978	1456	1458	1461	rVB	417	198	0.02%	0.003%
32	6.126	1502	1504	1506	rVB	461	221	0.02%	0.003%
33	6.245	1528	1541	1567	rBV	314999	609295	64.85%	8.567%
34	6.531	1623	1630	1631	rBV4	1047	940	0.10%	0.013%
35	6.621	1654	1658	1663	rBB	205	225	0.02%	0.003%
36	6.685	1664	1678	1698	rBV	206081	403968	43.00%	5.680%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057384.D
 Acq On : 08 Jan 2024 15:55
 Operator : MD/SY
 Sample : 05787-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

37	6.888	1739	1741	1744	rVB	266	166	0.02%	0.002%
38	6.994	1768	1774	1776	rBB	307	326	0.03%	0.005%
39	7.090	1801	1804	1807	rBB2	305	206	0.02%	0.003%
40	7.190	1828	1835	1837	rBV2	658	648	0.07%	0.009%
41	7.242	1847	1851	1854	rBV	312	250	0.03%	0.004%
42	7.261	1854	1857	1861	rVB	367	327	0.03%	0.005%
43	7.299	1865	1869	1870	rBV	251	172	0.02%	0.002%
44	7.467	1919	1921	1924	rBB2	282	172	0.02%	0.002%
45	7.560	1938	1950	1972	rBV2	114110	206030	21.93%	2.897%
46	7.669	1981	1984	1987	rVB	423	291	0.03%	0.004%
47	7.714	1995	1998	2001	rBV	506	397	0.04%	0.006%
48	7.804	2021	2026	2028	rBV2	403	363	0.04%	0.005%
49	7.846	2034	2039	2041	rBV2	302	279	0.03%	0.004%
50	7.894	2041	2054	2083	rBV	406060	732377	77.95%	10.298%
51	8.174	2131	2141	2162	rBV	82682	148597	15.82%	2.089%
52	8.303	2179	2181	2183	rVV	346	167	0.02%	0.002%
53	8.422	2215	2218	2221	rBV	293	201	0.02%	0.003%
54	8.441	2221	2224	2226	rVV	225	173	0.02%	0.002%
55	8.463	2226	2231	2235	rVV2	775	763	0.08%	0.011%
56	8.483	2235	2237	2241	rVB2	579	324	0.03%	0.005%
57	8.637	2274	2285	2316	rBV2	167563	372186	39.61%	5.233%
58	8.804	2335	2337	2345	rVB4	579	560	0.06%	0.008%
59	8.991	2389	2395	2397	rBV	348	287	0.03%	0.004%
60	9.315	2492	2496	2500	rBB	248	236	0.03%	0.003%
61	9.344	2501	2505	2508	rBB	199	178	0.02%	0.003%
62	9.412	2513	2526	2559	rBV	425767	739161	78.67%	10.393%
63	9.695	2609	2614	2618	rBV2	446	541	0.06%	0.008%
64	9.817	2649	2652	2659	rVB	286	226	0.02%	0.003%
65	9.913	2679	2682	2685	rBB	275	186	0.02%	0.003%
66	9.936	2685	2689	2695	rBV2	363	432	0.05%	0.006%
67	10.036	2717	2720	2725	rBV	224	243	0.03%	0.003%
68	10.122	2744	2747	2758	rVV3	554	738	0.08%	0.010%
69	10.232	2777	2781	2787	rBB	210	287	0.03%	0.004%
70	10.328	2804	2811	2814	rBV	469	407	0.04%	0.006%
71	10.428	2838	2842	2846	rBV	520	439	0.05%	0.006%
72	10.483	2856	2859	2865	rVB	965	885	0.09%	0.012%
73	10.511	2865	2868	2870	rBV	493	317	0.03%	0.004%
74	10.579	2886	2889	2891	rBV	366	255	0.03%	0.004%
75	10.753	2930	2943	2963	rVV	281644	464460	49.43%	6.531%
76	10.823	2963	2965	2968	rVV2	398	221	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057384.D
 Acq On : 08 Jan 2024 15:55
 Operator : MD/SY
 Sample : 05787-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

77	10.843	2969	2971	2973	rVB	416	185	0.02%	0.003%
78	10.888	2978	2985	2995	rVB4	2696	3794	0.40%	0.053%
79	10.962	3004	3008	3011	rBV	245	259	0.03%	0.004%
80	11.048	3031	3035	3038	rBB	182	185	0.02%	0.003%
81	11.090	3044	3048	3049	rBV	594	381	0.04%	0.005%
82	11.183	3075	3077	3082	rBV	267	261	0.03%	0.004%
83	11.299	3110	3113	3115	rBV	319	208	0.02%	0.003%
84	11.466	3159	3165	3173	rBV2	1027	1306	0.14%	0.018%
85	11.521	3180	3182	3185	rBV	277	161	0.02%	0.002%
86	11.749	3245	3253	3259	rBV4	1493	2131	0.23%	0.030%
87	11.807	3259	3271	3292	rBV	400038	647798	68.95%	9.108%
88	11.962	3317	3319	3325	rBV2	351	276	0.03%	0.004%
89	12.187	3377	3389	3415	rBV	402812	647920	68.96%	9.110%
90	12.476	3475	3479	3485	rVB2	317	327	0.03%	0.005%
91	12.762	3561	3568	3569	rBV2	1292	1168	0.12%	0.016%
92	12.862	3595	3599	3607	rVB2	586	520	0.06%	0.007%
93	13.013	3643	3646	3650	rBV	299	195	0.02%	0.003%
94	13.634	3835	3839	3844	rBV2	350	384	0.04%	0.005%
95	13.843	3896	3904	3915	rVB5	5262	7862	0.84%	0.111%
96	14.093	3974	3982	3996	rBV4	5256	9306	0.99%	0.131%
97	14.331	4049	4056	4066	rVB4	5771	8295	0.88%	0.117%
98	14.904	4230	4234	4236	rBV2	486	412	0.04%	0.006%
99	15.103	4292	4296	4300	rBV2	502	606	0.06%	0.009%
100	15.624	4456	4458	4461	rBV2	820	448	0.05%	0.006%




Sum of corrected areas: 7112077

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057384.D
Acq On : 08 Jan 2024 15:55
Operator : MD/SY
Sample : 05787-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

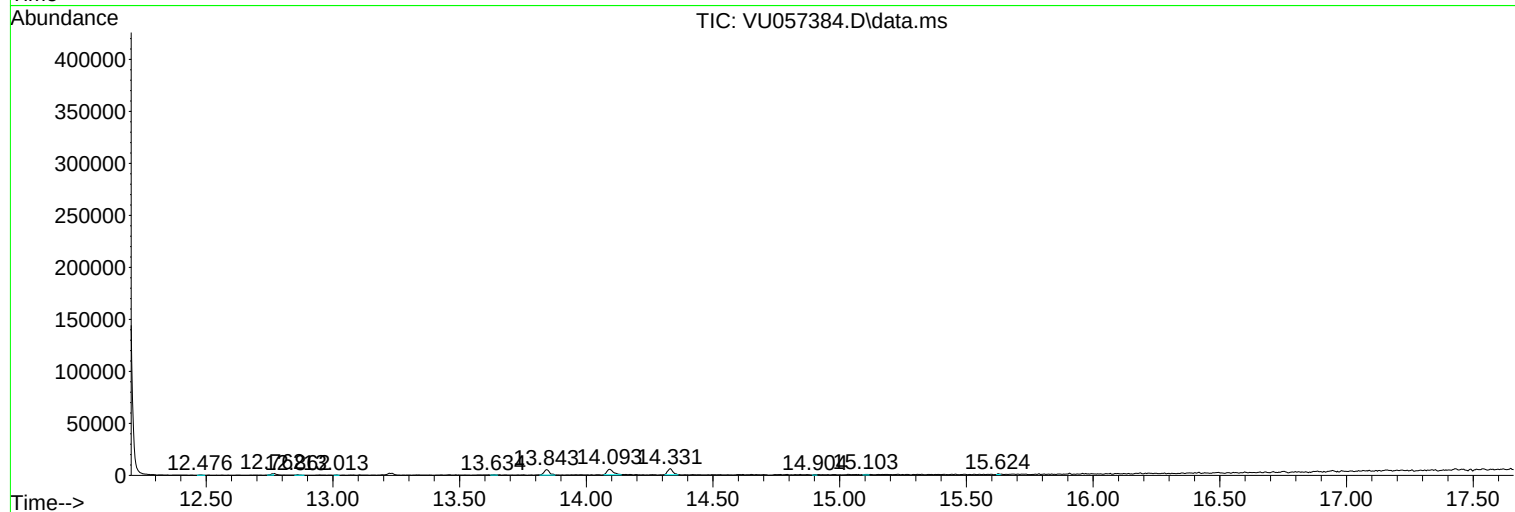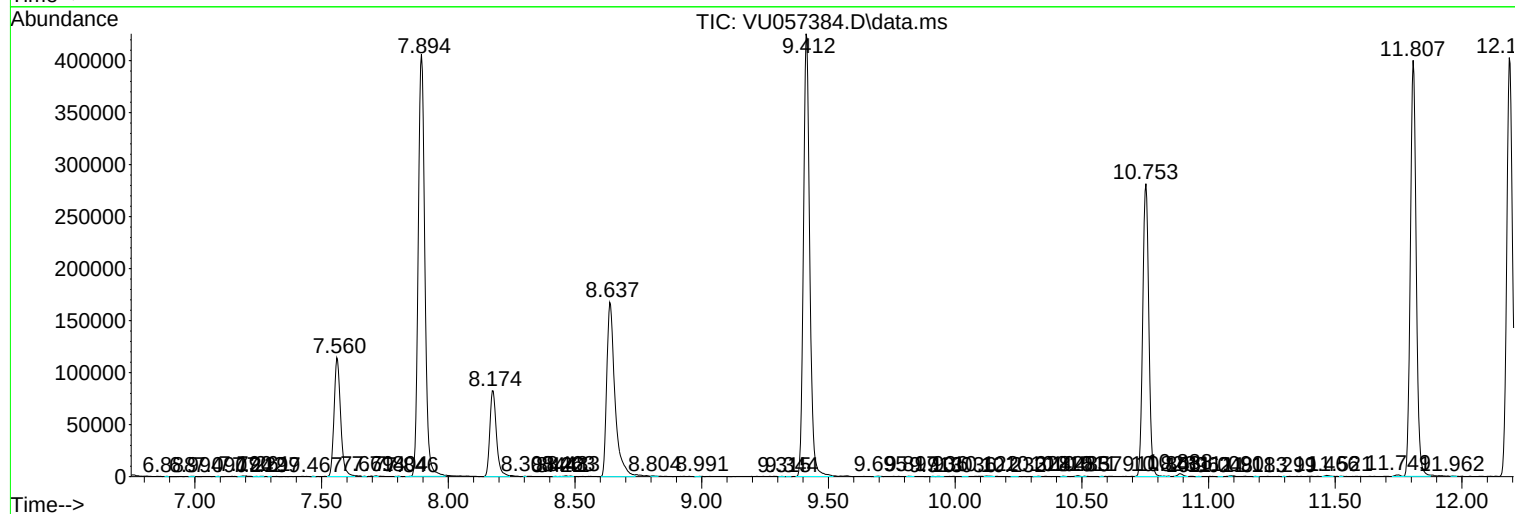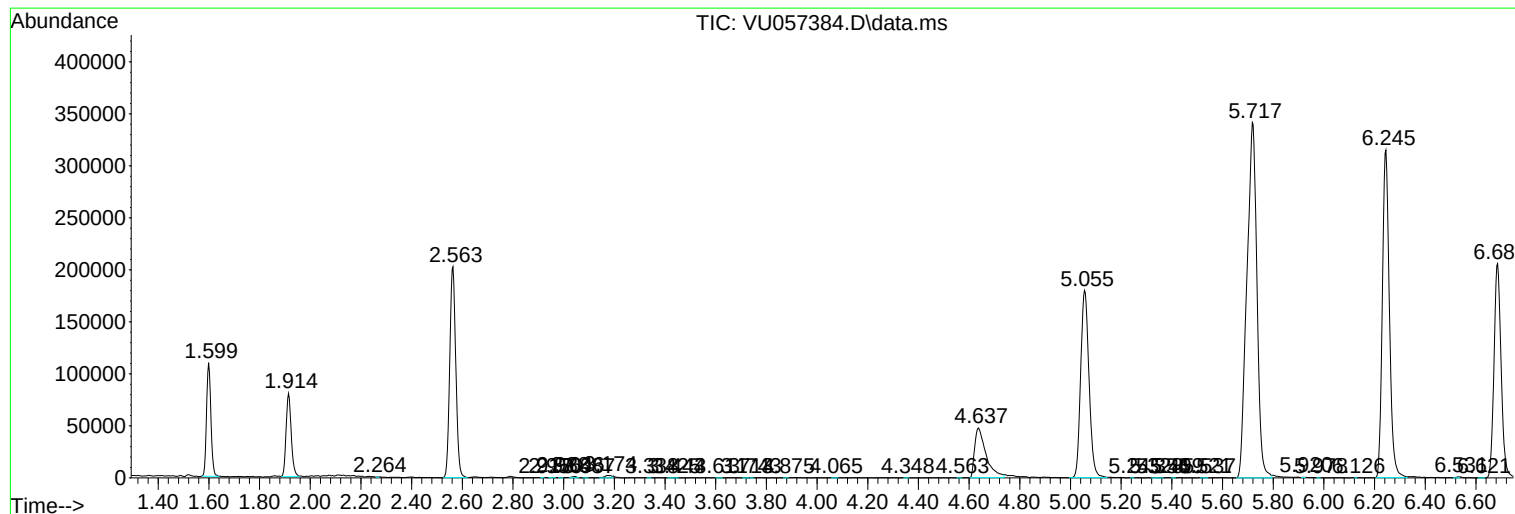

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057384.D
Acq On : 08 Jan 2024 15:55
Operator : MD/SY
Sample : 05787-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057384.D
Acq On : 08 Jan 2024 15:55
Operator : MD/SY
Sample : 05787-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------