

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057390.D
 Acq On : 08 Jan 2024 18:19
 Operator : MD/SY
 Sample : 05787-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

Signal : TIC: VU057390.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.357	15	21	32	rBV	17326	19941	1.45%	0.221%
2	1.599	87	96	112	rVB	115536	147311	10.69%	1.634%
3	1.914	185	194	209	rBV	77843	117356	8.52%	1.302%
4	2.554	380	393	412	rBV	217867	357032	25.91%	3.961%
5	2.779	456	463	469	rBV3	734	1181	0.09%	0.013%
6	2.846	478	484	486	rBV3	482	546	0.04%	0.006%
7	2.917	504	506	510	rVB3	513	280	0.02%	0.003%
8	2.959	517	519	521	rBV2	651	344	0.02%	0.004%
9	3.419	659	662	665	rBV	295	256	0.02%	0.003%
10	3.451	669	672	674	rBV	229	190	0.01%	0.002%
11	3.640	728	731	735	rBB	187	169	0.01%	0.002%
12	3.689	743	746	750	rBB2	380	207	0.02%	0.002%
13	3.724	755	757	762	rVB	217	199	0.01%	0.002%
14	3.843	783	794	796	rBV5	2595	4001	0.29%	0.044%
15	4.435	973	978	984	rBB2	353	437	0.03%	0.005%
16	4.483	990	993	996	rBV	388	247	0.02%	0.003%
17	4.560	1011	1017	1019	rBB	286	229	0.02%	0.003%
18	4.589	1020	1026	1029	rBV	166	219	0.02%	0.002%
19	4.644	1030	1043	1066	rBV2	47212	171045	12.41%	1.898%
20	4.952	1136	1139	1142	rBV3	677	498	0.04%	0.006%
21	5.055	1152	1171	1193	rBV	196026	443590	32.19%	4.922%
22	5.206	1214	1218	1223	rBV4	484	409	0.03%	0.005%
23	5.242	1226	1229	1233	rVB2	346	271	0.02%	0.003%
24	5.280	1239	1241	1246	rVB3	473	350	0.03%	0.004%
25	5.341	1257	1260	1264	rBB	473	337	0.02%	0.004%
26	5.624	1344	1348	1352	rBB	242	271	0.02%	0.003%
27	5.717	1355	1377	1404	rBV2	371884	1019658	73.99%	11.313%
28	5.910	1435	1437	1440	rVB2	480	273	0.02%	0.003%
29	5.936	1440	1445	1448	rVB4	686	644	0.05%	0.007%
30	5.962	1449	1453	1456	rBV2	451	411	0.03%	0.005%
31	5.984	1456	1460	1465	rVB2	331	187	0.01%	0.002%
32	6.007	1465	1467	1470	rVB	339	187	0.01%	0.002%
33	6.033	1471	1475	1476	rBV	396	282	0.02%	0.003%
34	6.097	1492	1495	1498	rBV	202	187	0.01%	0.002%
35	6.242	1525	1540	1564	rBV2	331212	650139	47.18%	7.213%
36	6.383	1580	1584	1586	rBV	379	253	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057390.D
 Acq On : 08 Jan 2024 18:19
 Operator : MD/SY
 Sample : 05787-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

37	6.457	1602	1607	1611	rVB2	339	243	0.02%	0.003%
38	6.496	1617	1619	1622	rVB2	344	210	0.02%	0.002%
39	6.537	1622	1632	1647	rBV4	12348	23560	1.71%	0.261%
40	6.618	1655	1657	1660	rVB2	338	179	0.01%	0.002%
41	6.682	1664	1677	1701	rBV	220200	432295	31.37%	4.796%
42	6.804	1712	1715	1721	rVB2	935	874	0.06%	0.010%
43	7.193	1831	1836	1842	rBV4	743	1025	0.07%	0.011%
44	7.560	1939	1950	1976	rBV2	120256	229503	16.65%	2.546%
45	7.676	1983	1986	1989	rBV	248	173	0.01%	0.002%
46	7.695	1989	1992	1994	rVV4	457	317	0.02%	0.004%
47	7.756	2009	2011	2014	rBB	283	169	0.01%	0.002%
48	7.891	2041	2053	2089	rBV	439760	802205	58.21%	8.900%
49	8.177	2130	2142	2164	rBV	80726	165658	12.02%	1.838%
50	8.489	2237	2239	2243	rVB	315	174	0.01%	0.002%
51	8.547	2244	2257	2276	rBV	809030	1378041	100.00%	15.289%
52	8.653	2277	2290	2321	rVB2	170402	402047	29.18%	4.461%
53	8.878	2357	2360	2365	rVB2	450	388	0.03%	0.004%
54	8.907	2365	2369	2371	rBV	247	213	0.02%	0.002%
55	9.007	2398	2400	2404	rBV	169	170	0.01%	0.002%
56	9.087	2422	2425	2428	rVV2	292	239	0.02%	0.003%
57	9.145	2439	2443	2448	rBB	154	170	0.01%	0.002%
58	9.171	2449	2451	2453	rBV	296	174	0.01%	0.002%
59	9.203	2458	2461	2466	rVB	437	357	0.03%	0.004%
60	9.254	2471	2477	2479	rBV	207	260	0.02%	0.003%
61	9.293	2485	2489	2493	rBV	397	389	0.03%	0.004%
62	9.415	2514	2527	2554	rBV2	428378	795683	57.74%	8.828%
63	9.685	2607	2611	2612	rBV	577	350	0.03%	0.004%
64	9.730	2622	2625	2627	rBV	352	225	0.02%	0.002%
65	9.958	2691	2696	2699	rBV	207	236	0.02%	0.003%
66	10.110	2738	2743	2745	rVB2	284	213	0.02%	0.002%
67	10.142	2750	2753	2759	rBV2	384	410	0.03%	0.005%
68	10.206	2770	2773	2777	rBB2	319	272	0.02%	0.003%
69	10.229	2777	2780	2783	rBV	246	199	0.01%	0.002%
70	10.325	2804	2810	2815	rBV	298	433	0.03%	0.005%
71	10.679	2914	2920	2923	rBV	263	318	0.02%	0.004%
72	10.756	2931	2944	2964	rBV	299266	488441	35.44%	5.419%
73	10.888	2980	2985	2986	rBV2	627	499	0.04%	0.006%
74	10.933	2994	2999	3001	rBV	211	243	0.02%	0.003%
75	11.203	3079	3083	3085	rBV	294	237	0.02%	0.003%
76	11.228	3089	3091	3094	rVB	358	230	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057390.D
 Acq On : 08 Jan 2024 18:19
 Operator : MD/SY
 Sample : 05787-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

77	11.251	3094	3098	3100	rBV	186	185	0.01%	0.002%
78	11.264	3100	3102	3109	rVB	398	355	0.03%	0.004%
79	11.376	3133	3137	3140	rBV	234	227	0.02%	0.003%
80	11.473	3163	3167	3172	rVB	421	354	0.03%	0.004%
81	11.611	3207	3210	3214	rBV	270	231	0.02%	0.003%
82	11.749	3248	3253	3259	rBV3	758	900	0.07%	0.010%
83	11.810	3259	3272	3299	rBV	414313	658627	47.79%	7.307%
84	12.084	3355	3357	3363	rVB2	466	476	0.03%	0.005%
85	12.113	3363	3366	3369	rBV	501	306	0.02%	0.003%
86	12.190	3377	3390	3413	rBV	413733	681569	49.46%	7.562%
87	12.325	3429	3432	3435	rBV2	268	169	0.01%	0.002%
88	12.399	3452	3455	3460	rVV	365	206	0.01%	0.002%
89	12.759	3563	3567	3568	rBV2	736	564	0.04%	0.006%
90	12.955	3626	3628	3634	rVB	342	217	0.02%	0.002%
91	13.142	3683	3686	3688	rBV	287	203	0.01%	0.002%
92	13.524	3803	3805	3809	rVB	372	225	0.02%	0.002%
93	13.926	3928	3930	3931	rBV	532	226	0.02%	0.003%
94	13.958	3936	3940	3942	rBV2	353	234	0.02%	0.003%
95	14.277	4037	4039	4041	rBV	337	182	0.01%	0.002%
96	14.476	4098	4101	4102	rBV2	517	277	0.02%	0.003%
97	14.524	4110	4116	4119	rBV2	382	486	0.04%	0.005%
98	15.051	4278	4280	4282	rBV	436	248	0.02%	0.003%
99	15.096	4292	4294	4296	rBV2	347	197	0.01%	0.002%
100	15.318	4361	4363	4365	rBV	637	219	0.02%	0.002%




Sum of corrected areas: 9013042

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057390.D
Acq On : 08 Jan 2024 18:19
Operator : MD/SY
Sample : 05787-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

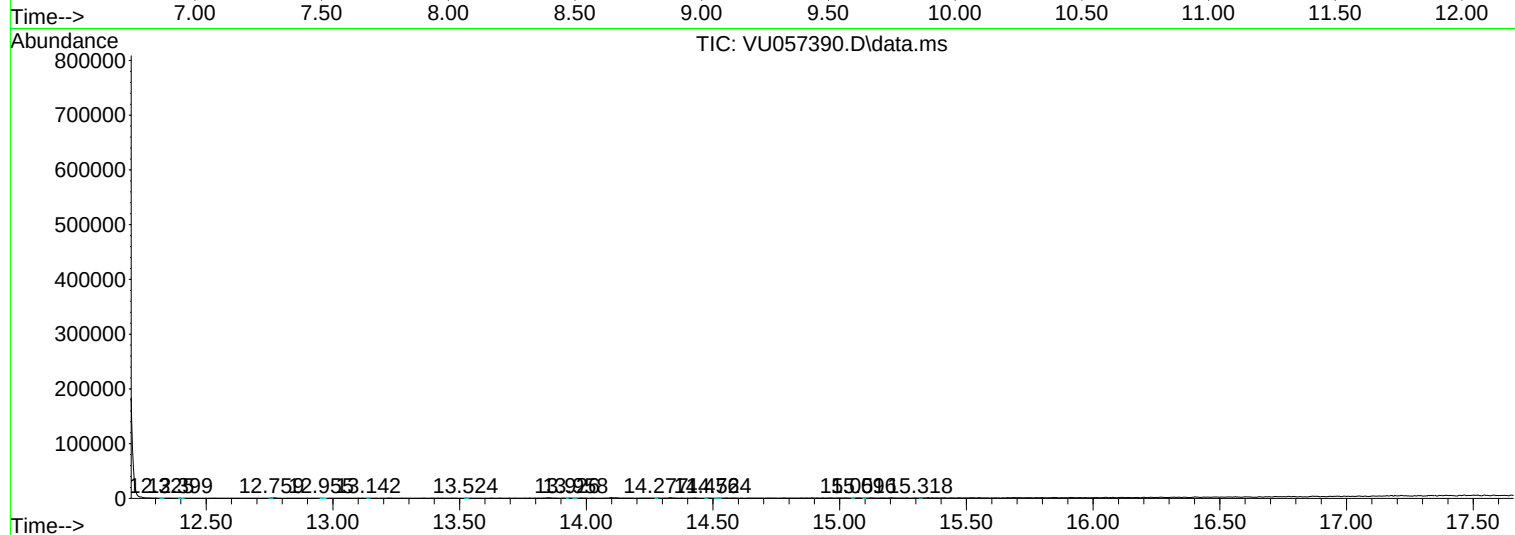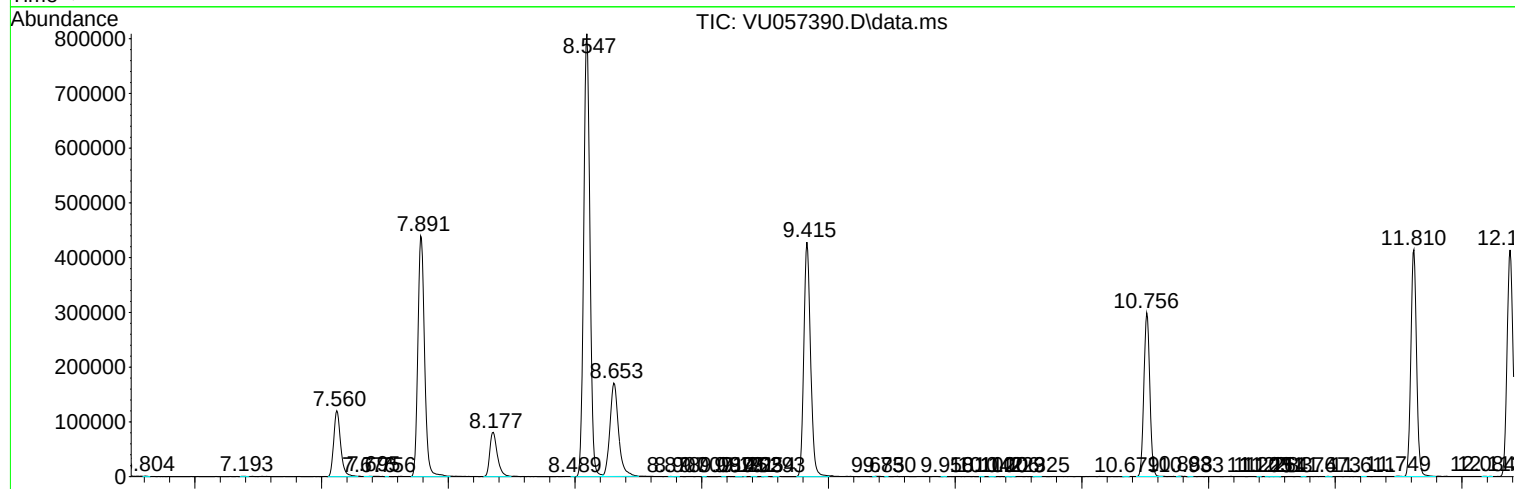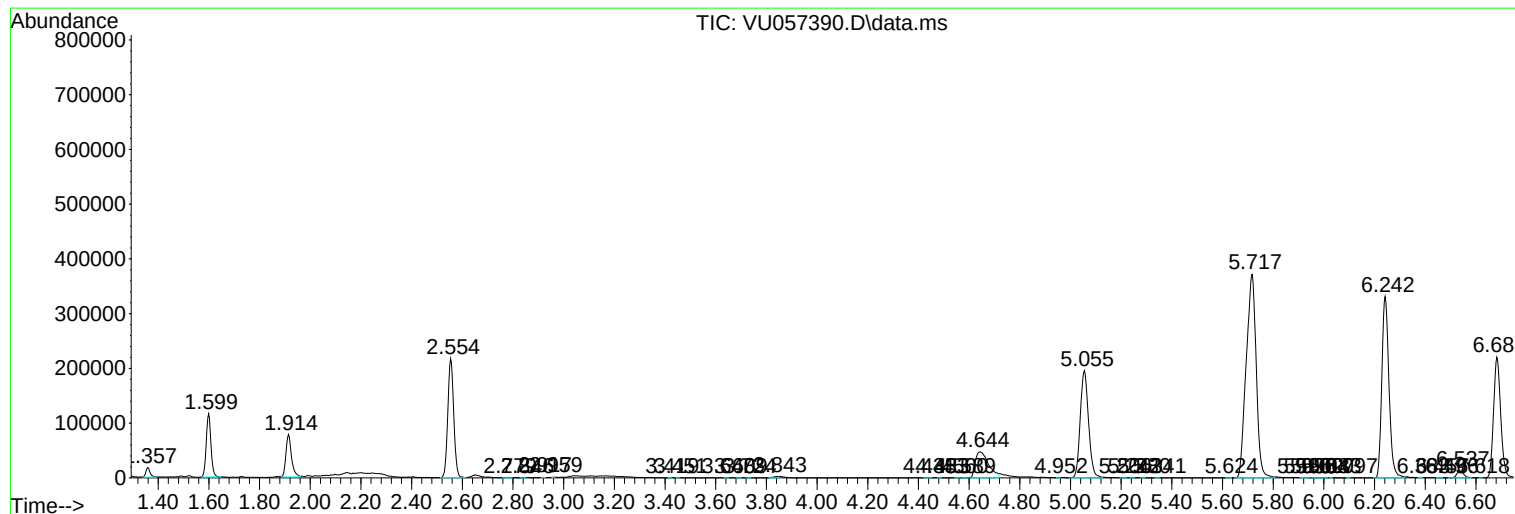

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057390.D
Acq On : 08 Jan 2024 18:19
Operator : MD/SY
Sample : 05787-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057390.D
Acq On : 08 Jan 2024 18:19
Operator : MD/SY
Sample : 05787-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc