

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057393.D
 Acq On : 08 Jan 2024 19:31
 Operator : MD/SY
 Sample : 05787-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M

Title : VOC Analysis

Signal : TIC: VU057393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	16	21	34	rVB	16142	17411	1.80%	0.239%
2	1.599	87	96	111	rVB	112770	137732	14.24%	1.893%
3	1.731	133	137	144	rVB4	1671	1792	0.19%	0.025%
4	1.914	186	194	209	rBV	81046	113940	11.78%	1.566%
5	2.386	338	341	344	rBV	523	341	0.04%	0.005%
6	2.486	369	372	374	rVV2	323	185	0.02%	0.003%
7	2.560	382	395	412	rBV	210687	341710	35.33%	4.697%
8	2.734	447	449	454	rVB	317	223	0.02%	0.003%
9	2.788	458	466	468	rBV	751	995	0.10%	0.014%
10	3.271	613	616	621	rVB2	393	252	0.03%	0.003%
11	3.361	641	644	649	rVV	466	315	0.03%	0.004%
12	3.541	697	700	703	rVB	279	201	0.02%	0.003%
13	3.711	750	753	755	rBV2	387	216	0.02%	0.003%
14	3.737	759	761	764	rVV	289	162	0.02%	0.002%
15	4.158	888	892	897	rBB	171	223	0.02%	0.003%
16	4.345	946	950	952	rBB	301	181	0.02%	0.002%
17	4.541	1008	1011	1014	rBB	230	162	0.02%	0.002%
18	4.634	1027	1040	1076	rBV	46924	152050	15.72%	2.090%
19	4.936	1130	1134	1136	rBV2	376	284	0.03%	0.004%
20	5.055	1153	1171	1194	rVV	191962	422157	43.64%	5.803%
21	5.254	1231	1233	1236	rBB	385	243	0.03%	0.003%
22	5.300	1244	1247	1250	rBB2	332	236	0.02%	0.003%
23	5.332	1255	1257	1259	rVB	385	168	0.02%	0.002%
24	5.717	1357	1377	1401	rBV2	346521	967284	100.00%	13.295%
25	5.878	1424	1427	1431	rBV2	399	290	0.03%	0.004%
26	5.946	1445	1448	1450	rVB	394	235	0.02%	0.003%
27	5.962	1451	1453	1459	rBV	377	327	0.03%	0.004%
28	6.004	1463	1466	1469	rBV	427	291	0.03%	0.004%
29	6.042	1472	1478	1481	rVV3	442	400	0.04%	0.005%
30	6.145	1507	1510	1514	rBB2	281	212	0.02%	0.003%
31	6.174	1514	1519	1521	rBV	310	246	0.03%	0.003%
32	6.242	1526	1540	1562	rBV	329436	633326	65.47%	8.705%
33	6.451	1603	1605	1608	rVB	394	221	0.02%	0.003%
34	6.534	1629	1631	1634	rVB3	689	318	0.03%	0.004%
35	6.682	1664	1677	1699	rVV	212785	415413	42.95%	5.710%
36	6.791	1708	1711	1714	rBV3	656	407	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057393.D
 Acq On : 08 Jan 2024 19:31
 Operator : MD/SY
 Sample : 05787-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

37	6.811	1714	1717	1720	rVB3	708	461	0.05%	0.006%
38	7.049	1788	1791	1793	rBV2	334	205	0.02%	0.003%
39	7.190	1832	1835	1839	rBV2	603	660	0.07%	0.009%
40	7.489	1922	1928	1930	rBV	185	193	0.02%	0.003%
41	7.560	1936	1950	1965	rBV	118106	212676	21.99%	2.923%
42	7.695	1989	1992	1994	rBV2	569	350	0.04%	0.005%
43	7.791	2020	2022	2025	rVB2	319	189	0.02%	0.003%
44	7.891	2041	2053	2071	rBV	419719	750354	77.57%	10.314%
45	8.174	2127	2141	2158	rBV	83114	152275	15.74%	2.093%
46	8.303	2179	2181	2184	rVB	379	178	0.02%	0.002%
47	8.370	2199	2202	2205	rVB	282	198	0.02%	0.003%
48	8.431	2219	2221	2224	rBV2	253	169	0.02%	0.002%
49	8.547	2251	2257	2264	rBV4	2958	4141	0.43%	0.057%
50	8.640	2271	2286	2321	rBV3	174455	383251	39.62%	5.268%
51	8.814	2336	2340	2344	rBV3	410	317	0.03%	0.004%
52	8.856	2349	2353	2357	rBV3	342	325	0.03%	0.004%
53	8.878	2357	2360	2367	rVB2	490	450	0.05%	0.006%
54	8.942	2376	2380	2384	rBV2	375	399	0.04%	0.005%
55	9.020	2399	2404	2406	rBB	237	214	0.02%	0.003%
56	9.071	2417	2420	2425	rBV	261	228	0.02%	0.003%
57	9.348	2502	2506	2508	rBV	212	202	0.02%	0.003%
58	9.412	2514	2526	2552	rBV	444978	772042	79.82%	10.612%
59	9.576	2574	2577	2578	rBV2	385	238	0.02%	0.003%
60	9.627	2588	2593	2595	rBV	286	245	0.03%	0.003%
61	9.653	2599	2601	2603	rVB	387	183	0.02%	0.003%
62	9.669	2604	2606	2608	rBV	339	174	0.02%	0.002%
63	9.688	2609	2612	2615	rVB2	336	224	0.02%	0.003%
64	9.708	2616	2618	2624	rBV2	355	380	0.04%	0.005%
65	9.788	2639	2643	2644	rBV	346	235	0.02%	0.003%
66	9.881	2669	2672	2675	rBV	258	248	0.03%	0.003%
67	9.904	2677	2679	2683	rVB2	257	173	0.02%	0.002%
68	9.952	2690	2694	2696	rVB	361	243	0.03%	0.003%
69	9.971	2697	2700	2704	rBV	222	209	0.02%	0.003%
70	10.058	2725	2727	2731	rVB	456	207	0.02%	0.003%
71	10.122	2743	2747	2749	rBV	200	202	0.02%	0.003%
72	10.238	2777	2783	2786	rBB	257	297	0.03%	0.004%
73	10.322	2807	2809	2811	rBV	233	160	0.02%	0.002%
74	10.351	2815	2818	2827	rVB2	421	391	0.04%	0.005%
75	10.389	2827	2830	2833	rBV2	220	164	0.02%	0.002%
76	10.704	2923	2928	2931	rVB	332	236	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057393.D
 Acq On : 08 Jan 2024 19:31
 Operator : MD/SY
 Sample : 05787-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

77	10.753	2931	2943	2961	rBV	289721	470803	48.67%	6.471%
78	10.884	2982	2984	2987	rBV	362	269	0.03%	0.004%
79	10.942	2997	3002	3005	rBV	410	372	0.04%	0.005%
80	11.174	3072	3074	3079	rVB2	270	181	0.02%	0.002%
81	11.302	3111	3114	3118	rVB2	234	165	0.02%	0.002%
82	11.376	3133	3137	3138	rBV2	323	257	0.03%	0.004%
83	11.624	3212	3214	3218	rVB	293	206	0.02%	0.003%
84	11.807	3259	3271	3289	rBV	402756	652241	67.43%	8.965%
85	12.081	3352	3356	3358	rBV2	338	285	0.03%	0.004%
86	12.187	3376	3389	3419	rBV	391013	651356	67.34%	8.953%
87	12.344	3435	3438	3441	rBV2	333	226	0.02%	0.003%
88	12.556	3501	3504	3506	rBV	305	212	0.02%	0.003%
89	12.695	3543	3547	3549	rBV	244	218	0.02%	0.003%
90	12.762	3561	3568	3576	rVB3	819	1290	0.13%	0.018%
91	13.023	3646	3649	3657	rVB2	745	717	0.07%	0.010%
92	13.556	3809	3815	3818	rBV2	383	493	0.05%	0.007%
93	13.743	3871	3873	3875	rBV2	315	205	0.02%	0.003%
94	13.810	3892	3894	3896	rBV2	385	171	0.02%	0.002%
95	14.100	3982	3984	3985	rBV	434	180	0.02%	0.002%
96	14.196	4010	4014	4015	rBV	473	221	0.02%	0.003%
97	14.322	4050	4053	4056	rBV	331	266	0.03%	0.004%
98	14.560	4124	4127	4130	rBV2	559	376	0.04%	0.005%
99	14.601	4137	4140	4141	rBV	464	223	0.02%	0.003%
100	14.772	4189	4193	4198	rBV2	637	574	0.06%	0.008%




Sum of corrected areas: 7275342

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057393.D
Acq On : 08 Jan 2024 19:31
Operator : MD/SY
Sample : 05787-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

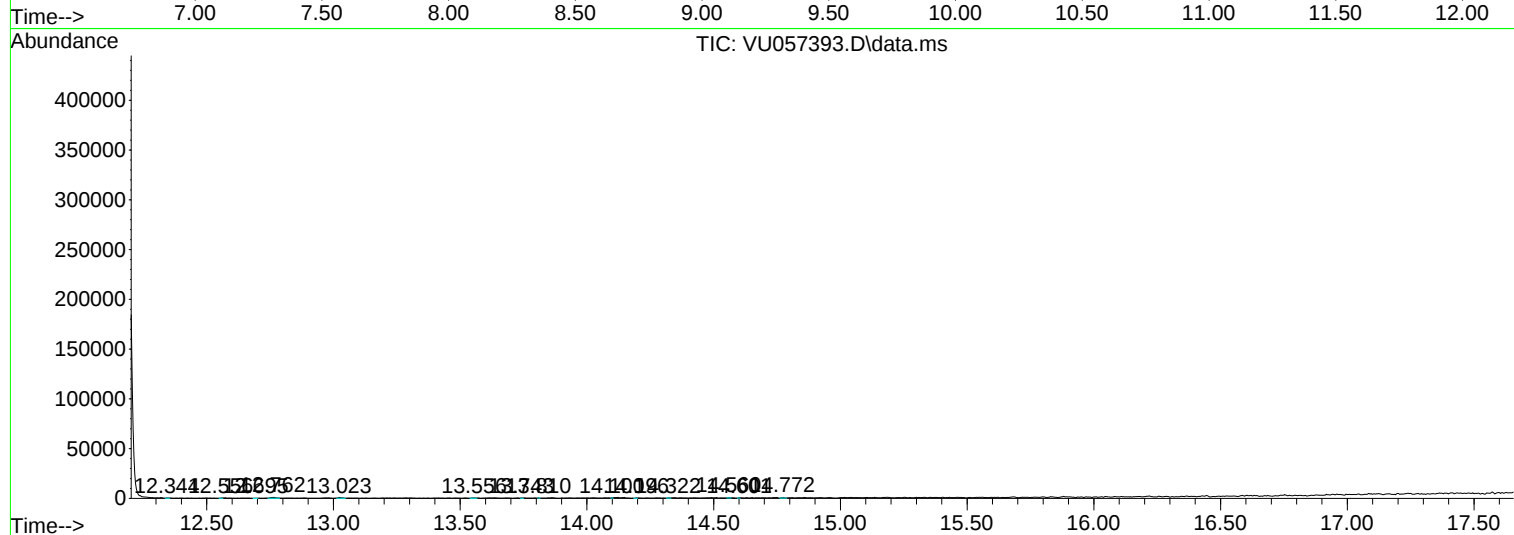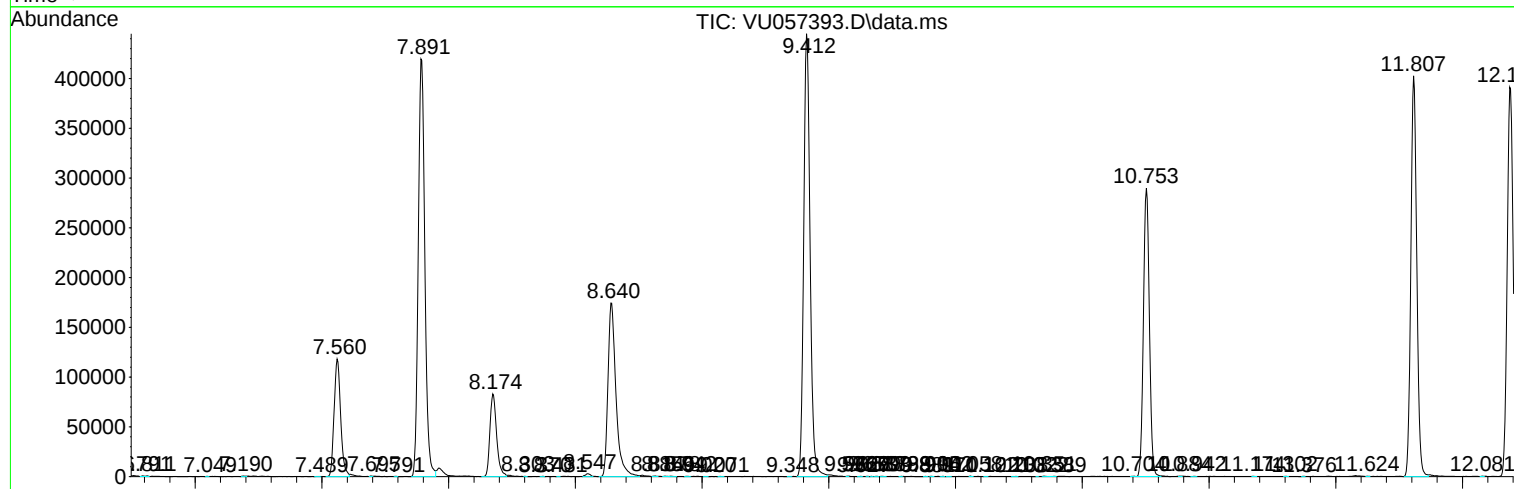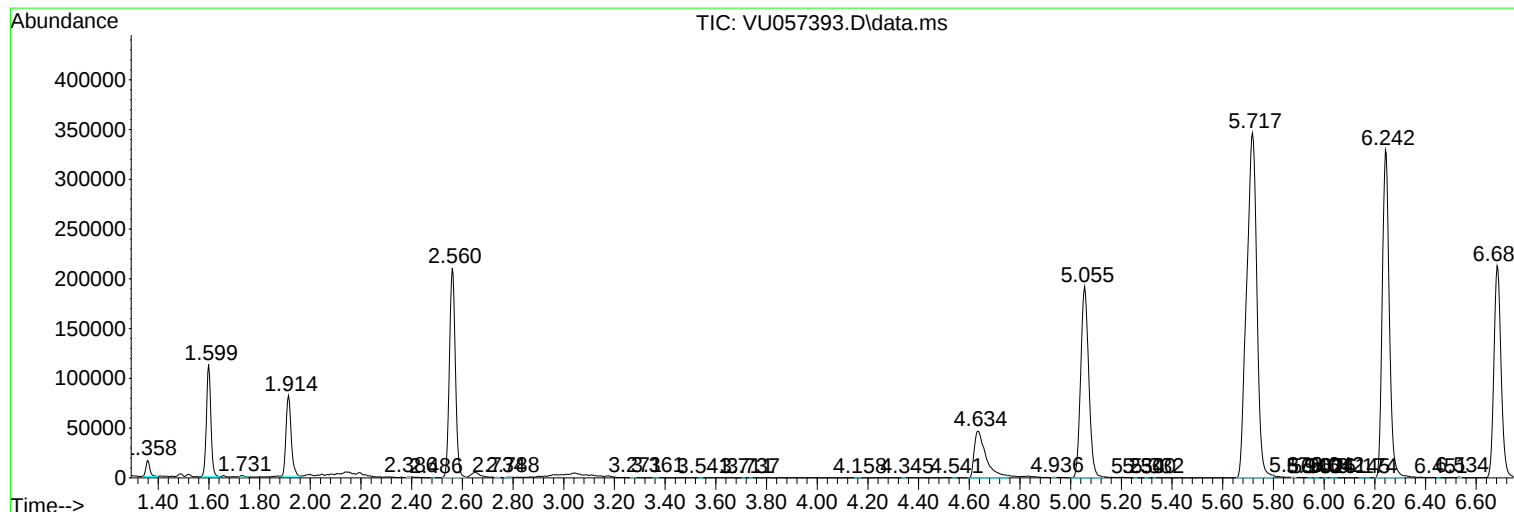

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057393.D
Acq On : 08 Jan 2024 19:31
Operator : MD/SY
Sample : 05787-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057393.D
Acq On : 08 Jan 2024 19:31
Operator : MD/SY
Sample : 05787-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc