

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057394.D
 Acq On : 08 Jan 2024 19:56
 Operator : MD/SY
 Sample : 05787-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

Signal : TIC: VU057394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	16	21	30	rVB4	9169	9742	1.00%	0.133%
2	1.599	88	96	112	rVB	107993	130861	13.42%	1.791%
3	1.914	186	194	210	rVB	74598	108567	11.13%	1.486%
4	2.486	371	372	376	rBV2	272	194	0.02%	0.003%
5	2.557	381	394	414	rBV	208940	340325	34.89%	4.659%
6	2.644	414	421	423	rBV4	1962	2142	0.22%	0.029%
7	2.776	456	462	463	rBV	483	431	0.04%	0.006%
8	2.859	486	488	490	rBV2	372	189	0.02%	0.003%
9	3.309	625	628	633	rBB	229	230	0.02%	0.003%
10	3.354	638	642	644	rBB	253	181	0.02%	0.002%
11	3.370	644	647	649	rBV	280	195	0.02%	0.003%
12	3.451	668	672	675	rBV	324	281	0.03%	0.004%
13	3.541	697	700	705	rBB	159	152	0.02%	0.002%
14	3.695	745	748	751	rBV2	414	317	0.03%	0.004%
15	3.840	788	793	796	rBB	239	228	0.02%	0.003%
16	3.940	821	824	827	rBB	191	158	0.02%	0.002%
17	4.065	861	863	865	rBV	286	178	0.02%	0.002%
18	4.338	946	948	950	rBV	286	172	0.02%	0.002%
19	4.370	956	958	962	rVB	397	222	0.02%	0.003%
20	4.486	991	994	996	rBV	193	150	0.02%	0.002%
21	4.637	1030	1041	1068	rBV2	42766	142175	14.58%	1.946%
22	4.914	1125	1127	1132	rVB2	429	240	0.02%	0.003%
23	4.940	1133	1135	1139	rVB	470	286	0.03%	0.004%
24	5.055	1154	1171	1197	rBV	189714	420442	43.11%	5.755%
25	5.255	1231	1233	1240	rBB	270	249	0.03%	0.003%
26	5.316	1248	1252	1255	rBV	317	330	0.03%	0.005%
27	5.718	1356	1377	1407	rBV2	355115	975301	100.00%	13.351%
28	5.985	1454	1460	1462	rBB	302	230	0.02%	0.003%
29	5.997	1462	1464	1469	rBV2	394	392	0.04%	0.005%
30	6.113	1496	1500	1503	rBB	298	203	0.02%	0.003%
31	6.139	1506	1508	1512	rBV	249	189	0.02%	0.003%
32	6.242	1527	1540	1563	rBV	334255	649029	66.55%	8.885%
33	6.470	1606	1611	1615	rBB2	479	427	0.04%	0.006%
34	6.528	1626	1629	1635	rBV3	697	645	0.07%	0.009%
35	6.579	1642	1645	1648	rBB2	392	252	0.03%	0.003%
36	6.599	1648	1651	1653	rBB2	534	298	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057394.D
 Acq On : 08 Jan 2024 19:56
 Operator : MD/SY
 Sample : 05787-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

37	6.615	1653	1656	1658	rBB	306	169	0.02%	0.002%
38	6.682	1659	1677	1700	rBV	208803	417878	42.85%	5.720%
39	6.808	1712	1716	1718	rBV2	552	358	0.04%	0.005%
40	6.930	1752	1754	1756	rBV2	285	193	0.02%	0.003%
41	6.959	1762	1763	1768	rVB2	256	164	0.02%	0.002%
42	7.197	1833	1837	1841	rBV2	722	773	0.08%	0.011%
43	7.251	1851	1854	1858	rBV2	165	173	0.02%	0.002%
44	7.284	1863	1864	1869	rBB	218	149	0.02%	0.002%
45	7.560	1939	1950	1971	rBV2	116860	214804	22.02%	2.940%
46	7.702	1990	1994	1999	rBV3	494	531	0.05%	0.007%
47	7.894	2036	2054	2072	rBV	421166	751343	77.04%	10.285%
48	8.110	2119	2121	2126	rVB2	241	212	0.02%	0.003%
49	8.174	2129	2141	2172	rBV2	81475	155898	15.98%	2.134%
50	8.283	2172	2175	2177	rVB	400	252	0.03%	0.003%
51	8.306	2177	2182	2185	rBB2	303	283	0.03%	0.004%
52	8.399	2209	2211	2213	rBV	279	177	0.02%	0.002%
53	8.554	2249	2259	2265	rBB4	2201	3591	0.37%	0.049%
54	8.592	2266	2271	2275	rBV	158	210	0.02%	0.003%
55	8.647	2275	2288	2318	rBV2	164473	379093	38.87%	5.189%
56	8.827	2342	2344	2346	rVB2	386	148	0.02%	0.002%
57	8.853	2350	2352	2354	rBV	259	167	0.02%	0.002%
58	9.280	2480	2485	2488	rBV	247	200	0.02%	0.003%
59	9.415	2514	2527	2562	rVV	436503	798891	81.91%	10.936%
60	9.605	2583	2586	2589	rBB	192	150	0.02%	0.002%
61	9.833	2654	2657	2660	rBB	304	221	0.02%	0.003%
62	9.856	2661	2664	2668	rBB	252	170	0.02%	0.002%
63	10.049	2720	2724	2726	rBV	227	163	0.02%	0.002%
64	10.184	2762	2766	2769	rBB2	252	200	0.02%	0.003%
65	10.274	2787	2794	2799	rBV	211	403	0.04%	0.006%
66	10.390	2827	2830	2831	rBV	297	180	0.02%	0.002%
67	10.467	2850	2854	2858	rBV	254	284	0.03%	0.004%
68	10.534	2870	2875	2878	rBB	194	217	0.02%	0.003%
69	10.553	2878	2881	2886	rBB	158	159	0.02%	0.002%
70	10.592	2887	2893	2896	rBV	371	439	0.05%	0.006%
71	10.756	2932	2944	2964	rBV	288400	471505	48.34%	6.454%
72	10.830	2964	2967	2968	rBV2	418	225	0.02%	0.003%
73	10.878	2979	2982	2983	rBV2	346	195	0.02%	0.003%
74	10.981	3010	3014	3018	rBV	233	286	0.03%	0.004%
75	11.000	3018	3020	3025	rVV	268	215	0.02%	0.003%
76	11.026	3025	3028	3032	rVV	168	175	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057394.D
 Acq On : 08 Jan 2024 19:56
 Operator : MD/SY
 Sample : 05787-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

77	11.062	3036	3039	3044	rBV	167	208	0.02%	0.003%
78	11.271	3100	3104	3109	rBV	315	260	0.03%	0.004%
79	11.521	3178	3182	3184	rBV	271	176	0.02%	0.002%
80	11.807	3259	3271	3294	rBV	417290	666670	68.36%	9.126%
81	11.962	3315	3319	3321	rBV2	439	317	0.03%	0.004%
82	12.110	3362	3365	3369	rBV2	360	195	0.02%	0.003%
83	12.190	3377	3390	3413	rBV	392039	645054	66.14%	8.830%
84	12.396	3447	3454	3457	rBV	347	457	0.05%	0.006%
85	12.428	3461	3464	3466	rVB	362	170	0.02%	0.002%
86	12.878	3602	3604	3607	rVB2	280	147	0.02%	0.002%
87	13.023	3646	3649	3655	rVB2	400	425	0.04%	0.006%
88	13.187	3697	3700	3703	rBV	319	210	0.02%	0.003%
89	13.229	3710	3713	3716	rVB2	304	178	0.02%	0.002%
90	13.248	3716	3719	3723	rBV2	284	244	0.03%	0.003%
91	13.402	3763	3767	3769	rBV2	346	273	0.03%	0.004%
92	13.431	3773	3776	3778	rBV2	290	202	0.02%	0.003%
93	13.672	3848	3851	3854	rBV	472	285	0.03%	0.004%
94	13.778	3881	3884	3886	rBV2	346	221	0.02%	0.003%
95	14.058	3968	3971	3974	rBV3	296	254	0.03%	0.003%
96	14.106	3979	3986	3988	rBV2	1000	1096	0.11%	0.015%
97	14.434	4085	4088	4089	rBV	392	222	0.02%	0.003%
98	14.717	4171	4176	4180	rBV3	905	866	0.09%	0.012%
99	14.775	4191	4194	4195	rBV	351	236	0.02%	0.003%
100	14.852	4215	4218	4221	rBV2	418	254	0.03%	0.003%




Sum of corrected areas: 7305067

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057394.D
Acq On : 08 Jan 2024 19:56
Operator : MD/SY
Sample : 05787-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

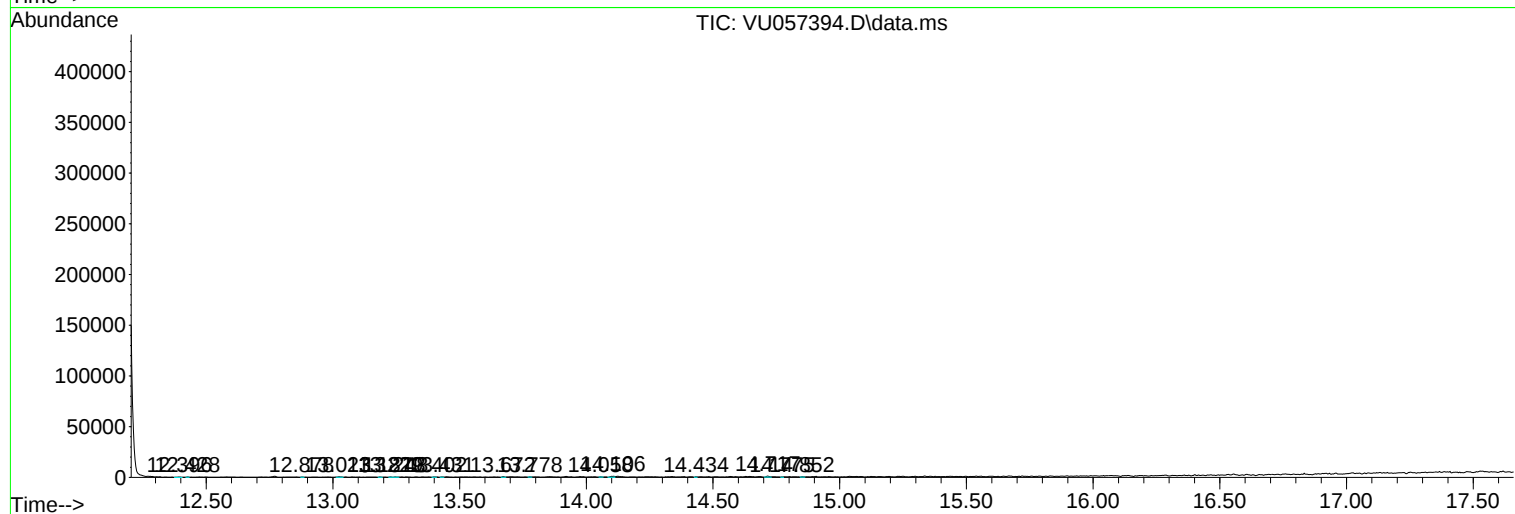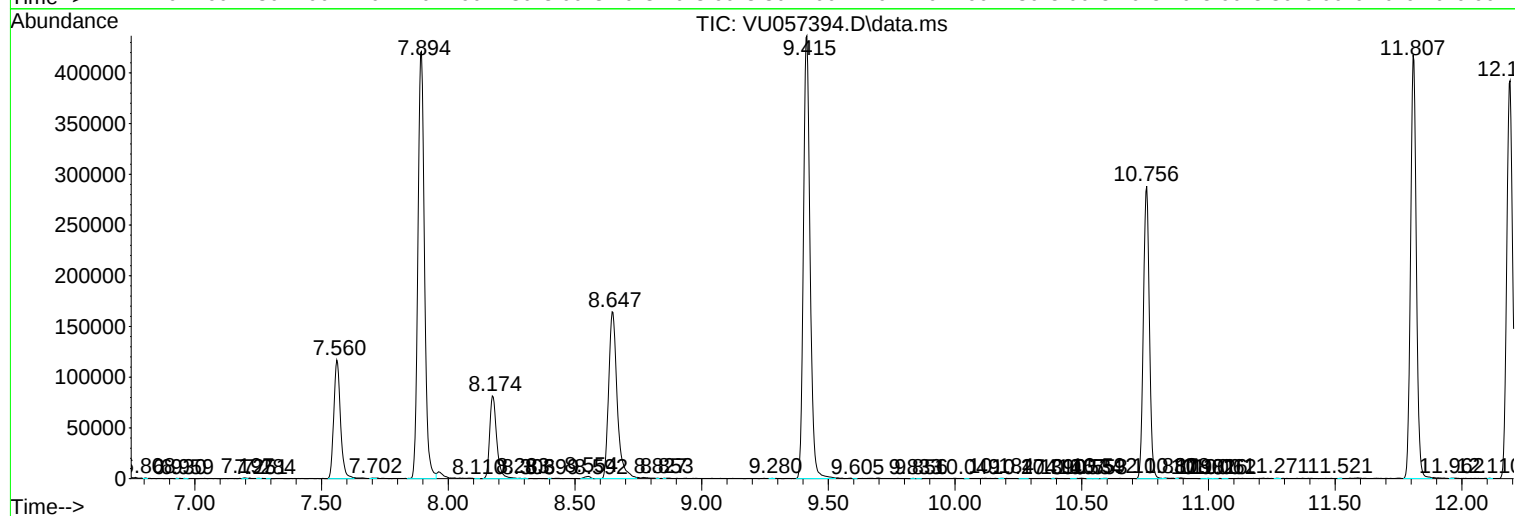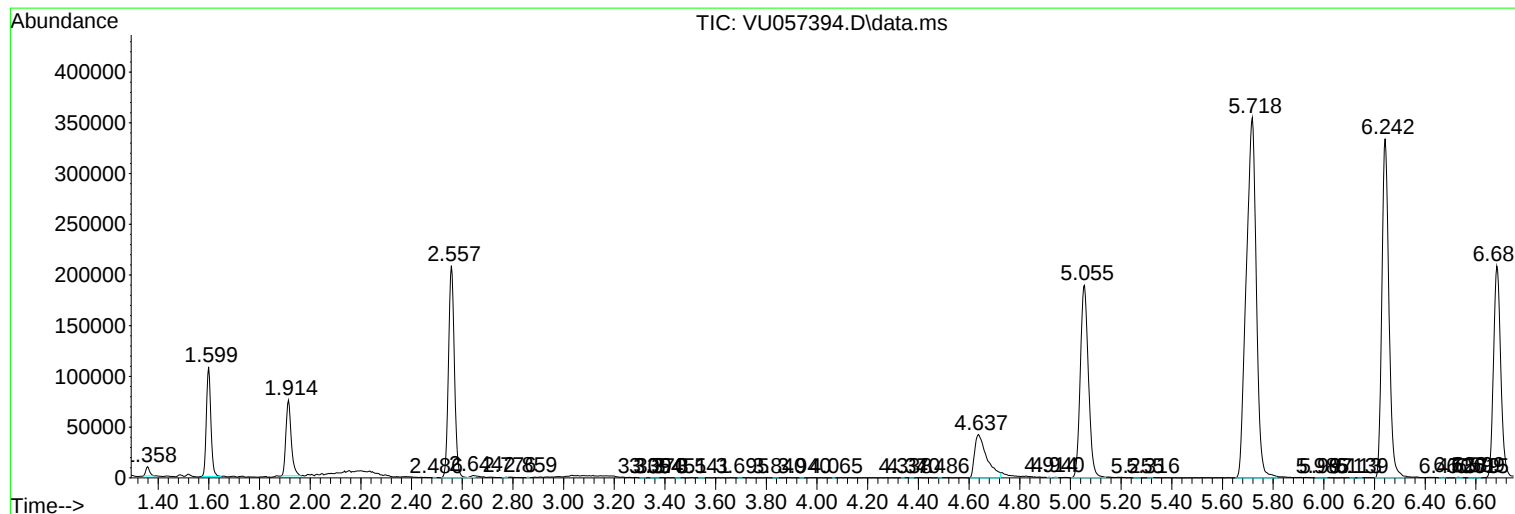

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057394.D
Acq On : 08 Jan 2024 19:56
Operator : MD/SY
Sample : 05787-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057394.D
Acq On : 08 Jan 2024 19:56
Operator : MD/SY
Sample : 05787-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------