

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057399.D
 Acq On : 08 Jan 2024 21:56
 Operator : MD/SY
 Sample : 05787-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

Signal : TIC: VU057399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	16	21	27	rBV2	4569	4600	0.48%	0.064%
2	1.519	68	71	81	rVB2	3343	3436	0.36%	0.048%
3	1.599	88	96	114	rVB	108086	129954	13.48%	1.816%
4	1.914	186	194	206	rBV	74981	107061	11.10%	1.496%
5	2.348	327	329	330	rBV	374	169	0.02%	0.002%
6	2.477	365	369	370	rBV2	282	178	0.02%	0.002%
7	2.506	375	378	381	rBV	378	215	0.02%	0.003%
8	2.560	382	395	412	rBV	203904	333564	34.59%	4.661%
9	2.708	439	441	445	rVB2	621	348	0.04%	0.005%
10	2.789	456	466	470	rBV2	752	1068	0.11%	0.015%
11	2.898	498	500	501	rBV	468	220	0.02%	0.003%
12	3.274	615	617	620	rVB	264	151	0.02%	0.002%
13	3.348	635	640	642	rBV	278	223	0.02%	0.003%
14	3.412	657	660	662	rVB2	314	201	0.02%	0.003%
15	3.560	703	706	708	rBV	233	154	0.02%	0.002%
16	3.682	741	744	747	rBB	185	142	0.01%	0.002%
17	3.940	821	824	826	rBV	341	218	0.02%	0.003%
18	3.959	826	830	833	rVB	278	245	0.03%	0.003%
19	4.406	966	969	972	rBB	249	164	0.02%	0.002%
20	4.634	1029	1040	1069	rBV	46231	146402	15.18%	2.046%
21	5.055	1154	1171	1192	rBV2	185937	421282	43.68%	5.887%
22	5.322	1250	1254	1259	rBV2	440	422	0.04%	0.006%
23	5.718	1355	1377	1398	rBV2	350083	964364	100.00%	13.476%
24	6.023	1469	1472	1474	rBV	380	247	0.03%	0.003%
25	6.152	1510	1512	1514	rVB	300	139	0.01%	0.002%
26	6.242	1527	1540	1569	rBV	314469	613398	63.61%	8.571%
27	6.515	1623	1625	1627	rVV	287	152	0.02%	0.002%
28	6.525	1627	1628	1631	rVV2	379	216	0.02%	0.003%
29	6.605	1650	1653	1656	rBV2	657	464	0.05%	0.006%
30	6.682	1663	1677	1699	rBV	213686	416603	43.20%	5.822%
31	6.798	1711	1713	1718	rVV	389	299	0.03%	0.004%
32	6.856	1728	1731	1733	rVB	270	156	0.02%	0.002%
33	6.972	1763	1767	1771	rBB	155	157	0.02%	0.002%
34	7.071	1796	1798	1801	rBB	262	153	0.02%	0.002%
35	7.190	1832	1835	1840	rBV2	538	455	0.05%	0.006%
36	7.255	1851	1855	1858	rBV3	296	218	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057399.D
 Acq On : 08 Jan 2024 21:56
 Operator : MD/SY
 Sample : 05787-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

37	7.319	1871	1875	1878	rBB2	249	219	0.02%	0.003%
38	7.412	1901	1904	1908	rBB	215	193	0.02%	0.003%
39	7.464	1917	1920	1922	rBV	181	143	0.01%	0.002%
40	7.560	1938	1950	1968	rVV2	116143	213124	22.10%	2.978%
41	7.663	1980	1982	1985	rBV	462	204	0.02%	0.003%
42	7.702	1990	1994	1997	rBV2	344	283	0.03%	0.004%
43	7.795	2021	2023	2026	rBV	310	198	0.02%	0.003%
44	7.891	2040	2053	2086	rBV	417735	752821	78.06%	10.520%
45	8.062	2103	2106	2108	rBV2	430	275	0.03%	0.004%
46	8.174	2129	2141	2167	rVV	79910	149519	15.50%	2.089%
47	8.264	2167	2169	2174	rVB2	588	396	0.04%	0.006%
48	8.345	2192	2194	2198	rVB2	271	229	0.02%	0.003%
49	8.486	2235	2238	2241	rBV2	229	145	0.02%	0.002%
50	8.554	2252	2259	2265	rVB4	2258	2893	0.30%	0.040%
51	8.595	2266	2272	2274	rBV	259	237	0.02%	0.003%
52	8.644	2274	2287	2321	rBV3	169789	378266	39.22%	5.286%
53	8.808	2334	2338	2341	rBV2	456	367	0.04%	0.005%
54	8.846	2348	2350	2353	rVB2	399	169	0.02%	0.002%
55	8.882	2358	2361	2363	rBV	312	161	0.02%	0.002%
56	8.923	2371	2374	2376	rBV	201	153	0.02%	0.002%
57	8.943	2378	2380	2385	rVV	242	204	0.02%	0.003%
58	9.078	2420	2422	2428	rVV	328	219	0.02%	0.003%
59	9.110	2429	2432	2438	rVB	303	319	0.03%	0.004%
60	9.145	2439	2443	2447	rBB2	267	202	0.02%	0.003%
61	9.412	2513	2526	2556	rBV	427084	762312	79.05%	10.652%
62	9.615	2587	2589	2594	rVB	374	197	0.02%	0.003%
63	9.647	2596	2599	2604	rBV2	299	256	0.03%	0.004%
64	9.718	2615	2621	2624	rBV2	327	359	0.04%	0.005%
65	9.853	2659	2663	2666	rBV	274	250	0.03%	0.003%
66	9.917	2681	2683	2688	rVB	245	168	0.02%	0.002%
67	9.965	2695	2698	2702	rBV	187	189	0.02%	0.003%
68	10.177	2761	2764	2767	rBV	183	174	0.02%	0.002%
69	10.209	2770	2774	2777	rBV2	455	338	0.04%	0.005%
70	10.258	2786	2789	2791	rBV	183	148	0.02%	0.002%
71	10.447	2843	2848	2849	rBV	168	168	0.02%	0.002%
72	10.486	2856	2860	2864	rBB	358	299	0.03%	0.004%
73	10.672	2914	2918	2921	rBB	294	269	0.03%	0.004%
74	10.698	2922	2926	2930	rBV	203	214	0.02%	0.003%
75	10.753	2930	2943	2964	rVV	288623	472506	49.00%	6.603%
76	10.885	2978	2984	2988	rVV2	430	559	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057399.D
 Acq On : 08 Jan 2024 21:56
 Operator : MD/SY
 Sample : 05787-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

77	10.952	2999	3005	3008	rBV	282	350	0.04%	0.005%
78	11.155	3066	3068	3071	rBV	232	169	0.02%	0.002%
79	11.370	3132	3135	3143	rVB2	524	390	0.04%	0.005%
80	11.412	3143	3148	3151	rBV2	264	224	0.02%	0.003%
81	11.476	3166	3168	3171	rVB	310	171	0.02%	0.002%
82	11.676	3225	3230	3234	rBV	279	357	0.04%	0.005%
83	11.721	3240	3244	3248	rBV	262	223	0.02%	0.003%
84	11.807	3258	3271	3290	rBV	389635	623615	64.67%	8.714%
85	12.190	3377	3390	3407	rBV	390261	639002	66.26%	8.929%
86	12.676	3539	3541	3543	rBV	310	141	0.01%	0.002%
87	12.772	3563	3571	3575	rBV3	835	1026	0.11%	0.014%
88	12.917	3614	3616	3622	rVB2	273	214	0.02%	0.003%
89	13.640	3839	3841	3846	rBV	232	162	0.02%	0.002%
90	13.759	3873	3878	3879	rBV	280	229	0.02%	0.003%
91	13.868	3909	3912	3913	rBV	304	191	0.02%	0.003%
92	14.338	4053	4058	4060	rBV2	579	445	0.05%	0.006%
93	14.402	4075	4078	4082	rBV	287	173	0.02%	0.002%
94	14.431	4082	4087	4093	rBV3	398	540	0.06%	0.008%
95	14.540	4119	4121	4122	rBV	392	176	0.02%	0.002%
96	14.676	4160	4163	4165	rBV	460	285	0.03%	0.004%
97	14.753	4183	4187	4189	rBV2	382	333	0.03%	0.005%
98	15.502	4417	4420	4424	rVB3	716	463	0.05%	0.006%
99	15.569	4439	4441	4442	rBV	658	225	0.02%	0.003%
100	15.933	4552	4554	4557	rBV3	864	380	0.04%	0.005%




Sum of corrected areas: 7156267

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057399.D
Acq On : 08 Jan 2024 21:56
Operator : MD/SY
Sample : 05787-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

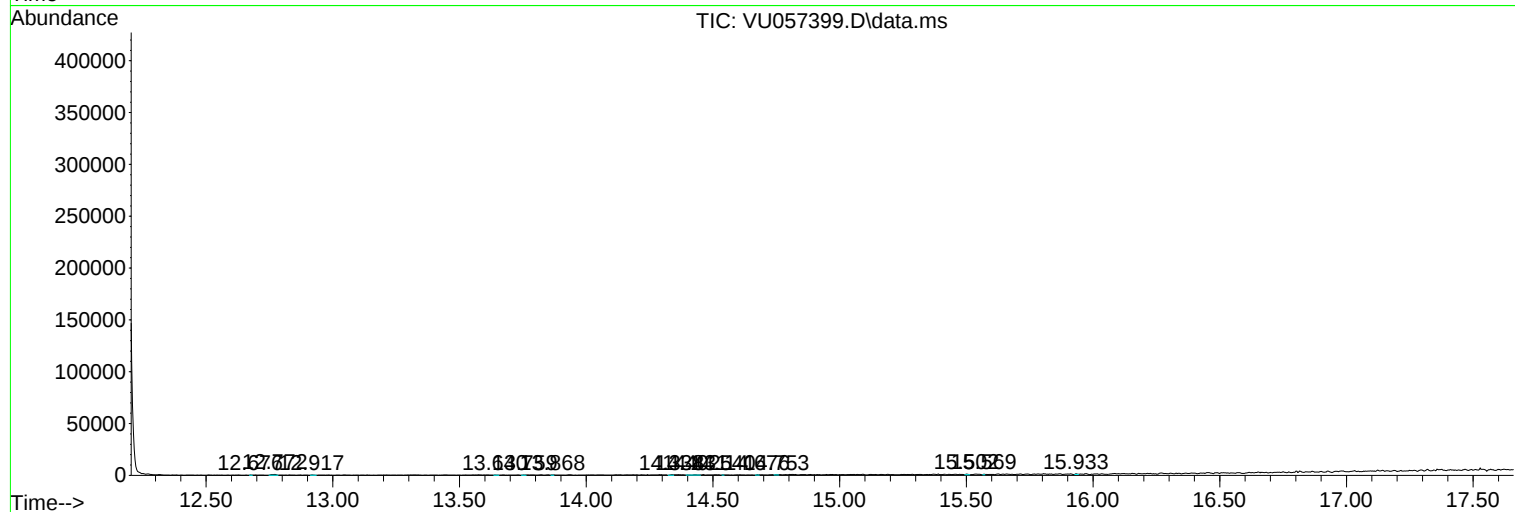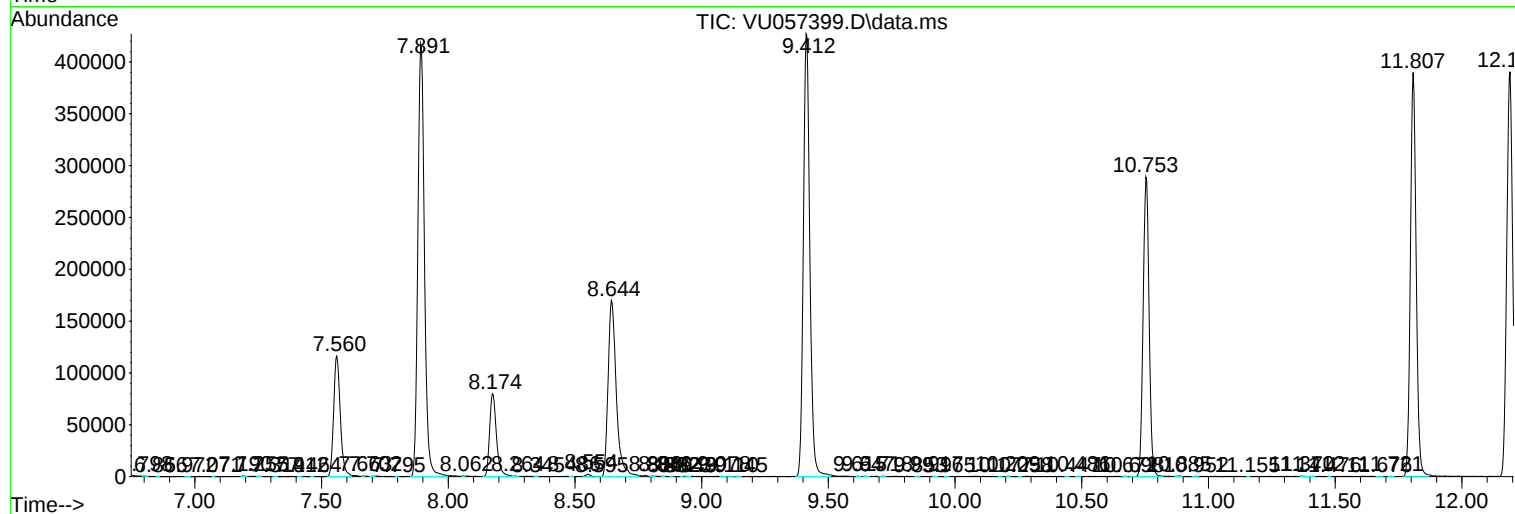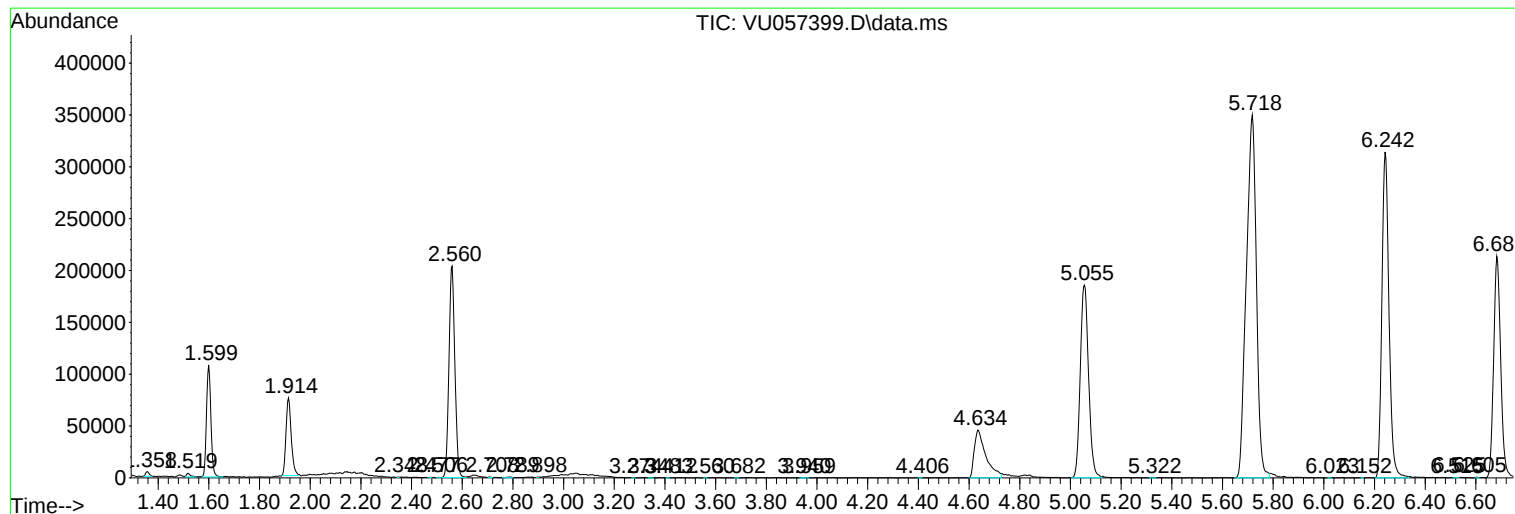

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057399.D
Acq On : 08 Jan 2024 21:56
Operator : MD/SY
Sample : 05787-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057399.D
Acq On : 08 Jan 2024 21:56
Operator : MD/SY
Sample : 05787-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------