

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057400.D
 Acq On : 08 Jan 2024 22:20
 Operator : MD/SY
 Sample : 05787-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

Signal : TIC: VU057400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	67	71	77	rBV2	3091	3048	0.31%	0.042%
2	1.599	88	96	111	rVB	108053	129669	13.19%	1.792%
3	1.914	186	194	211	rBV	76992	110048	11.19%	1.521%
4	2.390	340	342	346	rBV	472	264	0.03%	0.004%
5	2.557	381	394	413	rBV	210562	342046	34.79%	4.727%
6	2.782	456	464	472	rBB2	890	1494	0.15%	0.021%
7	2.843	481	483	485	rBV	377	195	0.02%	0.003%
8	3.248	607	609	612	rBV	282	193	0.02%	0.003%
9	3.312	624	629	631	rBV	313	269	0.03%	0.004%
10	3.325	631	633	637	rVB	364	214	0.02%	0.003%
11	3.393	652	654	658	rVB	366	214	0.02%	0.003%
12	3.422	658	663	667	rBB	239	240	0.02%	0.003%
13	3.470	675	678	681	rBB	196	152	0.02%	0.002%
14	3.509	685	690	692	rBV2	271	263	0.03%	0.004%
15	3.814	781	785	788	rBV	181	172	0.02%	0.002%
16	4.026	847	851	854	rBB	251	151	0.02%	0.002%
17	4.634	1025	1040	1063	rBV	43955	139090	14.15%	1.922%
18	5.055	1156	1171	1194	rVV	190832	422700	42.99%	5.842%
19	5.322	1250	1254	1256	rVV	302	241	0.02%	0.003%
20	5.341	1258	1260	1263	rVB	339	155	0.02%	0.002%
21	5.393	1272	1276	1277	rBV	230	178	0.02%	0.002%
22	5.454	1293	1295	1298	rBV	222	156	0.02%	0.002%
23	5.492	1305	1307	1310	rBB	318	190	0.02%	0.003%
24	5.717	1355	1377	1401	rBV2	356038	983227	100.00%	13.588%
25	5.981	1455	1459	1463	rBB	477	322	0.03%	0.004%
26	6.242	1527	1540	1565	rBV	320633	626307	63.70%	8.655%
27	6.399	1587	1589	1592	rBV	280	159	0.02%	0.002%
28	6.473	1609	1612	1619	rVB	283	290	0.03%	0.004%
29	6.531	1628	1630	1634	rVB3	507	274	0.03%	0.004%
30	6.550	1634	1636	1639	rVB	396	217	0.02%	0.003%
31	6.598	1649	1651	1654	rBV	354	276	0.03%	0.004%
32	6.631	1659	1661	1664	rBV	280	198	0.02%	0.003%
33	6.682	1664	1677	1696	rBV2	210050	412953	42.00%	5.707%
34	6.804	1713	1715	1717	rBV2	385	187	0.02%	0.003%
35	6.875	1734	1737	1741	rBB	311	220	0.02%	0.003%
36	6.923	1748	1752	1755	rBB	203	159	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057400.D
 Acq On : 08 Jan 2024 22:20
 Operator : MD/SY
 Sample : 05787-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

37	6.975	1764	1768	1773	rVB2	322	335	0.03%	0.005%
38	7.190	1832	1835	1836	rBV	504	233	0.02%	0.003%
39	7.245	1851	1852	1855	rBV	327	177	0.02%	0.002%
40	7.267	1857	1859	1864	rVB	451	272	0.03%	0.004%
41	7.393	1894	1898	1902	rBB	251	256	0.03%	0.004%
42	7.560	1937	1950	1970	rBV	118519	214943	21.86%	2.970%
43	7.663	1979	1982	1984	rBV2	255	177	0.02%	0.002%
44	7.891	2040	2053	2088	rBV	428048	763219	77.62%	10.547%
45	8.119	2122	2124	2127	rBV	303	181	0.02%	0.003%
46	8.174	2127	2141	2168	rVV	84042	154749	15.74%	2.139%
47	8.303	2178	2181	2186	rBV3	333	272	0.03%	0.004%
48	8.386	2204	2207	2211	rBV	141	177	0.02%	0.002%
49	8.428	2216	2220	2223	rBB2	289	242	0.02%	0.003%
50	8.454	2224	2228	2231	rBB	318	230	0.02%	0.003%
51	8.483	2231	2237	2239	rBB2	308	289	0.03%	0.004%
52	8.521	2244	2249	2251	rBV	309	260	0.03%	0.004%
53	8.547	2252	2257	2265	rBV5	1943	2480	0.25%	0.034%
54	8.647	2275	2288	2312	rBV2	169530	375807	38.22%	5.194%
55	8.843	2347	2349	2353	rVV2	243	165	0.02%	0.002%
56	9.065	2415	2418	2420	rBV2	356	200	0.02%	0.003%
57	9.277	2481	2484	2487	rBB	205	168	0.02%	0.002%
58	9.348	2502	2506	2508	rBV	208	175	0.02%	0.002%
59	9.415	2514	2527	2551	rBV	430209	776793	79.00%	10.735%
60	9.688	2609	2612	2615	rVB	466	294	0.03%	0.004%
61	9.711	2615	2619	2621	rBV	391	269	0.03%	0.004%
62	9.762	2632	2635	2636	rBV	335	166	0.02%	0.002%
63	9.839	2657	2659	2664	rBV	174	201	0.02%	0.003%
64	9.923	2678	2685	2689	rBB2	339	456	0.05%	0.006%
65	9.949	2690	2693	2696	rBV2	216	164	0.02%	0.002%
66	10.045	2720	2723	2727	rBV	278	214	0.02%	0.003%
67	10.068	2727	2730	2732	rVV2	209	153	0.02%	0.002%
68	10.299	2799	2802	2806	rBV2	261	210	0.02%	0.003%
69	10.566	2881	2885	2887	rVV	186	156	0.02%	0.002%
70	10.756	2931	2944	2963	rVV	293571	475954	48.41%	6.578%
71	10.888	2978	2985	2990	rBV2	598	746	0.08%	0.010%
72	10.965	3003	3009	3014	rBV2	404	440	0.04%	0.006%
73	11.026	3022	3028	3029	rBV	308	312	0.03%	0.004%
74	11.093	3046	3049	3053	rBV	216	216	0.02%	0.003%
75	11.309	3111	3116	3118	rBV	270	229	0.02%	0.003%
76	11.373	3132	3136	3141	rBV3	324	306	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057400.D
 Acq On : 08 Jan 2024 22:20
 Operator : MD/SY
 Sample : 05787-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

77	11.483	3163	3170	3174	rBV2	425	605	0.06%	0.008%
78	11.560	3190	3194	3196	rBV	323	284	0.03%	0.004%
79	11.601	3204	3207	3210	rVB	309	163	0.02%	0.002%
80	11.756	3251	3255	3256	rBV	309	222	0.02%	0.003%
81	11.807	3259	3271	3295	rVV	389364	634651	64.55%	8.771%
82	11.910	3300	3303	3311	rVB4	529	688	0.07%	0.010%
83	11.991	3325	3328	3331	rVB2	522	272	0.03%	0.004%
84	12.142	3367	3375	3377	rBV	355	406	0.04%	0.006%
85	12.190	3377	3390	3414	rBV	387446	645624	65.66%	8.922%
86	12.679	3539	3542	3546	rVB	488	351	0.04%	0.005%
87	12.701	3547	3549	3551	rBV	294	179	0.02%	0.002%
88	12.749	3560	3564	3567	rBV3	382	359	0.04%	0.005%
89	12.769	3567	3570	3579	rVB2	732	762	0.08%	0.011%
90	13.039	3651	3654	3656	rBV	376	207	0.02%	0.003%
91	13.244	3715	3718	3720	rBV	270	157	0.02%	0.002%
92	13.312	3737	3739	3743	rBV2	233	167	0.02%	0.002%
93	13.450	3780	3782	3785	rVB2	431	206	0.02%	0.003%
94	13.592	3822	3826	3828	rBV	220	198	0.02%	0.003%
95	13.994	3948	3951	3954	rBV	483	315	0.03%	0.004%
96	14.187	4008	4011	4014	rBV2	370	270	0.03%	0.004%
97	14.270	4033	4037	4038	rBV3	383	270	0.03%	0.004%
98	14.334	4055	4057	4059	rVB	509	210	0.02%	0.003%
99	14.351	4059	4062	4065	rBV2	544	390	0.04%	0.005%
100	14.801	4198	4202	4206	rBV3	836	705	0.07%	0.010%




Sum of corrected areas: 7236078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057400.D
Acq On : 08 Jan 2024 22:20
Operator : MD/SY
Sample : 05787-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

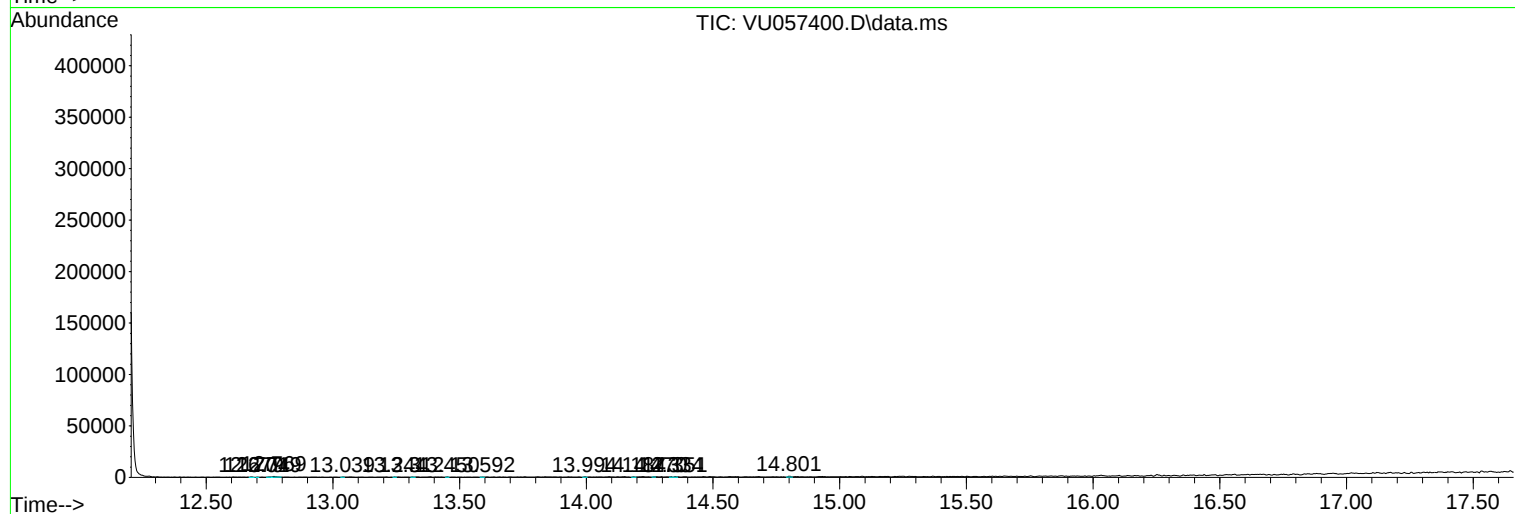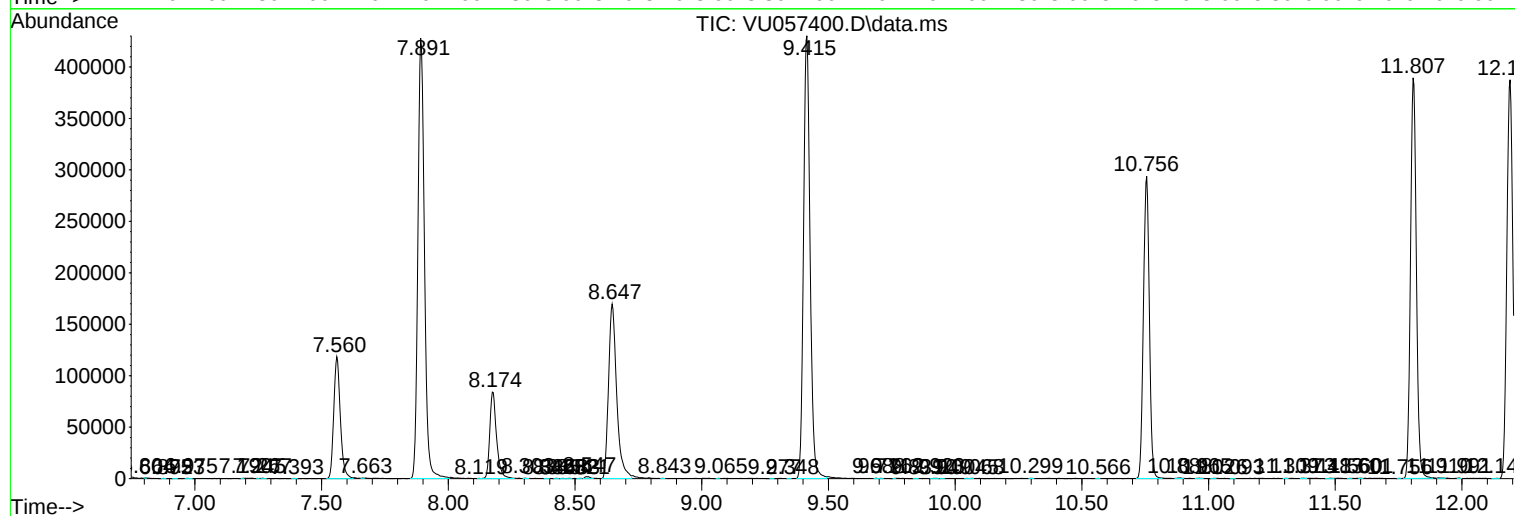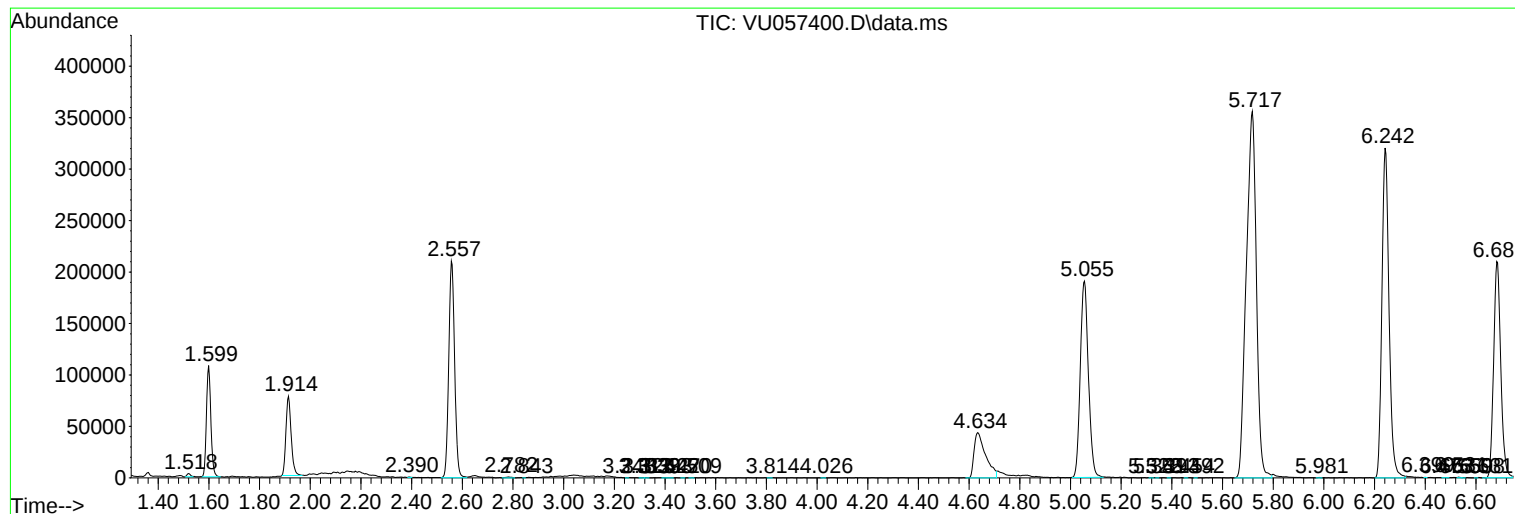

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057400.D
Acq On : 08 Jan 2024 22:20
Operator : MD/SY
Sample : 05787-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057400.D
Acq On : 08 Jan 2024 22:20
Operator : MD/SY
Sample : 05787-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------