

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057401.D
 Acq On : 08 Jan 2024 22:44
 Operator : MD/SY
 Sample : 05787-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

Signal : TIC: VU057401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	17	21	29	rBV5	3674	4093	0.41%	0.056%
2	1.599	88	96	111	rVB	105737	128826	12.98%	1.767%
3	1.914	186	194	212	rVB	75014	110561	11.14%	1.516%
4	2.557	381	394	411	rBV	208389	339190	34.18%	4.652%
5	2.641	412	420	421	rBV3	1630	1639	0.17%	0.022%
6	2.782	457	464	473	rVB3	679	1128	0.11%	0.015%
7	2.859	484	488	491	rVV2	287	288	0.03%	0.004%
8	2.891	493	498	502	rBV3	446	461	0.05%	0.006%
9	3.515	688	692	696	rBV	175	183	0.02%	0.003%
10	3.846	792	795	798	rBV	196	184	0.02%	0.003%
11	3.901	810	812	815	rVV	274	185	0.02%	0.003%
12	3.946	823	826	828	rVB2	308	180	0.02%	0.002%
13	4.055	858	860	864	rBB	263	185	0.02%	0.003%
14	4.303	934	937	940	rBV2	278	199	0.02%	0.003%
15	4.637	1029	1041	1077	rBV	40831	145839	14.70%	2.000%
16	4.962	1137	1142	1146	rVB3	547	465	0.05%	0.006%
17	4.988	1146	1150	1155	rVB2	474	384	0.04%	0.005%
18	5.052	1155	1170	1198	rBV	189788	432485	43.58%	5.932%
19	5.190	1211	1213	1215	rBV	296	199	0.02%	0.003%
20	5.313	1247	1251	1253	rBV	308	213	0.02%	0.003%
21	5.486	1302	1305	1307	rBV	277	195	0.02%	0.003%
22	5.714	1356	1376	1406	rBV2	364262	992390	100.00%	13.611%
23	5.952	1444	1450	1451	rBV	276	272	0.03%	0.004%
24	6.110	1495	1499	1500	rBV	543	294	0.03%	0.004%
25	6.242	1525	1540	1562	rBV	327638	638312	64.32%	8.755%
26	6.419	1590	1595	1597	rBV2	325	266	0.03%	0.004%
27	6.486	1613	1616	1619	rBV	395	211	0.02%	0.003%
28	6.525	1624	1628	1631	rBV3	842	649	0.07%	0.009%
29	6.605	1651	1653	1655	rBV	304	180	0.02%	0.002%
30	6.628	1659	1660	1663	rVB	509	183	0.02%	0.003%
31	6.682	1663	1677	1697	rBV2	214077	422858	42.61%	5.800%
32	6.776	1703	1706	1710	rVV3	702	458	0.05%	0.006%
33	6.801	1712	1714	1723	rVB4	973	1040	0.10%	0.014%
34	6.946	1756	1759	1762	rBV	225	198	0.02%	0.003%
35	7.013	1777	1780	1784	rBB	175	174	0.02%	0.002%
36	7.419	1903	1906	1910	rBV	216	213	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057401.D
 Acq On : 08 Jan 2024 22:44
 Operator : MD/SY
 Sample : 05787-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

37	7.560	1938	1950	1968	rBV	116643	218173	21.98%	2.992%
38	7.702	1990	1994	1996	rBV3	395	293	0.03%	0.004%
39	7.740	2003	2006	2010	rBV	373	341	0.03%	0.005%
40	7.775	2014	2017	2019	rBV	286	189	0.02%	0.003%
41	7.891	2040	2053	2086	rBV	426789	771807	77.77%	10.586%
42	8.129	2125	2127	2130	rBV	268	214	0.02%	0.003%
43	8.174	2130	2141	2160	rVV	77423	151347	15.25%	2.076%
44	8.316	2179	2185	2187	rBB	161	180	0.02%	0.002%
45	8.367	2197	2201	2203	rVV	387	230	0.02%	0.003%
46	8.393	2207	2209	2212	rBV	347	200	0.02%	0.003%
47	8.480	2233	2236	2239	rBV	314	229	0.02%	0.003%
48	8.547	2252	2257	2264	rBV5	1926	2490	0.25%	0.034%
49	8.592	2268	2271	2275	rBV	202	233	0.02%	0.003%
50	8.650	2275	2289	2319	rBV2	162734	373937	37.68%	5.129%
51	8.827	2340	2344	2352	rVB2	586	701	0.07%	0.010%
52	9.245	2470	2474	2480	rVB	369	436	0.04%	0.006%
53	9.338	2499	2503	2506	rBB	235	186	0.02%	0.003%
54	9.415	2509	2527	2549	rBV	424117	775363	78.13%	10.635%
55	9.582	2576	2579	2581	rBV	354	243	0.02%	0.003%
56	9.701	2613	2616	2619	rVB2	379	244	0.02%	0.003%
57	9.766	2631	2636	2638	rBV2	464	353	0.04%	0.005%
58	9.817	2650	2652	2655	rBB	341	232	0.02%	0.003%
59	9.836	2655	2658	2661	rBV	236	212	0.02%	0.003%
60	10.004	2707	2710	2713	rVB	380	274	0.03%	0.004%
61	10.123	2745	2747	2752	rBV	325	262	0.03%	0.004%
62	10.222	2775	2778	2781	rBB	253	187	0.02%	0.003%
63	10.251	2781	2787	2790	rBB	390	375	0.04%	0.005%
64	10.280	2791	2796	2799	rBB	244	240	0.02%	0.003%
65	10.322	2806	2809	2818	rBV	145	197	0.02%	0.003%
66	10.402	2832	2834	2840	rVB	244	186	0.02%	0.003%
67	10.476	2854	2857	2859	rBV	218	174	0.02%	0.002%
68	10.496	2861	2863	2865	rVV	443	194	0.02%	0.003%
69	10.570	2881	2886	2889	rBV	321	250	0.03%	0.003%
70	10.756	2931	2944	2965	rVV	290699	473201	47.68%	6.490%
71	10.859	2970	2976	2979	rBV3	358	297	0.03%	0.004%
72	10.878	2979	2982	2983	rBV2	351	202	0.02%	0.003%
73	10.894	2983	2987	2991	rVB2	350	311	0.03%	0.004%
74	10.930	2996	2998	3005	rVB	340	275	0.03%	0.004%
75	10.965	3006	3009	3011	rBV	221	175	0.02%	0.002%
76	11.129	3057	3060	3062	rBV	312	201	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
 Data File : VU057401.D
 Acq On : 08 Jan 2024 22:44
 Operator : MD/SY
 Sample : 05787-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCMF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

77	11.245	3093	3096	3099	rBV	207	205	0.02%	0.003%
78	11.476	3162	3168	3170	rBV	423	325	0.03%	0.004%
79	11.611	3207	3210	3212	rBV	295	197	0.02%	0.003%
80	11.807	3259	3271	3291	rBV	401138	634262	63.91%	8.699%
81	12.190	3375	3390	3408	rBV	400875	649129	65.41%	8.903%
82	12.348	3433	3439	3442	rBV4	440	425	0.04%	0.006%
83	12.663	3534	3537	3540	rBV	243	178	0.02%	0.002%
84	12.872	3598	3602	3606	rBV	274	206	0.02%	0.003%
85	13.151	3687	3689	3696	rVB	455	392	0.04%	0.005%
86	13.434	3774	3777	3778	rBV	514	297	0.03%	0.004%
87	13.505	3796	3799	3800	rBV	331	176	0.02%	0.002%
88	13.586	3821	3824	3826	rBV	299	174	0.02%	0.002%
89	13.708	3859	3862	3865	rVB3	301	202	0.02%	0.003%
90	13.766	3877	3880	3882	rBV	336	174	0.02%	0.002%
91	13.856	3906	3908	3910	rBV	460	260	0.03%	0.004%
92	14.203	4013	4016	4019	rBV2	345	232	0.02%	0.003%
93	14.508	4108	4111	4115	rBV	426	410	0.04%	0.006%
94	14.643	4150	4153	4154	rBV	396	227	0.02%	0.003%
95	14.721	4174	4177	4182	rVB2	694	417	0.04%	0.006%
96	14.756	4182	4188	4191	rBV2	504	516	0.05%	0.007%
97	14.949	4245	4248	4257	rVB2	939	1125	0.11%	0.015%
98	14.994	4257	4262	4263	rBV2	543	467	0.05%	0.006%
99	15.521	4423	4426	4431	rBV3	958	871	0.09%	0.012%
100	15.682	4472	4476	4478	rBV3	598	509	0.05%	0.007%




Sum of corrected areas: 7290990

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057401.D
Acq On : 08 Jan 2024 22:44
Operator : MD/SY
Sample : 05787-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

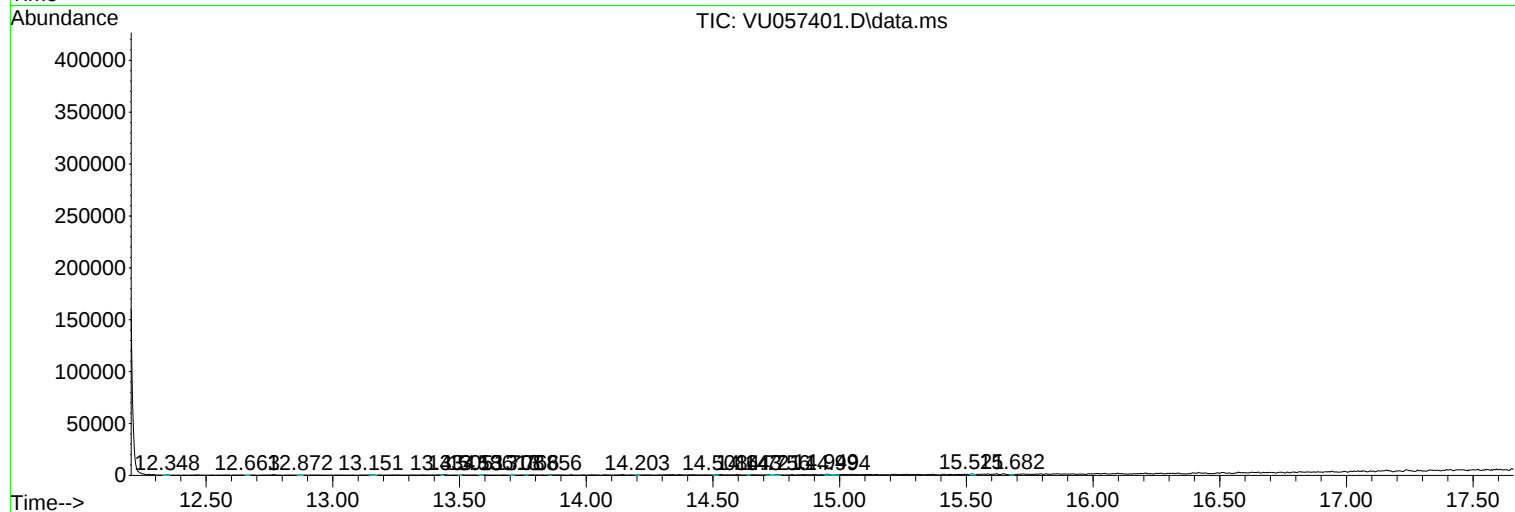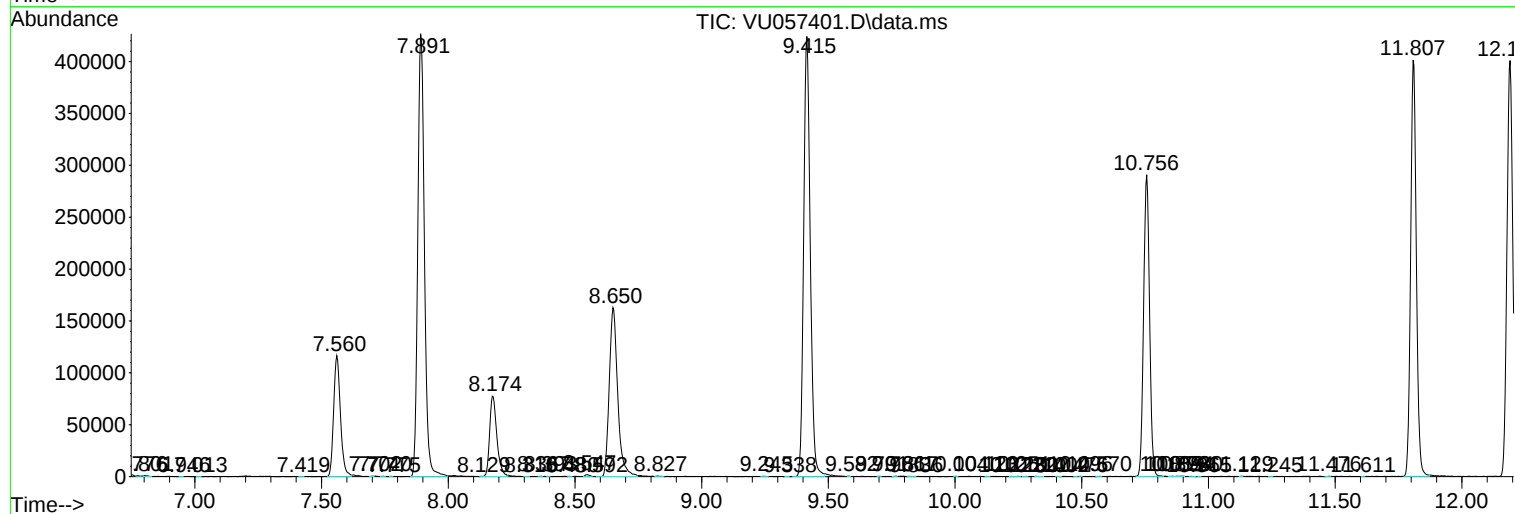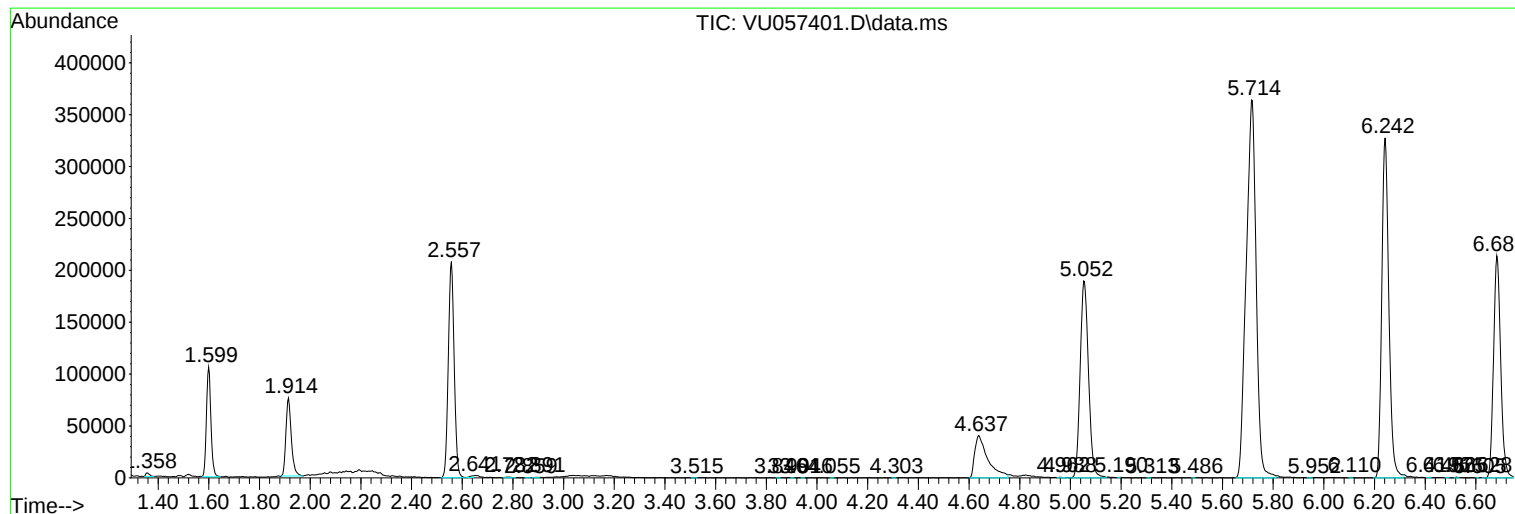

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057401.D
Acq On : 08 Jan 2024 22:44
Operator : MD/SY
Sample : 05787-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057401.D
Acq On : 08 Jan 2024 22:44
Operator : MD/SY
Sample : 05787-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCMF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------