


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010824\
Data File : VU057375.D
Acq On : 08 Jan 2024 10:54
Operator : MD/SY
Sample : BFB031
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB031

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Title : VOC Analysis
Last Update : Tue Jan 09 06:09:25 2024

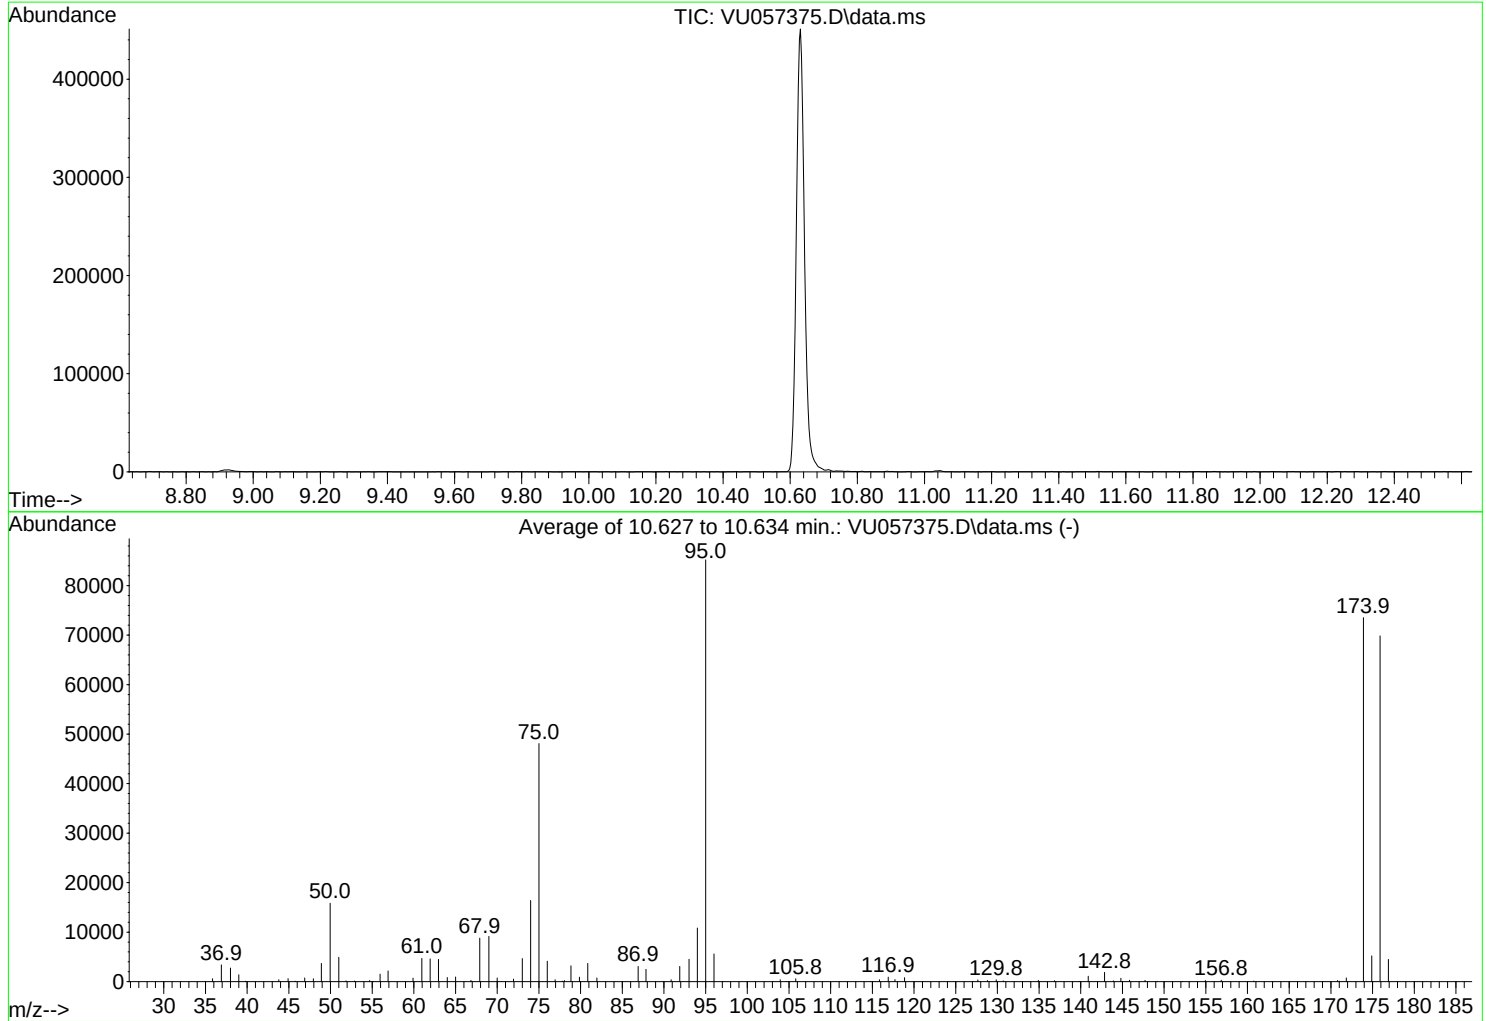

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	15851	PASS
75	95	30	80	56.5	48109	PASS
95	95	100	100	100.0	85208	PASS
96	95	5	9	6.6	5595	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.3	73520	PASS
175	174	5	9	7.1	5223	PASS
176	174	95	101	95.0	69864	PASS
177	176	5	9	6.5	4509	PASS

m/z	Abundance
43.80	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.80	604.0
36.90	3546.0
38.00	2790.0
39.00	1513.0
43.90	524.0
44.90	657.0
46.90	685.0
47.90	599.0
48.90	3914.0
49.90	16001.0
51.00	4850.0
51.90	181.0
52.90	171.0
54.70	225.0
55.90	1559.0
56.90	2268.0
60.00	818.0
61.00	5015.0
61.90	4636.0
62.90	4259.0
64.00	820.0
65.00	837.0
66.90	268.0
67.90	8798.0
69.00	9378.0
70.00	781.0
71.90	610.0
73.00	4809.0
74.00	16552.0
75.00	48856.0
76.00	4209.0
76.90	373.0
78.10	348.0
78.90	3345.0
79.80	962.0
80.80	3679.0
81.90	708.0
86.90	3276.0
87.80	2478.0
90.90	425.0
91.90	3026.0
93.00	4601.0
94.00	11005.0
95.00	85992.0
96.00	5643.0
103.90	429.0
104.70	122.0
105.80	607.0
114.80	113.0
115.90	332.0
116.90	1067.0
117.70	423.0
118.90	751.0
127.60	338.0
128.80	217.0
129.80	360.0
130.70	188.0
134.90	224.0
136.90	203.0
139.80	117.0
140.90	1216.0
142.80	1856.0
143.90	188.0
144.80	791.0
145.90	243.0
147.70	250.0
149.10	132.0
154.90	229.0
156.80	265.0
160.80	126.0
170.90	348.0
171.90	704.0
173.90	73336.0
174.90	5231.0
175.90	68920.0
176.90	4545.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.80	558.0
36.90	3501.0
38.00	2754.0
39.00	1453.0
39.80	155.0
43.80	589.0
44.90	636.0
45.70	121.0
46.90	803.0
47.90	593.0
48.90	3788.0
49.90	16504.0
51.00	5103.0
51.90	161.0
52.90	155.0
54.70	227.0
55.10	164.0
55.90	1574.0
56.90	2235.0
59.90	727.0
61.00	4837.0
61.90	4676.0
63.00	4651.0
64.00	901.0
65.00	1005.0
66.90	293.0
67.90	8963.0
69.00	9450.0
70.00	734.0
72.00	582.0
73.00	4830.0
74.00	16928.0
75.00	49632.0
76.00	4258.0
77.00	391.0
78.00	307.0
78.80	3152.0
79.80	929.0
80.80	3807.0
81.90	766.0
86.90	3214.0
87.90	2566.0
90.80	404.0
91.90	3227.0
93.00	4794.0
94.00	11164.0
95.00	87480.0
96.00	5688.0
97.00	116.0
103.90	405.0
104.90	102.0
105.80	601.0
115.90	386.0
116.90	923.0
117.70	443.0
118.80	872.0
127.60	359.0
128.80	248.0
129.80	418.0
130.70	165.0
134.90	303.0
136.80	208.0
139.80	113.0
140.90	1136.0
142.90	1990.0
143.90	164.0
144.80	697.0
145.90	314.0
147.70	265.0
149.20	111.0
152.20	100.0
154.90	221.0
156.90	328.0
160.70	122.0
170.70	298.0
171.90	701.0
173.90	75560.0
174.90	5360.0
175.90	71864.0
176.90	4706.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.90	546.0
36.90	3141.0
38.00	2687.0
39.00	1251.0
39.80	140.0
43.80	560.0
44.90	591.0
45.80	142.0
46.90	745.0
48.00	533.0
48.90	3346.0
50.00	15048.0
51.00	4792.0
51.80	129.0
52.90	105.0
54.70	202.0
56.00	1412.0
56.90	2019.0
59.80	624.0
60.90	4228.0
62.00	4468.0
63.00	4531.0
64.00	820.0
65.00	990.0
66.80	248.0
67.90	8639.0
69.00	8621.0
70.00	740.0
72.00	410.0
73.00	4303.0
74.00	15677.0
75.00	45840.0
76.00	3986.0
77.00	439.0
77.80	331.0
78.80	3068.0
79.90	859.0
80.90	3594.0
82.00	785.0
86.90	2770.0
87.90	2467.0
90.80	392.0
91.90	3008.0
93.00	4223.0
94.00	10341.0
95.00	82152.0
96.00	5454.0
97.10	129.0
104.00	374.0
105.00	118.0
105.80	529.0
115.80	457.0
116.90	725.0
117.70	452.0
118.90	830.0
127.70	340.0
128.80	232.0
129.90	441.0
130.70	107.0
134.90	294.0
136.80	220.0
140.90	944.0
142.90	1764.0
143.90	124.0
144.80	595.0
145.80	324.0
147.70	239.0
155.00	231.0
156.90	296.0
160.70	104.0
171.00	255.0
171.80	794.0
173.90	71664.0
174.90	5077.0
175.90	68808.0
176.90	4275.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031