

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010919\  
 Data File : VU029086.D  
 Acq On : 09 Jan 2019 13:48  
 Operator : MD/SY  
 Sample : PB116248ZHE#01  
 Misc : 5.0mL/MSVOA U/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :

Quant Time: Jan 10 04:04:42 2019  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\82U010319W.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Jan 04 02:22:53 2019  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 4.98  | 168  | 113550   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 5.88  | 114  | 197178   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 9.09  | 117  | 185899   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 11.48 | 152  | 74755    | 50.00 | ug/l  | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc  | Units   | Dev(Min) |
|-----------------------------|-------|------|----------|-------|---------|----------|
| 33) 1,2-Dichloroethane-d4   | 5.31  | 65   | 75629    | 53.88 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 107.76% |          |
| 35) Dibromofluoromethane    | 4.88  | 113  | 67613    | 52.90 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 105.80% |          |
| 50) Toluene-d8              | 7.56  | 98   | 254079   | 50.35 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 100.70% |          |
| 62) 4-Bromofluorobenzene    | 10.30 | 95   | 79632    | 43.91 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 87.82%  |          |


| Target Compounds               | R.T.  | QIon | Response | Conc      | Units  | Qvalue |
|--------------------------------|-------|------|----------|-----------|--------|--------|
| 3) Chloromethane               | 1.33  | 50   | 665      | Below Cal |        | 98     |
| 5) Bromomethane                | 1.63  | 94   | 20       | Below Cal | #      | 2      |
| 11) Tert butyl alcohol         | 2.83  | 59   | 129      | 0.362     | ug/l # | 73     |
| 16) Acetone                    | 2.32  | 43   | 5840     | 6.604     | ug/l   | 100    |
| 17) Carbon Disulfide           | 2.48  | 76   | 415      | Below Cal | #      | 75     |
| 18) Methyl Acetate             | 2.62  | 43   | 1302     | 0.633     | ug/l # | 54     |
| 20) Methylene Chloride         | 2.70  | 84   | 2108     | 1.404     | ug/l   | 95     |
| 31) Cyclohexane                | 4.98  | 56   | 1914     | Below Cal | #      | 1      |
| 36) 1,1-Dichloropropene        | 4.98  | 75   | 8304     | 4.213     | ug/l # | 45     |
| 38) Carbon Tetrachloride       | 4.98  | 117  | 10154    | 6.177     | ug/l # | 17     |
| 43) Isopropyl Acetate          | 5.55  | 43   | 9620     | 2.899     | ug/l   | 96     |
| 45) 1,2-Dichloropropane        | 6.70  | 63   | 672      | 0.414     | ug/l # | 43     |
| 48) Methyl methacrylate        | 6.70  | 41   | 56304    | 34.844    | ug/l # | 37     |
| 51) 4-Methyl-2-Pentanone       | 7.56  | 43   | 5054     | 2.238     | ug/l   | 96     |
| 54) cis-1,3-Dichloropropene    | 7.42  | 75   | 24209    | 9.760     | ug/l # | 60     |
| 57) 1,3-Dichloropropane        | 8.41  | 76   | 5474     | 2.134     | ug/l # | 42     |
| 59) 2-Hexanone                 | 8.31  | 43   | 7518     | 4.241     | ug/l # | 21     |
| 74) N-amyl acetate             | 9.76  | 43   | 7053     | 2.958     | ug/l # | 48     |
| 76) 1,2,3-Trichloropropane     | 10.30 | 75   | 37726    | 20.597    | ug/l # | 36     |
| 81) trans-1,4-Dichloro-2-buten | 10.30 | 75   | 37726    | 53.121    | ug/l # | 100    |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU010919\  
Data File : VU029086.D  
Acq On : 09 Jan 2019 13:48  
Operator : MD/SY  
Sample : PB116248ZHE#01  
Misc : 5.0mL/MSVOA U/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :

Quant Time: Jan 10 04:04:42 2019  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_U\METHOD\82U010319W.M  
Quant Title : SW846 8260  
QLast Update : Fri Jan 04 02:22:53 2019  
Response via : Initial Calibration

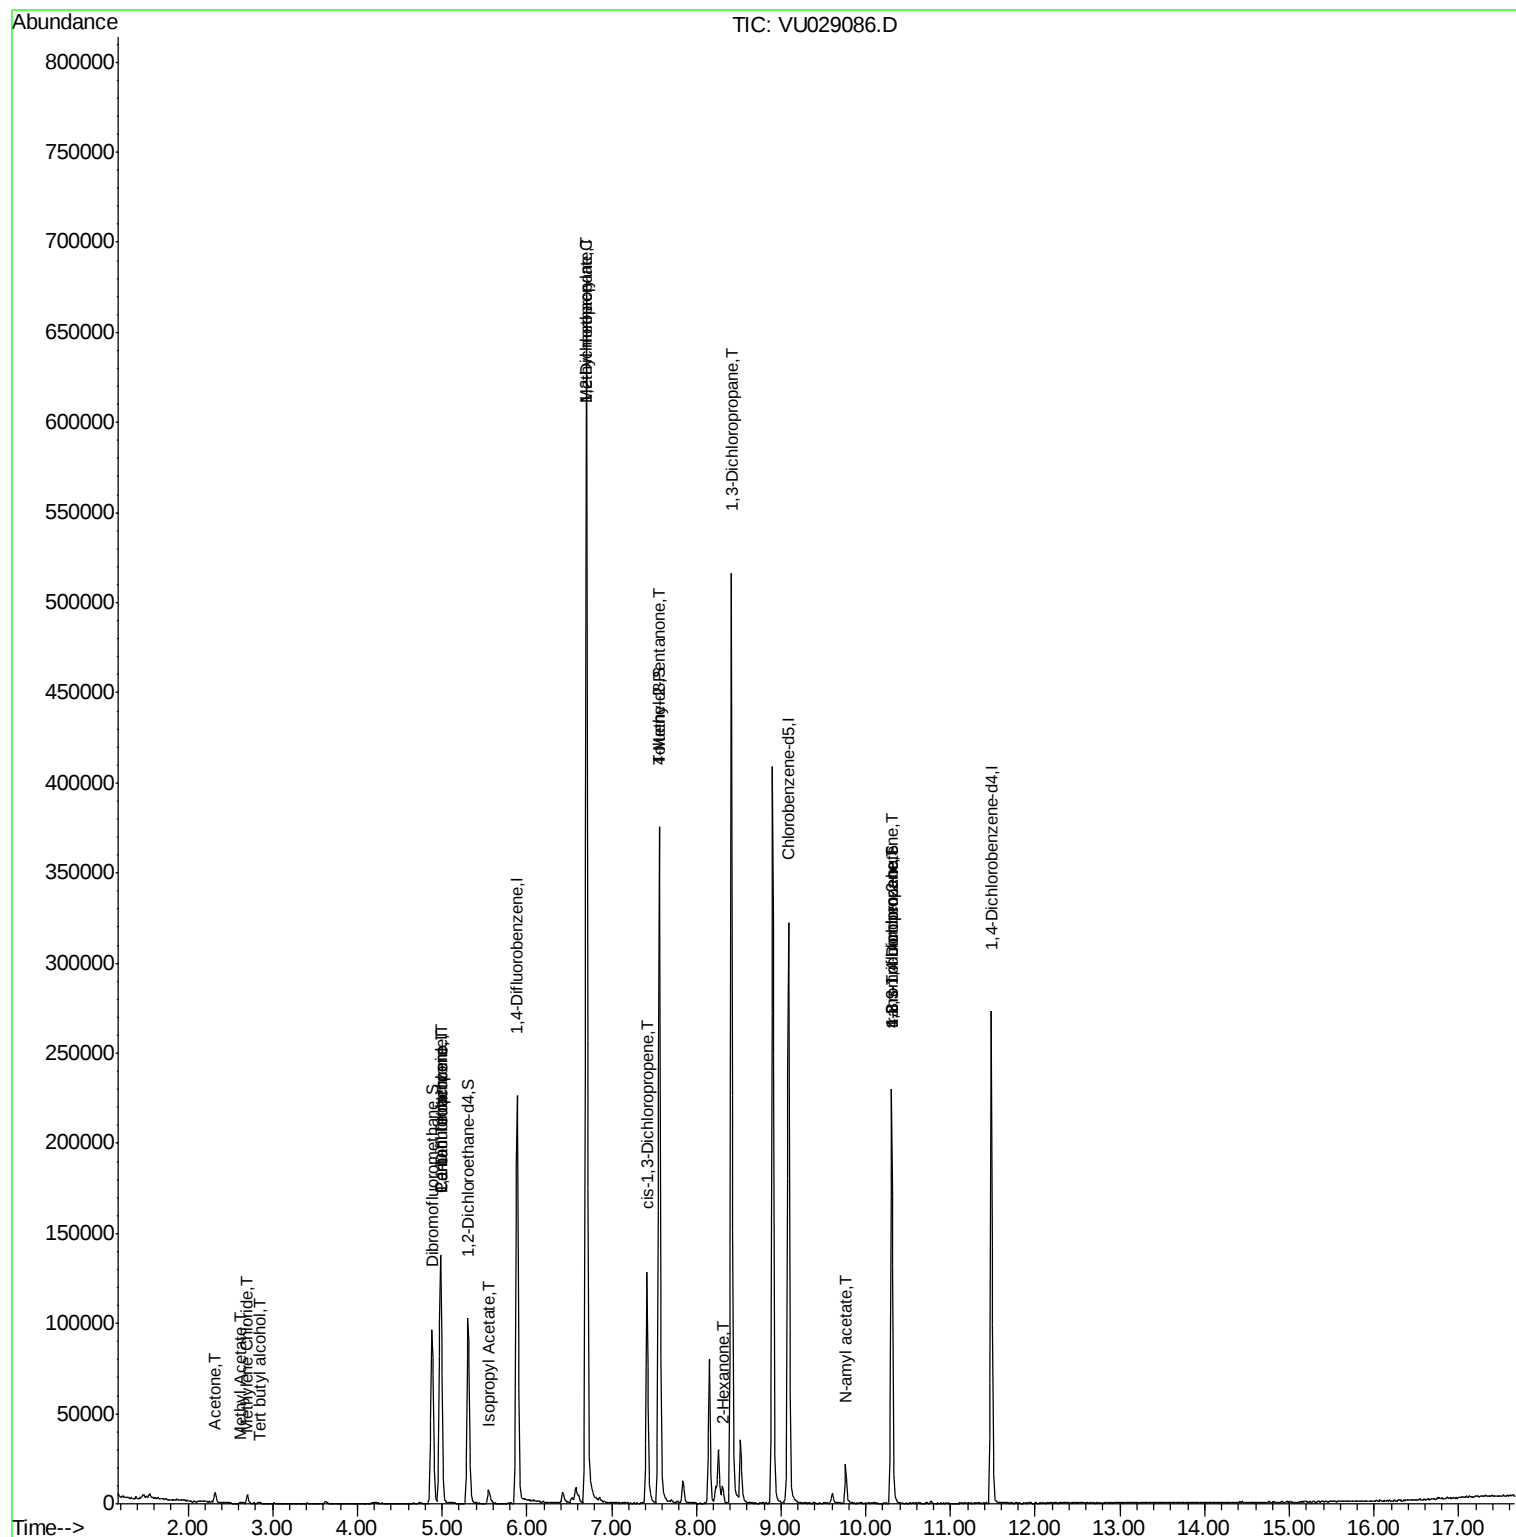

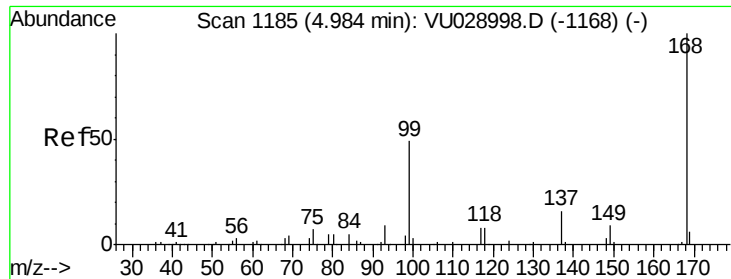

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1185

Delta R.T. 0.00 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48


Instrument :  
MSVOA\_U  
ClientSampleId :

Tot Ion:168 Resp: 113550

Ion Ratio Lower Upper




168 100

99 52.3 42.0 63.0



Abundance Ion 167.90 (167.60 to 168.60): VU028998.D (-1168) (-)

Ion 98.90 (98.60 to 99.60): VU028998.D (-1168) (-)

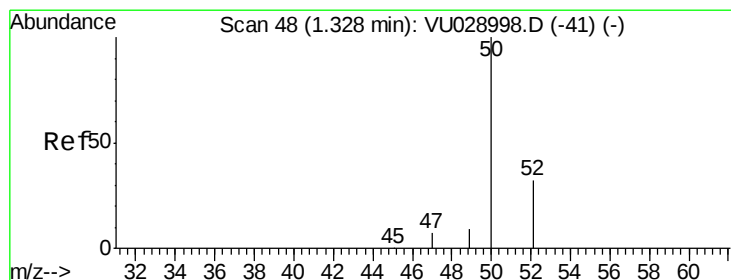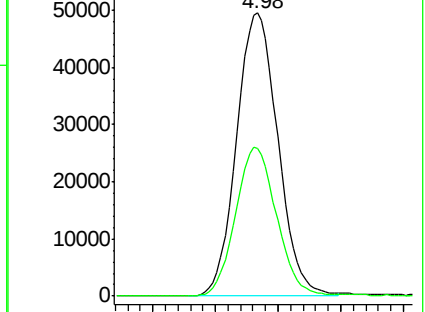

#3

Chloromethane

Concen: Below Cal

RT: 1.33 min Scan# 48

Delta R.T. 0.00 min

Lab File: VU029086.D


Acq: 09 Jan 2019 13:48

Tgt Ion: 50 Resp: 665

Ion Ratio Lower Upper



50 100


52 33.8 26.1 39.1

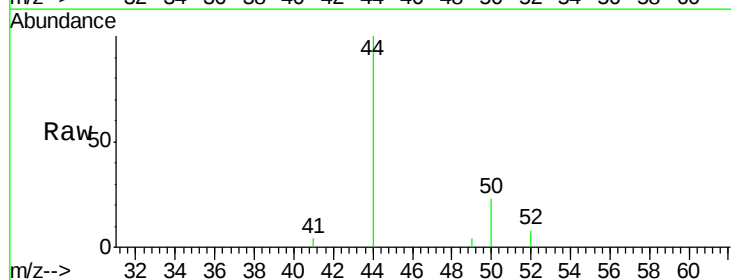

Abundance Ion 49.90 (49.60 to 50.60): VU028998.D (-41) (-)

Ion 51.90 (51.60 to 52.60): VU028998.D (-41) (-)

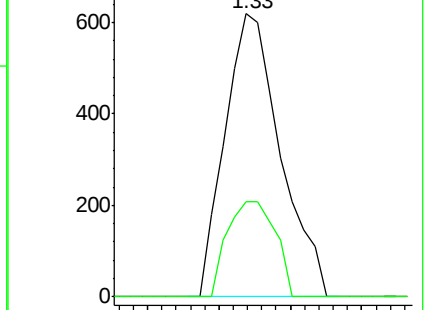

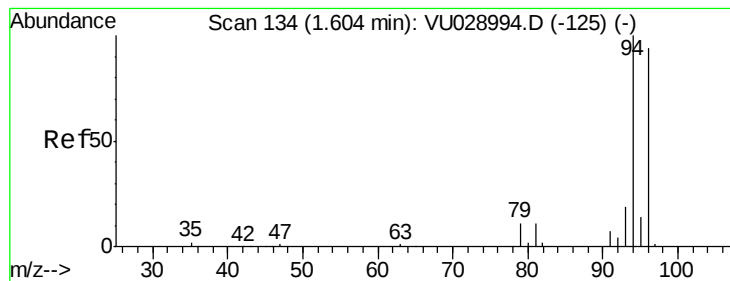

#5

Bromomethane

Concen: Below Cal

RT: 1.63 min Scan# 142

Delta R.T. 0.03 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48


Instrument :  
MSVOA\_U  
ClientSampled :

Tot Ion: 94 Resp: 20

Ion Ratio Lower Upper

94 100

96 0.0 75.5 113.3#

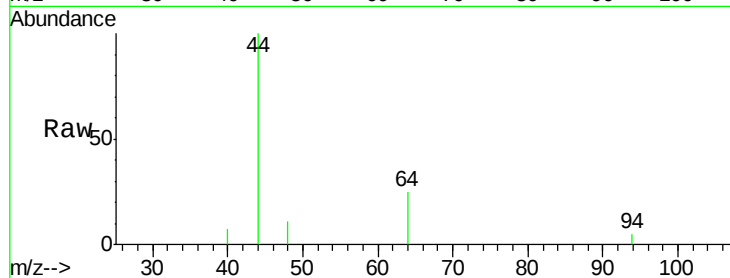


Abundance Ion 93.90 (93.60 to 94.60): VU028994.D (-125) (-)

Ion 95.90 (95.60 to 96.60): VU028994.D (-125) (-)

1.63

Time-->

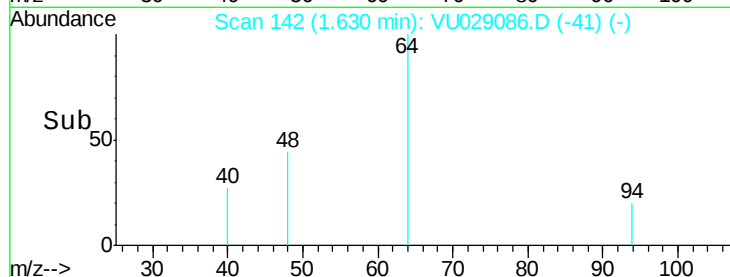


Abundance Ion 93.90 (93.60 to 94.60): VU029086.D (-41) (-)

Ion 95.90 (95.60 to 96.60): VU029086.D (-41) (-)

1.63

Time-->

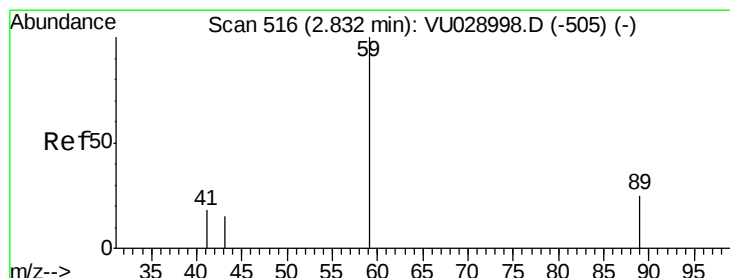

#11

Tert butyl alcohol

Concen: 0.362 ug/l

RT: 2.83 min Scan# 515

Delta R.T. -0.00 min

Lab File: VU029086.D


Acq: 09 Jan 2019 13:48

Tgt Ion: 59 Resp: 129

Ion Ratio Lower Upper

59 100

57 0.0 7.9 11.9#

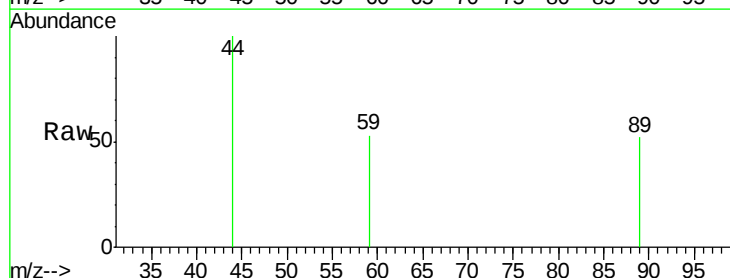


Abundance Ion 59.00 (58.70 to 59.70): VU028998.D (-505) (-)

Ion 57.00 (56.70 to 57.70): VU028998.D (-505) (-)

2.83

Time-->

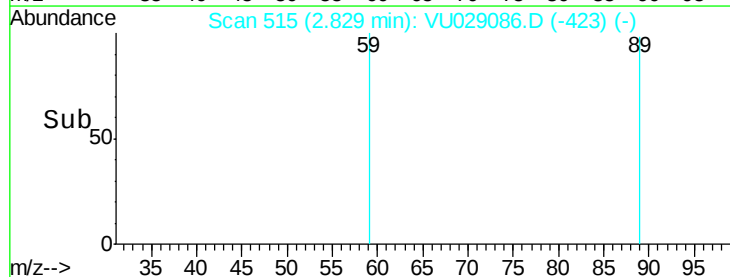


Abundance Ion 59.00 (58.70 to 59.70): VU029086.D (-423) (-)

Ion 57.00 (56.70 to 57.70): VU029086.D (-423) (-)

2.83

Time-->

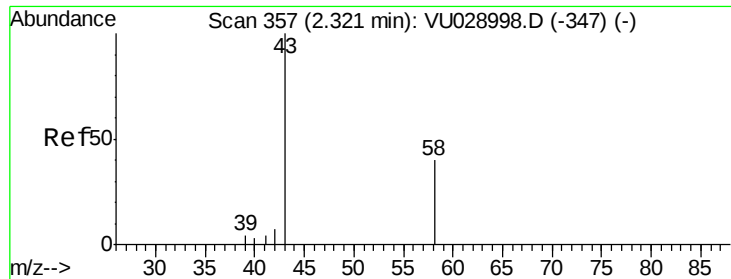

#16

Acetone

Concen: 6.604 ug/l

RT: 2.32 min Scan# 357

Delta R.T. -0.00 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48

Instrument :

MSVOA\_U


ClientSampleId :

Tot Ion: 43 Resp: 5840

Ion Ratio Lower Upper

43 100

58 35.5 28.6 42.8



Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

2.32



3000

2000

1000

0

Time--> 2.25 2.30 2.35



#17

Carbon Disulfide

Concen: Below Cal

RT: 2.48 min Scan# 406

Delta R.T. 0.01 min

Lab File: VU029086.D


Acq: 09 Jan 2019 13:48

Tgt Ion: 76 Resp: 415

Ion Ratio Lower Upper

76 100

78 0.0 7.2 10.8#



Abundance Ion 75.90 (75.60 to 76.60): VU0

Ion 77.90 (77.60 to 78.60): VU0

2.48


300


200

100

0

Time--> 2.44 2.46 2.48 2.50







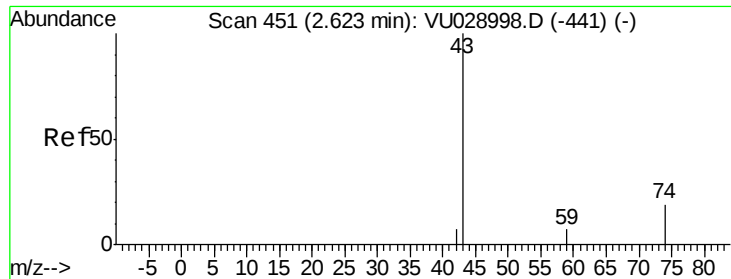

#18  
Methyl Acetate  
Concen: 0.633 ug/l  
RT: 2.62 min Scan# 450  
Delta R.T. 0.01 min  
Lab File: VU029086.D  
Acq: 09 Jan 2019 13:48




Instrument :  
MSVOA\_U  
ClientSampleId :


Tot Ion: 43 Resp: 1302  
Ion Ratio Lower Upper  
43 100  
74 1.6 19.5 29.3#

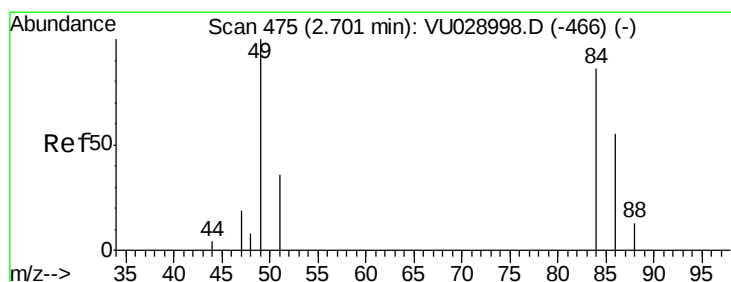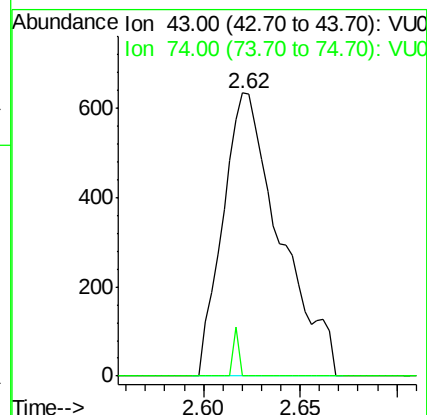

#20  
Methylene Chloride  
Concen: 1.404 ug/l  
RT: 2.70 min Scan# 476  
Delta R.T. 0.01 min  
Lab File: VU029086.D  
Acq: 09 Jan 2019 13:48

Tgt Ion: 84 Resp: 2108  
Ion Ratio Lower Upper  
84 100  
49 117.4 91.9 137.9  
51 39.2 29.2 43.8  
86 57.4 51.8 77.6

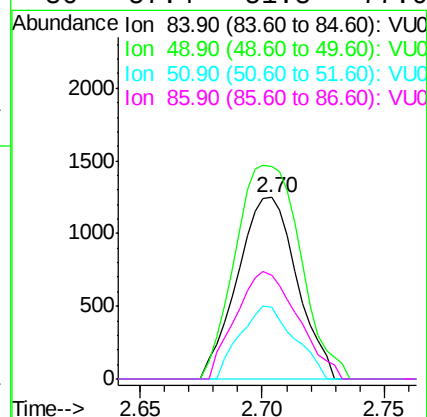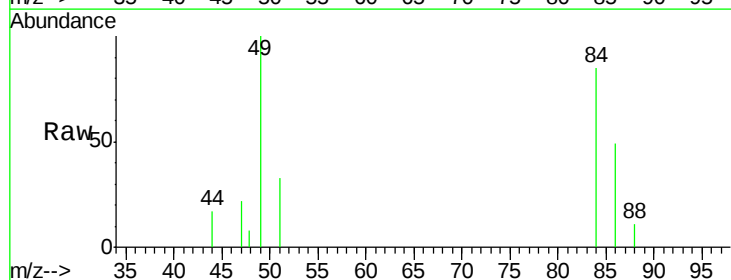

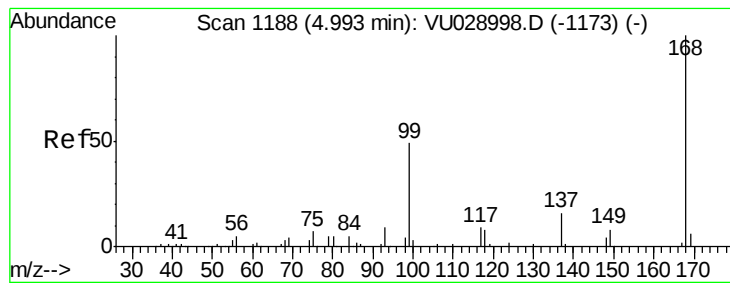

#31

Cyclohexane

Concen: Below Cal

RT: 4.98 min Scan# 1183

Delta R.T. -0.02 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48

Instrument :

MSVOA\_U

ClientSampleId :


Tot Ion: 56 Resp: 1914

Ion Ratio Lower Upper

56 100

69 212.7 26.7 40.1#




84 172.5 65.7 98.5#

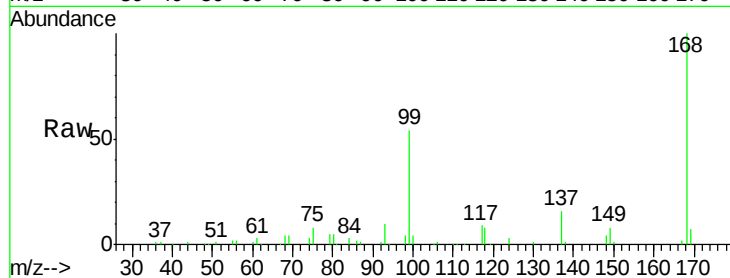

Abundance Ion 56.00 (55.70 to 56.70): VU028998.D (-1173) (-)

Ion 69.00 (68.70 to 69.70): VU028998.D (-1173) (-)

Ion 84.00 (83.70 to 84.70): VU028998.D (-1173) (-)

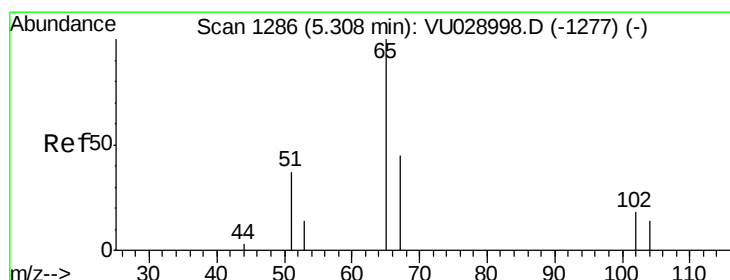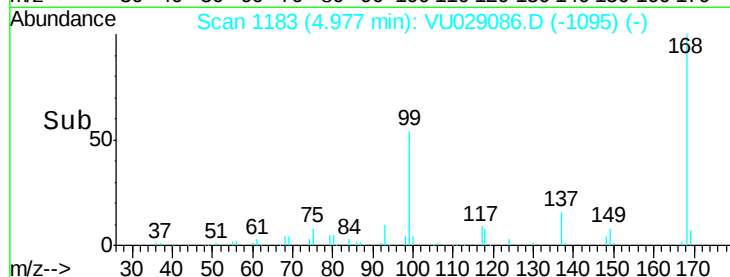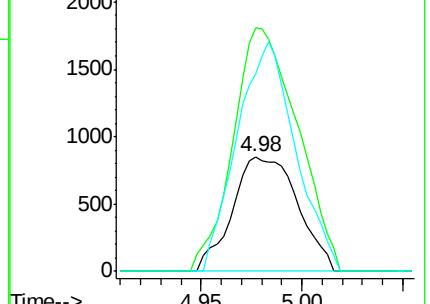

#33

1,2-Dichloroethane-d4

Concen: 53.878 ug/l

RT: 5.31 min Scan# 1286

Delta R.T. 0.00 min

Lab File: VU029086.D


Acq: 09 Jan 2019 13:48

Tgt Ion: 65 Resp: 75629

Ion Ratio Lower Upper



65 100


67 56.7 0.0 111.0

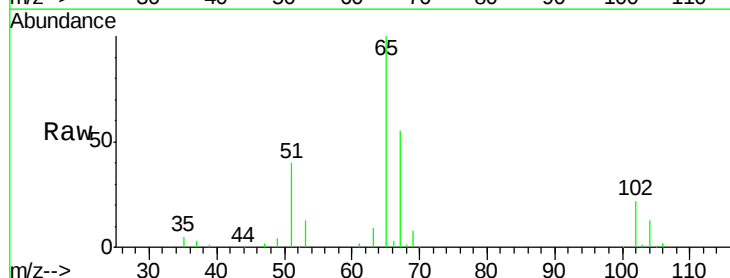

Abundance Ion 64.90 (64.60 to 65.60): VU028998.D (-1277) (-)

Ion 66.90 (66.60 to 67.60): VU028998.D (-1277) (-)

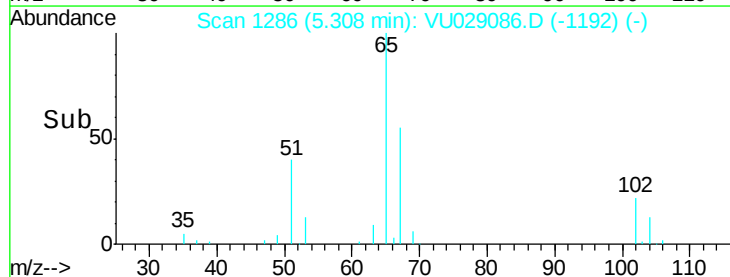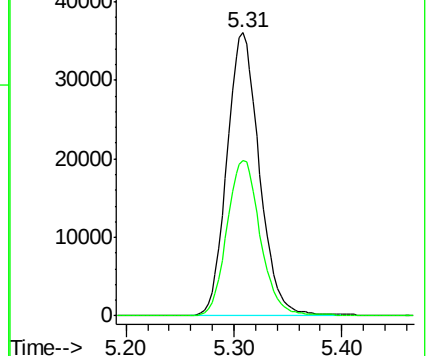


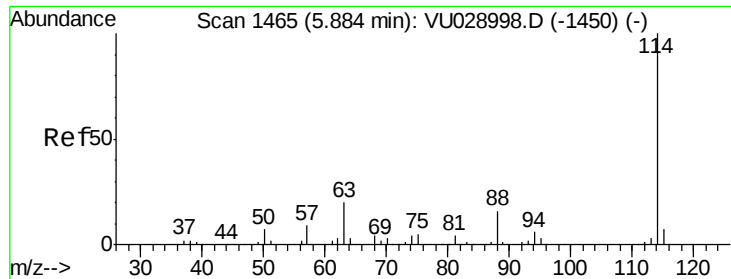




#34  
 1,4-Difluorobenzene  
 Concen: 50.000 ug/l  
 RT: 5.88 min Scan# 1465  
 Delta R.T. -0.00 min  
 Lab File: VU029086.D  
 Acq: 09 Jan 2019 13:48

Instrument :  
 MSVOA\_U  
 ClientSampleId :

Tot Ion:114 Resp: 197178  
 Ion Ratio Lower Upper  
 114 100  
 63 20.7 0.0 40.2  
 88 16.3 0.0 30.4




Abundance Ion 113.90 (113.60 to 114.60): V  
 Ion 63.00 (62.70 to 63.70): VU0  
 Ion 87.90 (87.60 to 88.60): VU0


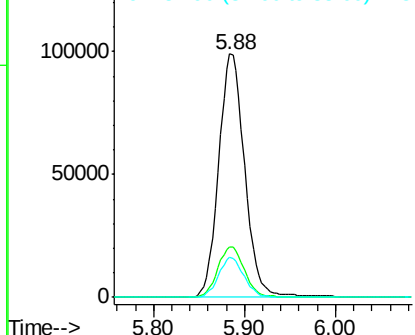



#35  
 Dibromofluoromethane  
 Concen: 52.898 ug/l  
 RT: 4.88 min Scan# 1153  
 Delta R.T. -0.00 min  
 Lab File: VU029086.D  
 Acq: 09 Jan 2019 13:48

Tgt Ion:113 Resp: 67613  
 Ion Ratio Lower Upper  
 113 100  
 111 103.0 81.4 122.2  
 192 20.6 16.8 25.2



Abundance Ion 112.80 (112.50 to 113.50): V  
 Ion 110.80 (110.50 to 111.50): V  
 Ion 191.70 (191.40 to 192.40): V

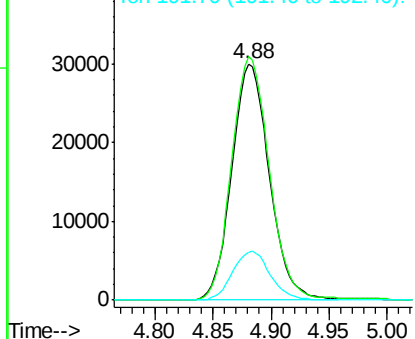


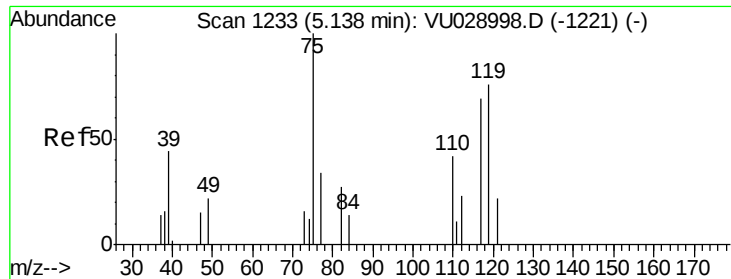




#36  
 1,1-Dichloropropene  
 Concen: 4.213 ug/l  
 RT: 4.98 min Scan# 1185  
 Delta R.T. -0.15 min  
 Lab File: VU029086.D  
 Acq: 09 Jan 2019 13:48

Instrument :  
 MSVOA\_U  
 ClientSampleId :

| Tot Ion   | 75  | Resp  | 8304  |
|-----------|-----|-------|-------|
| Ion Ratio | 100 | Lower | Upper |
| 75        | 100 |       |       |
| 110       | 4.6 | 18.4  | 55.4# |
| 77        | 0.0 | 25.1  | 37.7# |




Abundance Ion 74.90 (74.60 to 75.60): VU028998.D (-1221) (-)  
 Ion 109.90 (109.60 to 110.60): VU028998.D (-1221) (-)  
 Ion 76.90 (76.60 to 77.60): VU028998.D (-1221) (-)


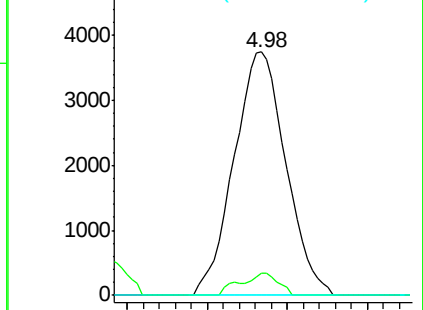



#38  
 Carbon Tetrachloride  
 Concen: 6.177 ug/l  
 RT: 4.98 min Scan# 1185  
 Delta R.T. -0.15 min  
 Lab File: VU029086.D  
 Acq: 09 Jan 2019 13:48

| Tgt Ion                                              | 117 | Resp  | 10154  |
|------------------------------------------------------|-----|-------|--------|
| Ion Ratio <td>100</td> <td>Lower</td> <td>Upper</td> | 100 | Lower | Upper  |
| 117                                                  | 100 |       |        |
| 119                                                  | 4.5 | 74.6  | 111.8# |
| 121                                                  | 0.0 | 25.0  | 37.6#  |



Abundance Ion 116.80 (116.50 to 117.50): VU028998.D (-1221) (-)  
 Ion 118.80 (118.50 to 119.50): VU028998.D (-1221) (-)  
 Ion 120.80 (120.50 to 121.50): VU028998.D (-1221) (-)

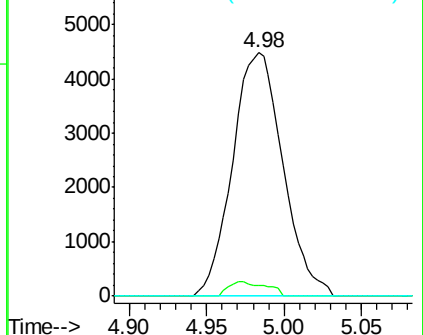



#43

Isopropyl Acetate

Concen: 2.899 ug/l

RT: 5.55 min Scan# 1361

Delta R.T. 0.00 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48

Instrument :

MSVOA\_U

ClientSampled :





Tot Ion: 43 Resp: 9620

Ion Ratio Lower Upper

43 100

61 20.9 17.8 26.6

87 11.3 11.3 16.9

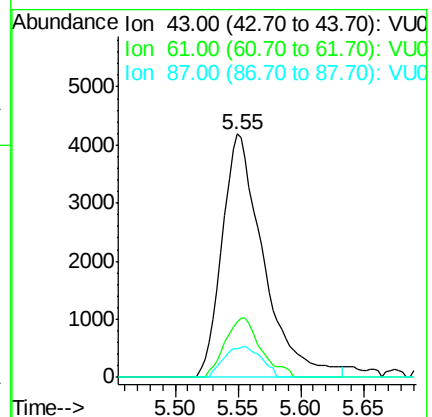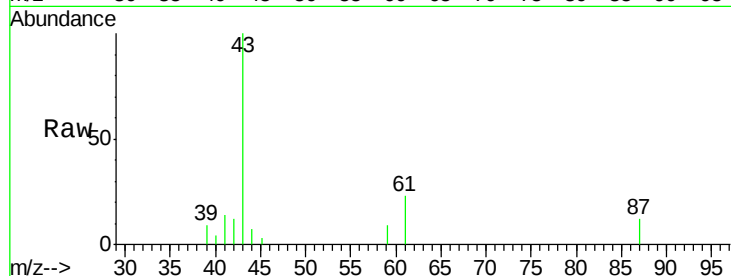

#45

1,2-Dichloropropane

Concen: 0.414 ug/l

RT: 6.70 min Scan# 1718

Delta R.T. 0.27 min

Lab File: VU029086.D




Acq: 09 Jan 2019 13:48


Tgt Ion: 63 Resp: 672

Ion Ratio Lower Upper

63 100

65 0.0 25.1 37.7#

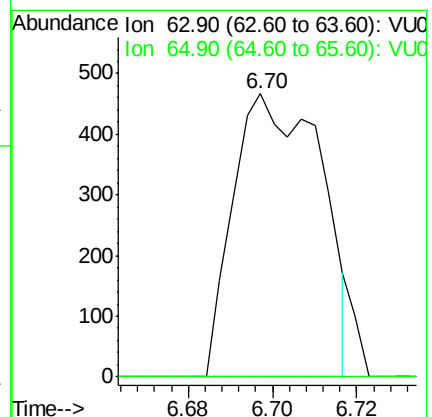



#48

Methvl methacrylate

Concen: 34.844 ug/l

RT: 6.70 min Scan# 1720


Delta R.T. 0.08 min

Lab File: VU029086.D




Acq: 09 Jan 2019 13:48

Instrument :  
MSVOA\_U  
ClientSampleId :

Tot Ion: 41 Resp: 56304  
Ion Ratio Lower Upper  
41 100  
69 0.0 73.6 110.4#  
39 48.8 39.6 59.4

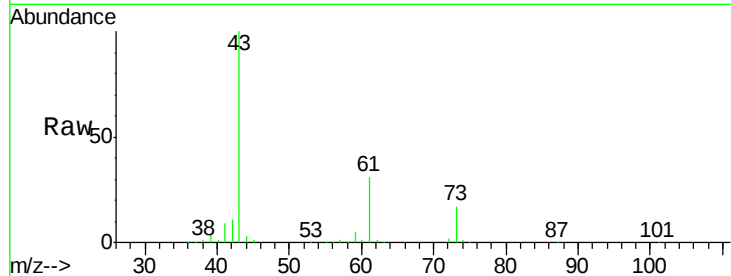

Abundance Ion 41.00 (40.70 to 41.70): VU0  
Ion 69.00 (68.70 to 69.70): VU0  
Ion 39.00 (38.70 to 39.70): VU0

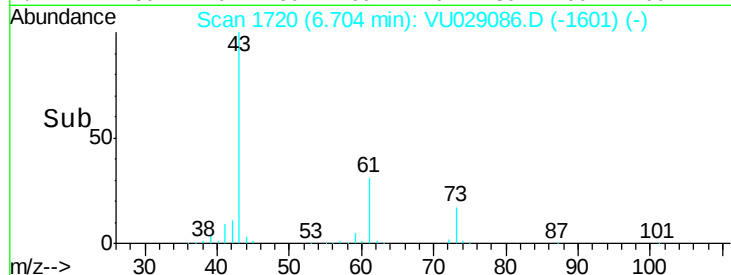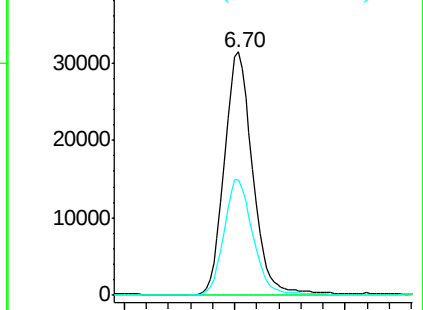

#50

Toluene-d8

Concen: 50.352 ug/l


RT: 7.56 min Scan# 1987

Delta R.T. -0.00 min



Lab File: VU029086.D


Acq: 09 Jan 2019 13:48

Tgt Ion: 98 Resp: 254079  
Ion Ratio Lower Upper  
98 100  
100 63.9 51.6 77.4

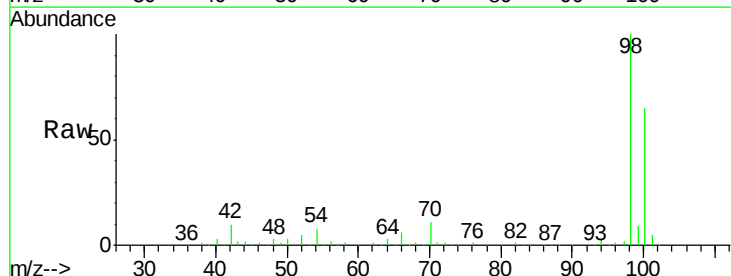

Abundance Ion 98.00 (97.70 to 98.70): VU0  
Ion 100.00 (99.70 to 100.70): VU0

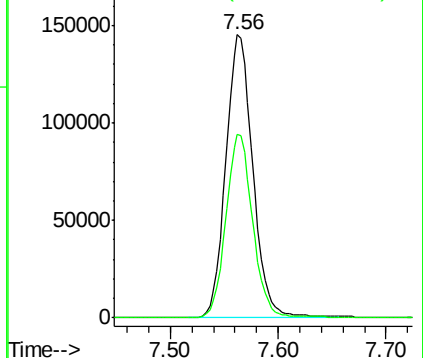

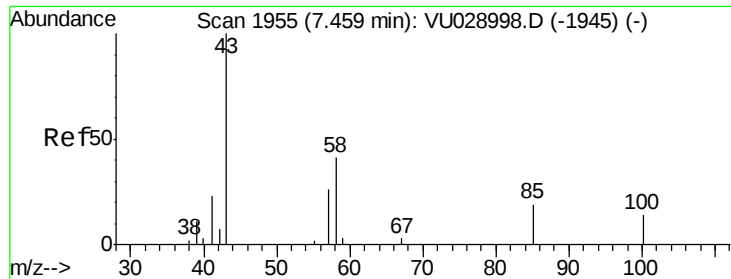

#51

4-Methyl-2-Pentanone

Concen: 2.238 ug/l

RT: 7.56 min Scan# 1986

Delta R.T. 0.10 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48

Instrument :

MSVOA\_U


ClientSampled :

Tot Ion: 43 Resp: 5054

Ion Ratio Lower Upper




43 100

58 39.6 33.9 50.9

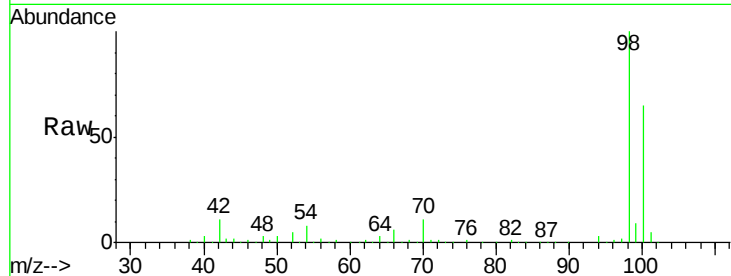

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

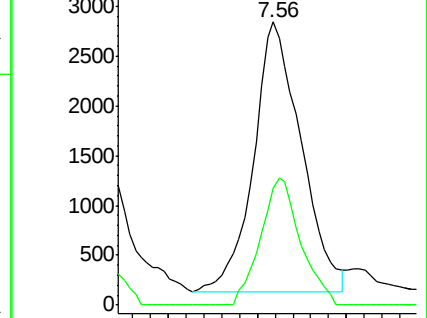

#54

cis-1,3-Dichloropropene

Concen: 9.760 ug/l

RT: 7.42 min Scan# 1943

Delta R.T. 0.15 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48


Tgt Ion: 75 Resp: 24209

Ion Ratio Lower Upper

75 100

77 0.0 25.0 37.6#



39 23.3 32.2 48.4#




Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 76.90 (76.60 to 77.60): VU0

Ion 39.00 (38.70 to 39.70): VU0

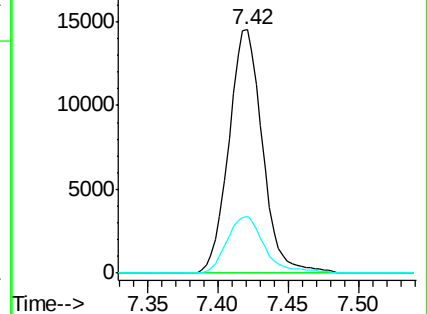

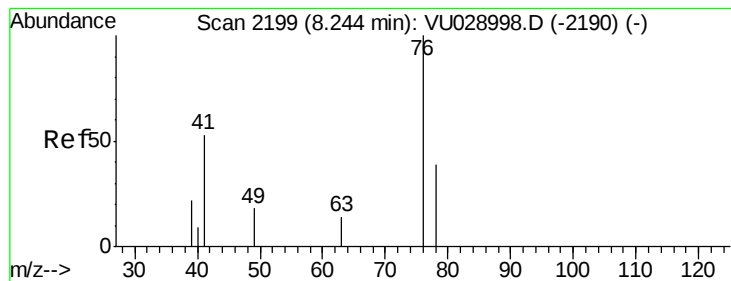

#57

1,3-Dichloropropane

Concen: 2.134 ug/l

RT: 8.41 min Scan# 2252

Delta R.T. 0.17 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48

Instrument :

MSVOA\_U


ClientSampleId :

Tot Ion: 76 Resp: 5474

Ion Ratio Lower Upper




76 100

78 0.0 26.0 39.0#

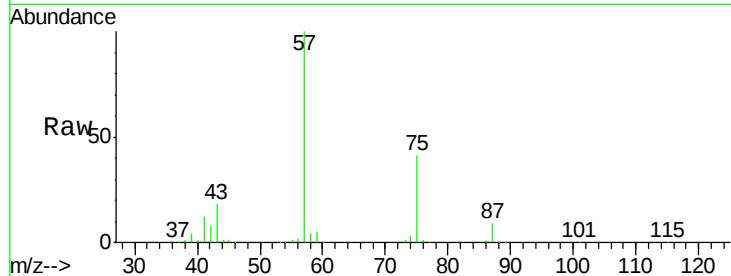

Abundance Ion 75.90 (75.60 to 76.60): VU0

Ion 77.90 (77.60 to 78.60): VU0

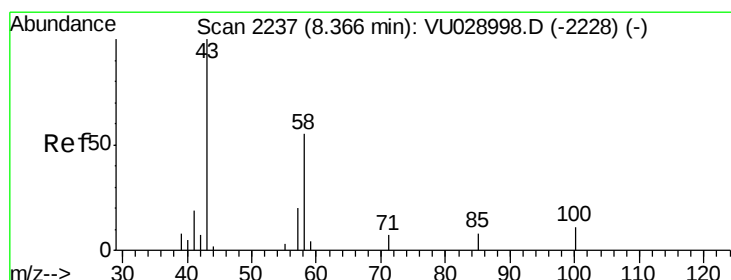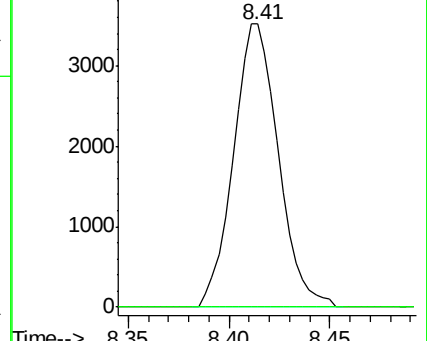

#59

2-Hexanone

Concen: 4.241 ug/l

RT: 8.31 min Scan# 2220

Delta R.T. -0.05 min

Lab File: VU029086.D


Acq: 09 Jan 2019 13:48

Tgt Ion: 43 Resp: 7518

Ion Ratio Lower Upper



43 100


58 0.0 29.8 89.4#



Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0




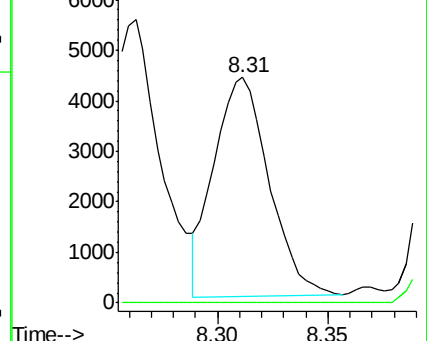




#62  
4-Bromofluorobenzene  
Concen: 43.912 ug/l  
RT: 10.30 min Scan# 2840  
Delta R.T. -0.00 min  
Lab File: VU029086.D  
Acq: 09 Jan 2019 13:48




Instrument :  
MSVOA\_U  
ClientSampleId :


Tot Ion: 95 Resp: 79632  
Ion Ratio Lower Upper  
95 100  
174 84.3 0.0 170.6  
176 81.8 0.0 165.0

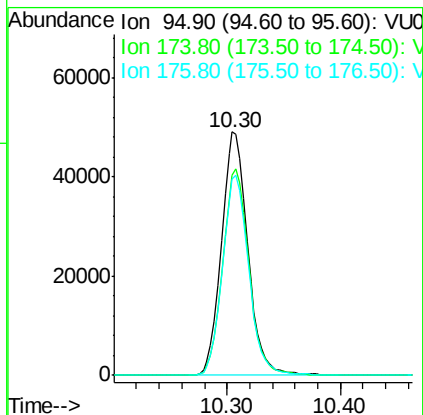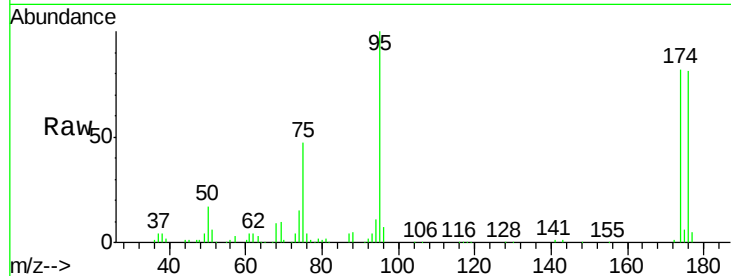

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 9.09 min Scan# 2462  
Delta R.T. 0.00 min  
Lab File: VU029086.D  
Acq: 09 Jan 2019 13:48

Tgt Ion: 117 Resp: 185899  
Ion Ratio Lower Upper  
117 100  
82 56.4 43.9 65.9  
119 31.9 26.0 39.0

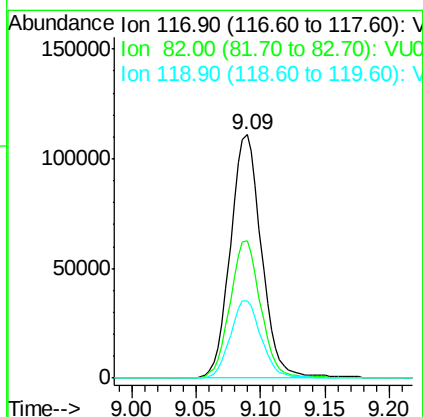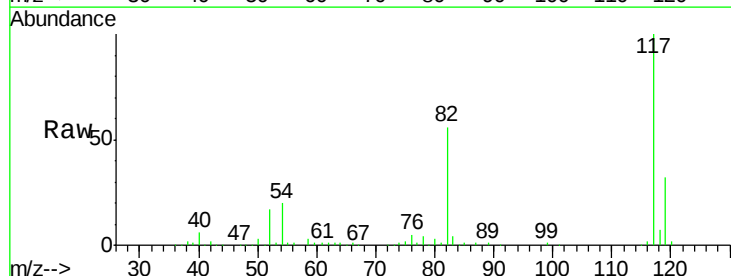

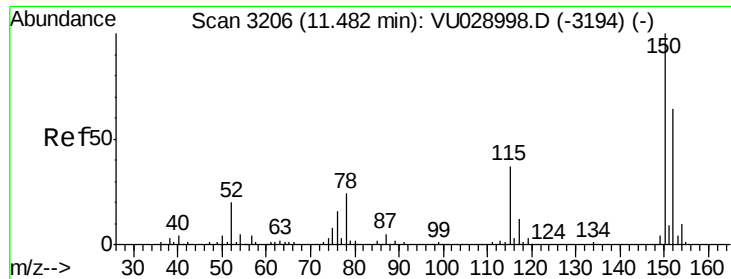

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.48 min Scan# 3206

Delta R.T. -0.00 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48


Instrument :

MSVOA\_U

ClientSampleId :

Tot Ion:152 Resp: 74755




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 152 | 100   |       |       |
| 115 | 56.9  | 40.1  | 120.3 |
| 150 | 154.7 | 0.0   | 345.2 |



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

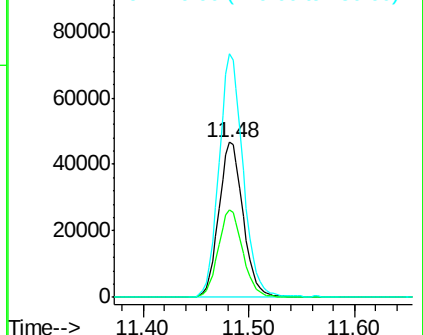

#74

N-ethyl acetate

Concen: 2.958 ug/l

RT: 9.76 min Scan# 2672


Delta R.T. -0.25 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48

Tgt Ion: 43 Resp: 7053

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 43  | 100   |       |       |
| 70  | 0.0   | 36.3  | 54.5# |
| 55  | 4.2   | 20.5  | 30.7# |
| 61  | 9.5   | 21.8  | 32.8# |






Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 55.00 (54.70 to 55.70): VU0

Ion 61.00 (60.70 to 61.70): VU0

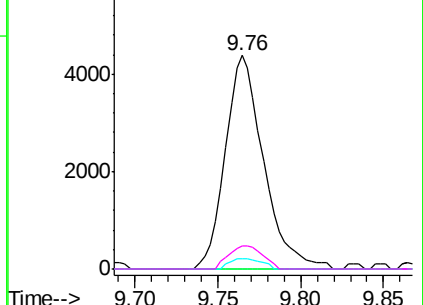

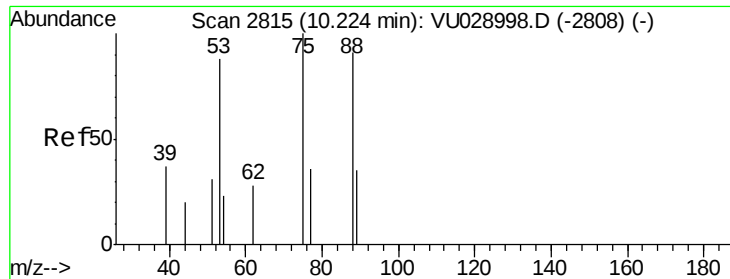

#76

1,2,3-Trichloropropane

Concen: 20.597 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. -0.19 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48

Instrument :

MSVOA\_U


ClientSampled :

Tot Ion: 75 Resp: 37726

Ion Ratio Lower Upper




75 100

77 1.3 20.9 62.8#

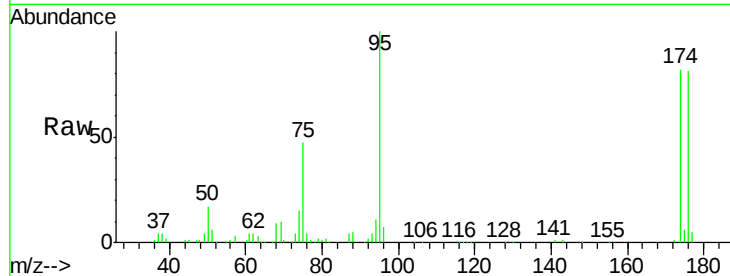

Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 77.00 (76.70 to 77.70): VU0

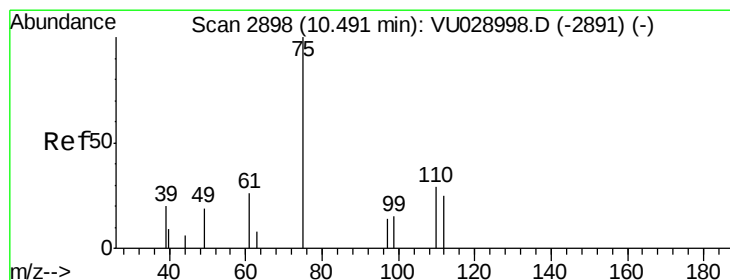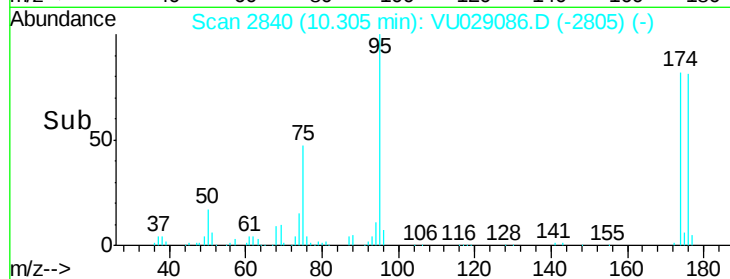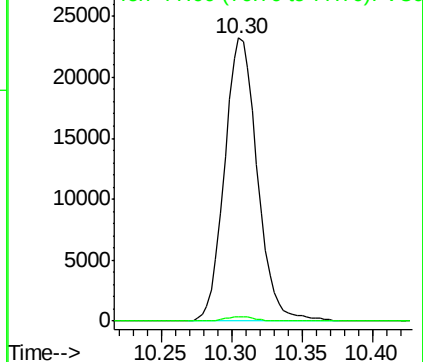

#81

trans-1,4-Dichloro-2-butene

Concen: 53.121 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. -0.21 min

Lab File: VU029086.D

Acq: 09 Jan 2019 13:48


Tgt Ion: 75 Resp: 37726

Ion Ratio Lower Upper

75 100

53 0.0 0.0 0.0

89 0.0 0.0 0.0

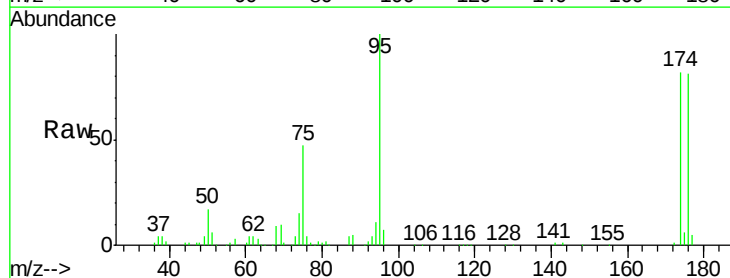

Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 53.00 (52.70 to 53.70): VU0

Ion 88.90 (88.60 to 89.60): VU0

