


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010919\
Data File : VU029079.D
Acq On : 09 Jan 2019 08:34
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
Title : SW846 8260
Last Update : Fri Jan 04 02:22:53 2019

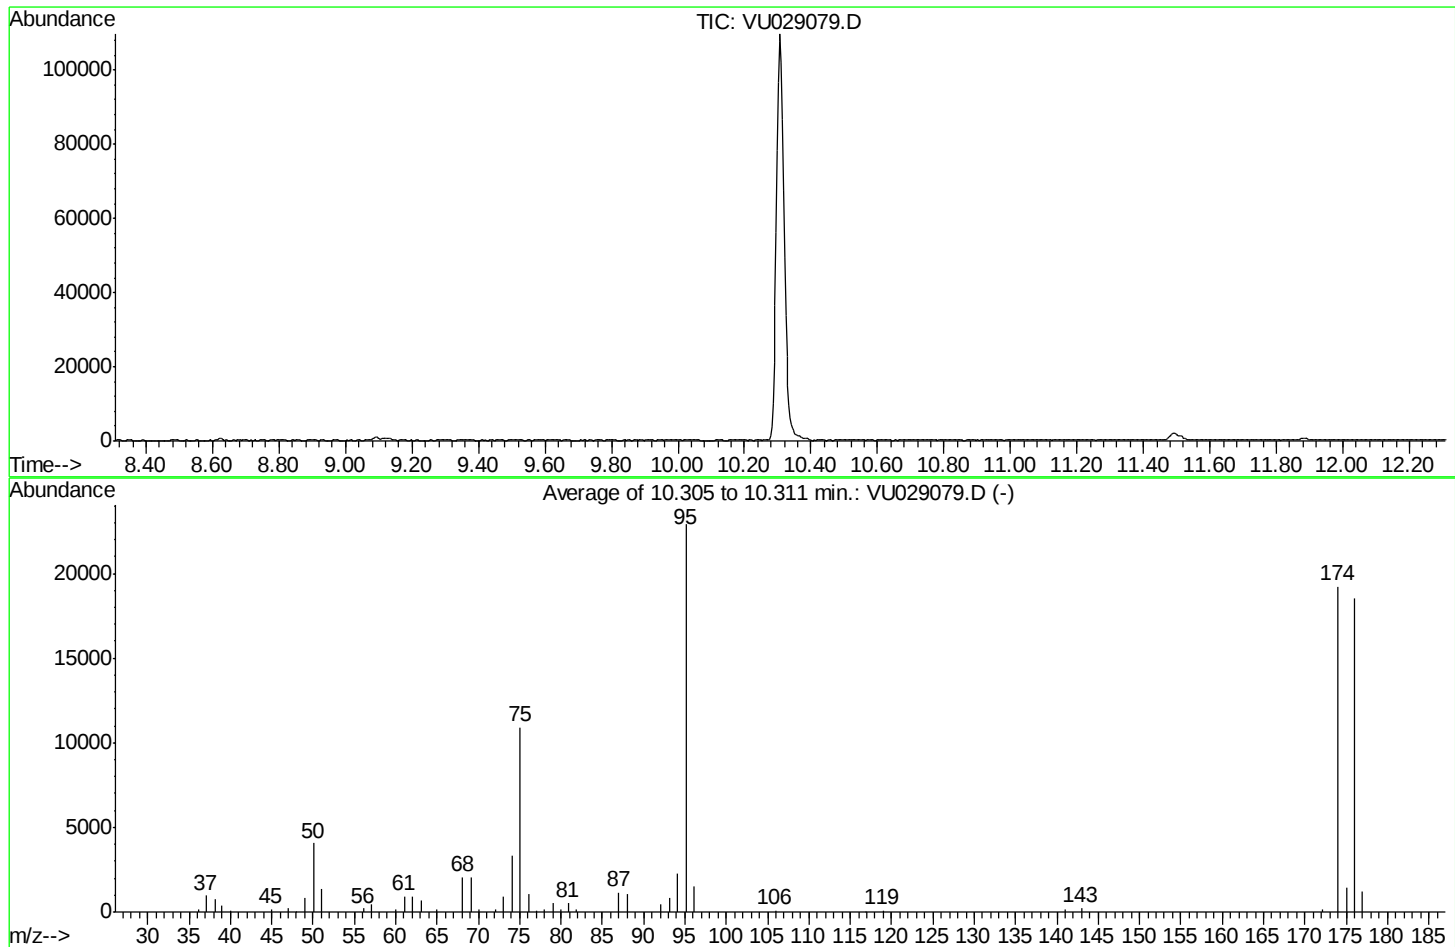

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	4077	PASS
75	95	30	60	47.6	10907	PASS
95	95	100	100	100.0	22906	PASS
96	95	5	9	6.5	1486	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.0	19245	PASS
175	174	5	9	7.4	1429	PASS
176	174	95	101	96.4	18560	PASS
177	176	5	9	6.6	1230	PASS