


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU010920\
 Data File : VU036414.D
 Acq On : 09 Jan 2020 09:15
 Operator : JC/MD
 Sample : BFB36
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB36

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 10 04:07:29 2020

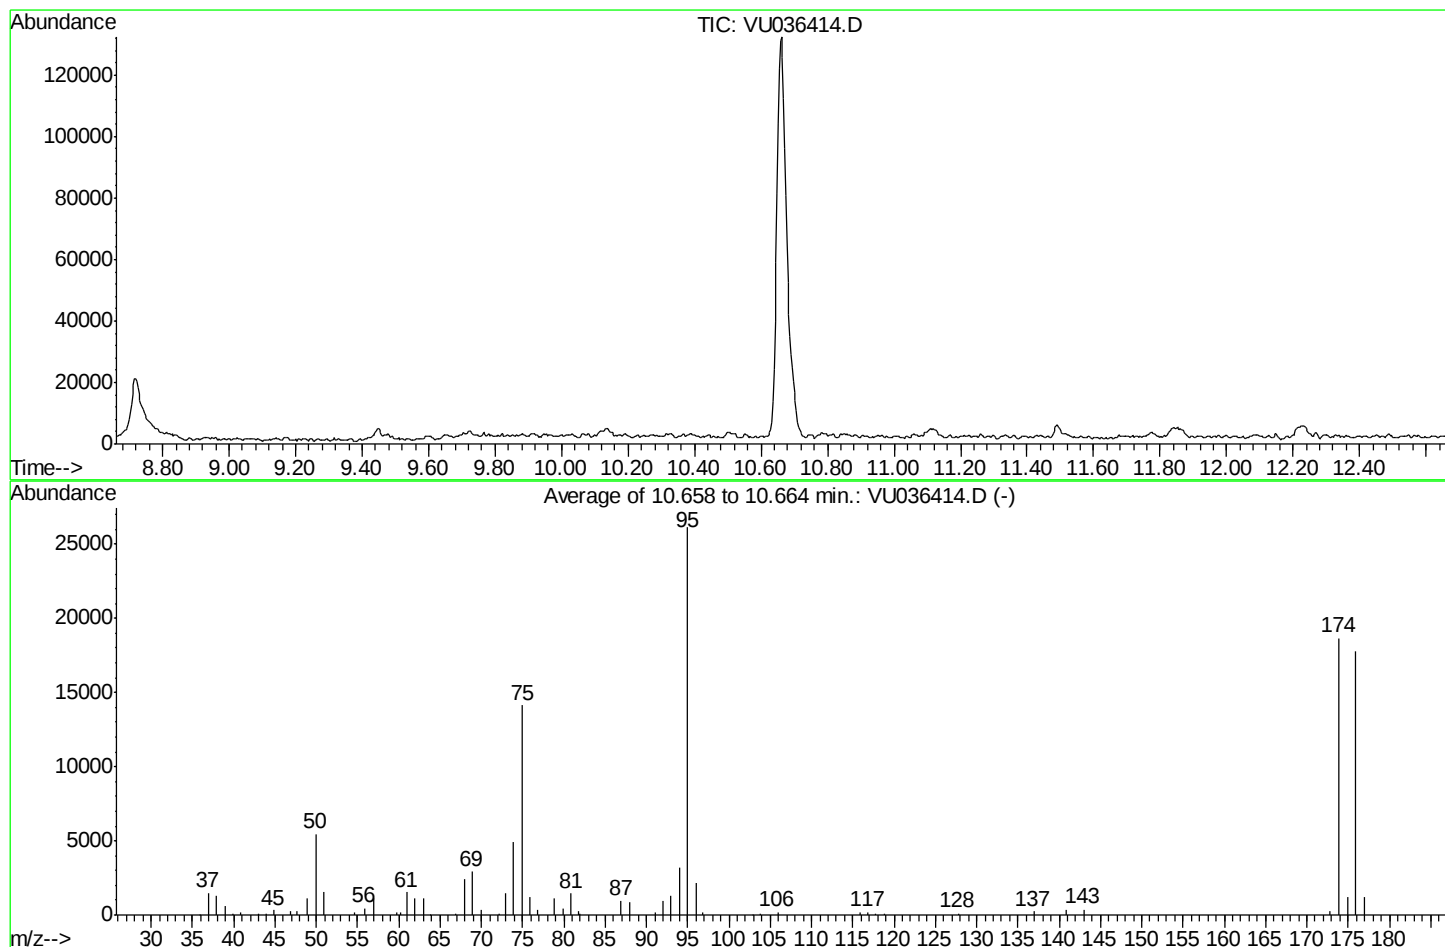

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	5445	PASS
75	95	30	80	54.1	14143	PASS
95	95	100	100	100.0	26136	PASS
96	95	5	9	8.2	2151	PASS
173	174	0.00	2	1.5	284	PASS
174	95	50	120	71.4	18650	PASS
175	174	5	9	6.6	1228	PASS
176	174	95	101	95.3	17778	PASS
177	176	5	9	6.6	1176	PASS

m/z	Abundance
35.80	589.0
36.90	1570.0
37.90	1612.0
39.00	656.0
39.90	375.0
40.80	189.0
43.00	178.0
43.90	1062.0
44.80	341.0
46.90	404.0
47.70	208.0
48.90	1173.0
49.90	5498.0
50.90	1657.0
54.70	151.0
55.80	543.0
57.00	1082.0
60.20	232.0
60.90	1332.0
61.90	1280.0
63.00	1116.0
63.80	125.0
66.90	112.0
68.00	2574.0
69.00	3141.0
70.00	349.0
72.20	118.0
73.00	1537.0
73.90	5289.0
75.00	14444.0
75.90	1125.0
76.90	321.0
78.80	1085.0
79.90	404.0
80.90	1369.0
81.80	423.0
87.00	1002.0
87.90	842.0
91.00	148.0
92.00	964.0
92.90	1346.0
94.00	3012.0
95.00	26608.0
96.00	2186.0
96.90	158.0
103.90	120.0
105.90	260.0
116.00	210.0
116.80	246.0
118.80	134.0
127.80	163.0
136.90	127.0
140.80	438.0
142.90	358.0
172.70	329.0
173.90	18216.0
175.00	1268.0
176.00	18048.0
176.90	1191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
35.80	691.0
36.90	1672.0
37.90	1677.0
39.00	640.0
40.00	403.0
40.80	163.0
43.00	127.0
43.90	1085.0
44.80	307.0
47.00	237.0
47.60	261.0
48.90	1111.0
50.00	5593.0
51.00	1580.0
54.70	172.0
55.80	426.0
57.00	1143.0
59.80	218.0
60.10	181.0
61.00	1542.0
61.90	1133.0
63.00	1127.0
66.80	123.0
68.00	2474.0
69.00	3104.0
70.10	422.0
72.10	138.0
73.00	1523.0
73.90	5082.0
75.00	14452.0
75.90	1332.0
76.80	367.0
78.80	1092.0
79.80	395.0
80.90	1511.0
81.80	322.0
86.90	979.0
87.90	789.0
91.00	140.0
92.00	1053.0
92.90	1251.0
94.00	3260.0
95.00	26672.0
96.00	2230.0
96.80	163.0
103.80	138.0
105.90	183.0
115.90	171.0
116.90	213.0
117.80	120.0
118.80	157.0
127.80	141.0
136.90	235.0
140.90	358.0
143.00	348.0
172.80	273.0
173.90	19104.0
175.00	1252.0
175.90	18104.0
176.90	1221.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
35.90	921.0
36.90	1562.0
37.90	1545.0
38.90	582.0
40.00	378.0
40.80	141.0
43.90	1124.0
44.80	281.0
47.10	116.0
47.60	286.0
48.90	1184.0
50.00	5246.0
51.00	1450.0
54.70	152.0
55.90	383.0
56.90	1169.0
59.80	291.0
61.00	1742.0
61.80	1020.0
62.90	1053.0
66.80	133.0
68.00	2321.0
68.90	2861.0
70.10	319.0
72.00	137.0
72.90	1377.0
73.90	4395.0
75.00	13535.0
75.90	1251.0
76.70	360.0
78.80	1226.0
79.80	406.0
80.90	1481.0
82.00	279.0
86.90	909.0
87.90	933.0
91.00	142.0
92.00	927.0
92.90	1201.0
94.00	3311.0
95.00	25128.0
96.00	2037.0
96.80	141.0
102.80	115.0
103.80	137.0
105.80	118.0
115.90	107.0
116.90	163.0
117.80	190.0
118.80	105.0
136.90	319.0
140.90	269.0
143.00	374.0
172.90	251.0
173.90	18632.0
175.00	1164.0
175.90	17184.0
176.90	1116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

Scan 2886 (10.619 min): VU036414.D
BFB36

m/z	Abundance
35.80	712.0
36.90	117.0
37.80	302.0
40.00	268.0
43.90	971.0
55.10	230.0
68.80	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36