

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU010921\
 Data File : VU041906.D
 Acq On : 08 Jan 2021 15:36
 Operator : SY/MD
 Sample : M1049-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AQ5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	93	rVB	52707	57977	1.88%	0.626%
2	1.919	171	180	193	rBV	55790	69658	2.25%	0.752%
3	2.090	224	233	241	rBV	39934	54594	1.77%	0.589%
4	2.147	241	251	265	rVB	335101	479381	15.50%	5.173%
5	2.578	373	385	399	rBV	97765	156252	5.05%	1.686%
6	4.681	1016	1039	1077	rBV3	91330	371702	12.02%	4.011%
7	5.080	1147	1163	1183	rBV	95742	216893	7.02%	2.340%
8	5.739	1347	1368	1386	rBV2	170755	447257	14.47%	4.826%
9	6.260	1512	1530	1548	rBV	152472	284463	9.20%	3.069%
10	6.552	1605	1621	1654	rBV	1664794	3091835	100.00%	33.361%
11	6.700	1654	1667	1683	rVB	107395	206828	6.69%	2.232%
12	7.572	1927	1938	1954	rBV2	48031	85761	2.77%	0.925%
13	7.903	2027	2041	2058	rBV	194720	338721	10.96%	3.655%
14	8.183	2116	2128	2145	rBV2	32486	54834	1.77%	0.592%
15	8.555	2231	2244	2259	rBV	956620	1615459	52.25%	17.431%
16	8.639	2259	2270	2295	rVB	301581	591266	19.12%	6.380%
17	9.417	2500	2512	2532	rBV	213375	359680	11.63%	3.881%
18	10.755	2916	2928	2943	rBV2	101005	159818	5.17%	1.724%
19	11.806	3243	3255	3270	rVB	196076	314482	10.17%	3.393%
20	12.186	3362	3373	3389	rVB	188182	310823	10.05%	3.354%




Sum of corrected areas: 9267684

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU010921\
Data File : VU041906.D
Acq On : 08 Jan 2021 15:36
Operator : SY/MD
Sample : M1049-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AQ5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

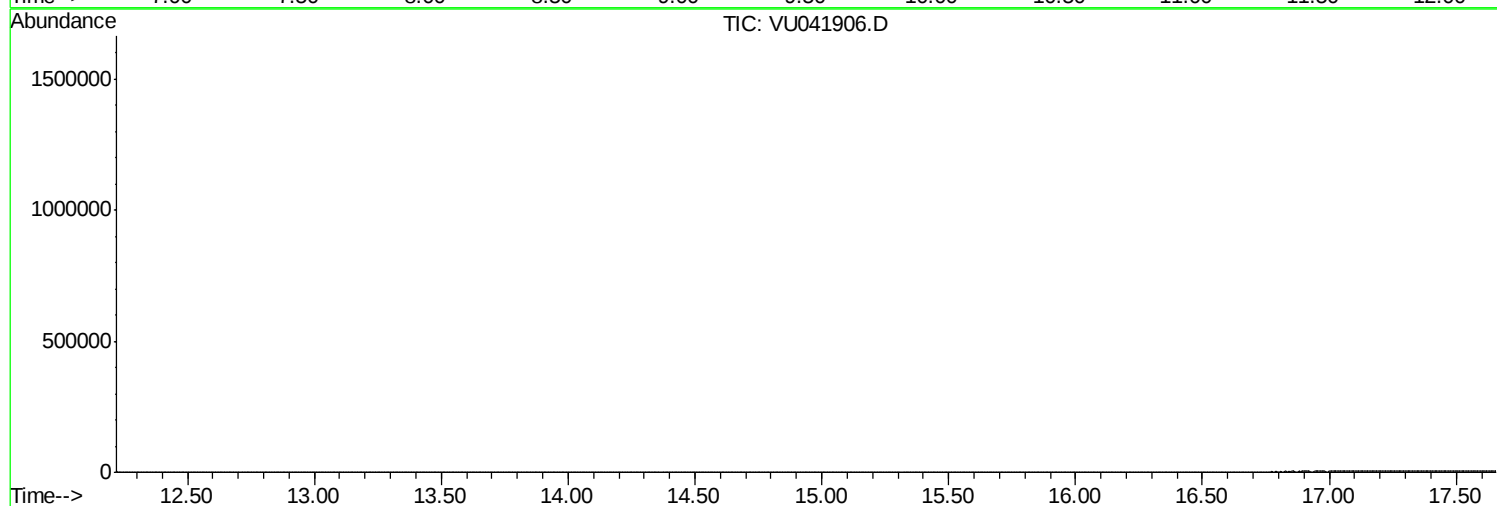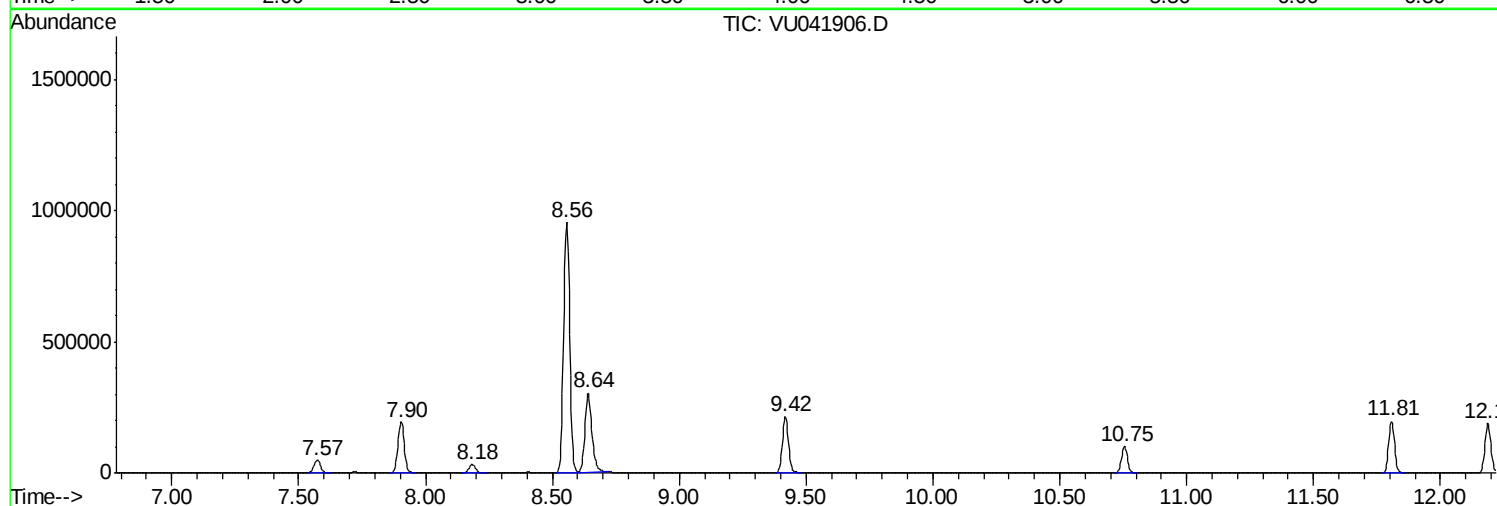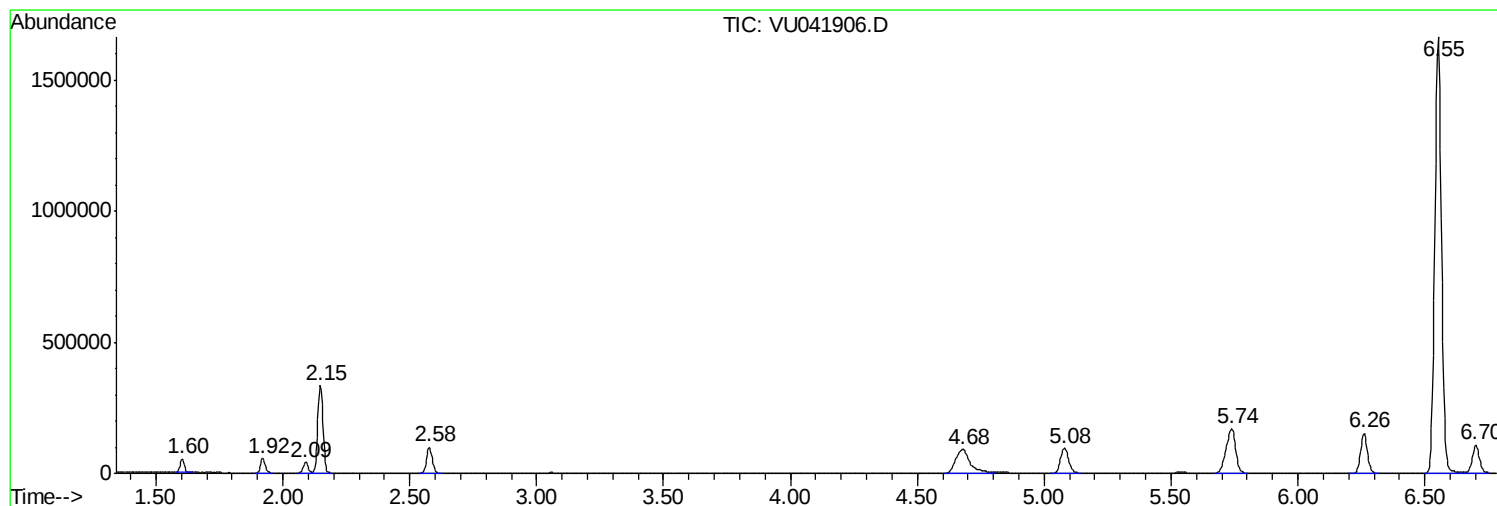

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU010921\
Data File : VU041906.D
Acq On : 08 Jan 2021 15:36
Operator : SY/MD
Sample : M1049-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AQ5










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.09	0.96 ug/L	54594	1,4-Difluorobenzene	6.26

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
4			Cyclopentene, 1-chloro-	102	C5H7Cl	000930-29-0	7
5			Methanamine, N,N-difluoro-	67	CH3F2N	000753-58-2	4

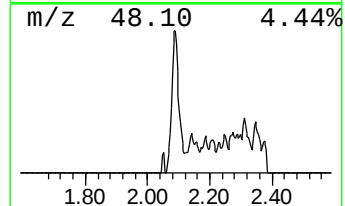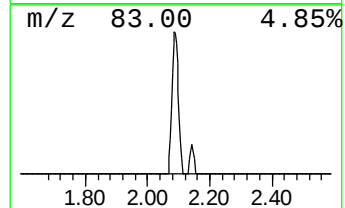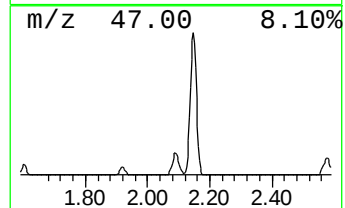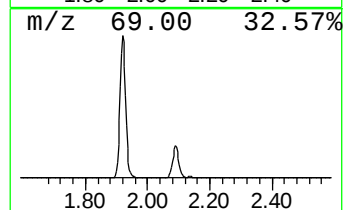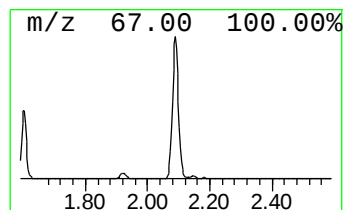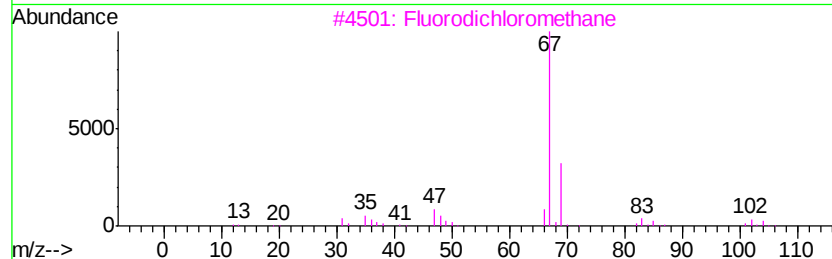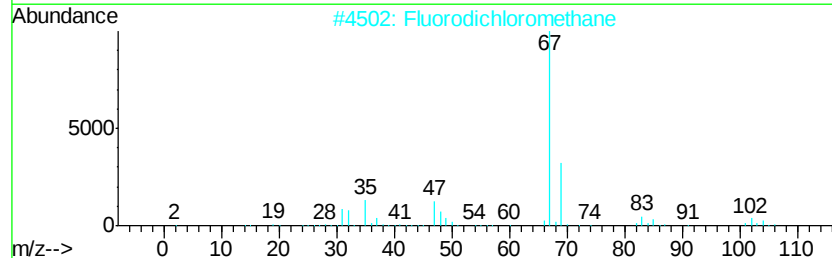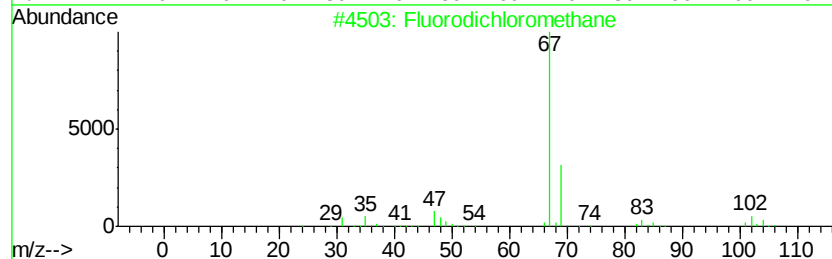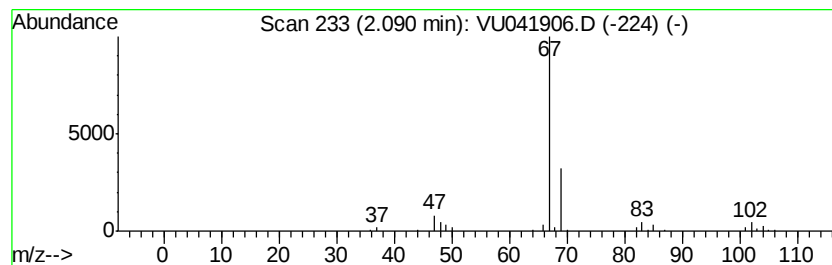

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU010921\
Data File : VU041906.D
Acq On : 08 Jan 2021 15:36
Operator : SY/MD
Sample : M1049-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AQ5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichloromet...	2.09	1.0	ug/L	54594	1	6.26	284463	5.0