


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010921\
 Data File : VU041868.D
 Acq On : 07 Jan 2021 12:43
 Operator : SY/MD
 Sample : BFB33
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB33

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Jan 09 01:31:59 2021

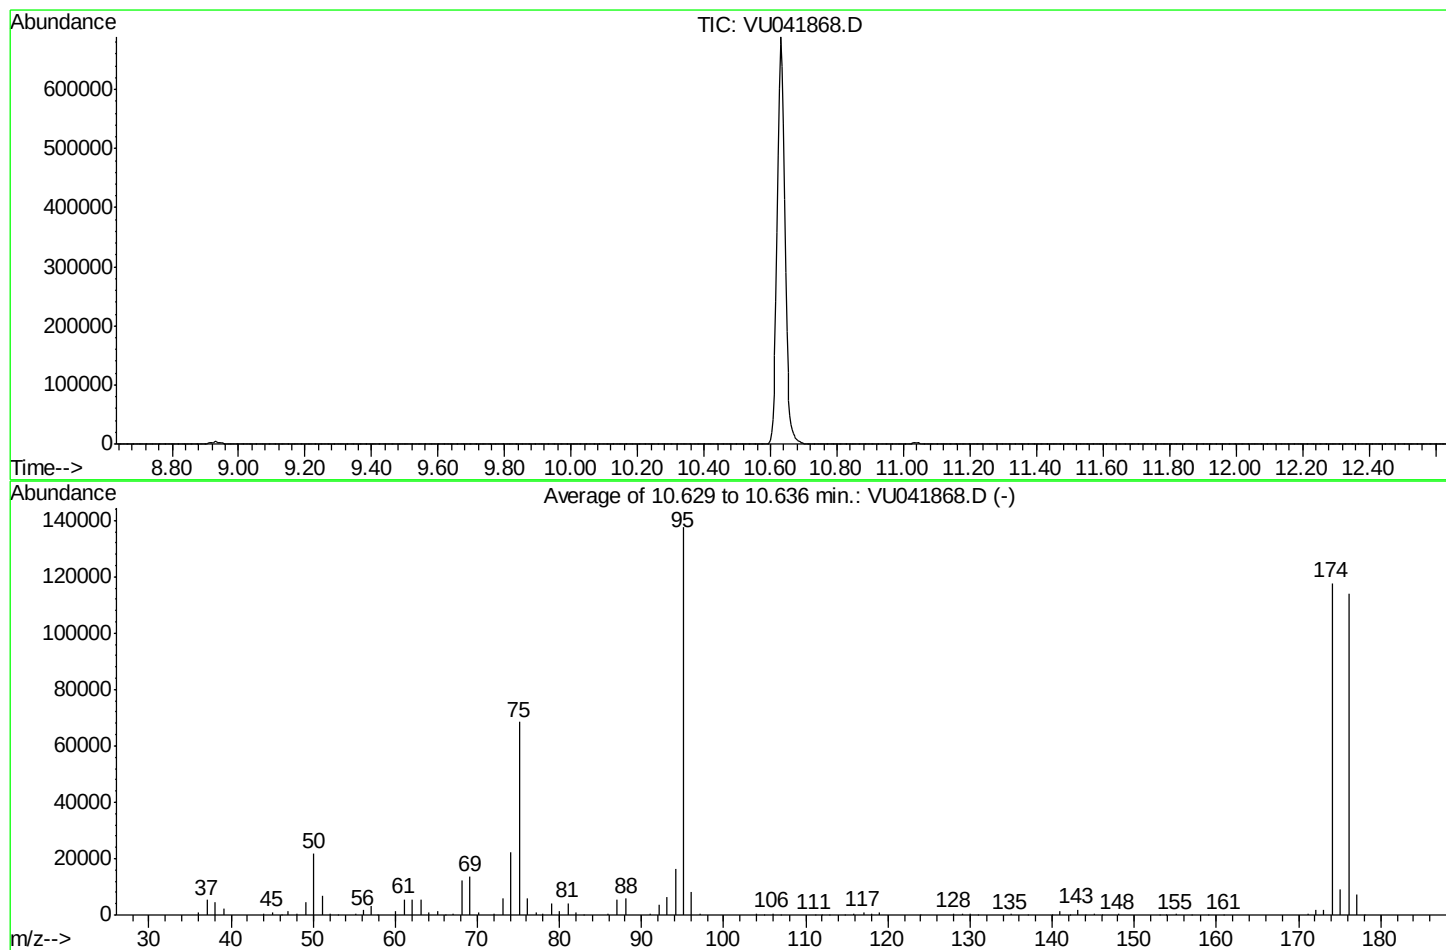

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	21744	PASS
75	95	30	80	49.7	68365	PASS
95	95	100	100	100.0	137536	PASS
96	95	5	9	6.0	8282	PASS
173	174	0.00	2	1.5	1752	PASS
174	95	50	120	85.7	117832	PASS
175	174	5	9	7.8	9186	PASS
176	174	95	101	96.8	114008	PASS
177	176	5	9	6.5	7441	PASS

Scan 2875 (10.584 min): VU041868.D
BFB33

m/z	Abundance
44.00	330.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
36.10	859.0
37.10	5027.0
38.10	4419.0
39.10	1832.0
44.00	828.0
45.00	965.0
46.20	175.0
47.00	1346.0
48.00	665.0
49.10	4334.0
50.10	20664.0
51.10	6189.0
52.10	223.0
55.20	315.0
56.10	1488.0
57.10	2985.0
60.00	1269.0
61.10	5319.0
62.10	5347.0
63.10	5168.0
64.10	835.0
65.10	1492.0
67.00	307.0
68.10	11113.0
69.10	12906.0
70.10	838.0
72.00	581.0
73.00	5605.0
74.10	20824.0
75.10	64648.0
76.10	5952.0
77.10	783.0
78.00	367.0
79.00	3953.0
80.00	1105.0
81.00	3825.0
82.00	776.0
83.00	144.0
85.90	288.0
87.00	5137.0
88.10	5492.0
91.00	394.0
92.10	3821.0
93.10	6222.0
94.10	15336.0
95.10	131328.0
96.10	7358.0
97.10	334.0
104.00	591.0
104.90	163.0
106.00	516.0
107.00	101.0
111.10	115.0
112.90	118.0
115.90	461.0
117.00	938.0
118.00	388.0
119.00	710.0
128.00	487.0
129.00	251.0
130.10	374.0
130.90	165.0
135.00	243.0
137.00	262.0
140.10	121.0
141.00	1314.0
142.00	166.0
143.10	1894.0
144.00	173.0
145.10	636.0
146.00	235.0
148.00	307.0
153.00	190.0
155.00	326.0
157.10	240.0
159.00	124.0
160.90	129.0
171.10	328.0
172.10	1688.0
173.10	1553.0
174.10	115464.0
175.10	8857.0
176.10	112240.0
177.10	6965.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
36.10	992.0
37.10	5606.0
38.10	4860.0
39.10	2160.0
44.00	877.0
45.00	1007.0
46.10	217.0
47.00	1501.0
47.90	658.0
49.10	4853.0
50.10	22152.0
51.10	7115.0
52.10	307.0
53.10	148.0
55.10	370.0
56.10	1707.0
57.10	3265.0
57.90	125.0
60.00	1388.0
61.10	5909.0
62.10	5793.0
63.10	5830.0
64.10	891.0
65.10	1631.0
66.10	109.0
67.00	327.0
68.10	12703.0
69.10	13946.0
70.10	1037.0
72.00	627.0
73.00	6083.0
74.10	22800.0
75.10	70624.0
76.10	6316.0
77.10	918.0
78.00	423.0
79.00	4199.0
80.00	1220.0
81.00	4339.0
82.00	848.0
83.00	121.0
85.90	302.0
87.00	5886.0
88.10	6153.0
91.00	450.0
92.10	3949.0
93.10	6536.0
94.10	16832.0
95.10	141888.0
96.10	8490.0
97.10	326.0
104.00	542.0
104.90	206.0
106.00	557.0
106.90	120.0
111.10	123.0
112.00	100.0
114.80	119.0
115.90	375.0
117.00	1043.0
117.90	440.0
119.00	878.0
124.00	104.0
128.00	525.0
129.00	265.0
130.10	356.0
130.90	134.0
135.00	269.0
137.00	221.0
140.10	131.0
141.00	1369.0
142.10	160.0
143.10	1984.0
144.00	260.0
145.10	690.0
146.10	187.0
148.00	343.0
153.00	173.0
155.10	367.0
157.10	224.0
158.90	121.0
161.00	119.0
171.20	363.0
172.10	1831.0
173.10	1855.0
174.10	121224.0
175.10	9404.0
176.10	117304.0
177.10	7561.0
178.00	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
36.00	971.0
37.00	5562.0
38.10	4777.0
39.10	2279.0
44.00	821.0
45.00	958.0
46.00	218.0
47.00	1384.0
48.00	653.0
49.00	4914.0
50.10	22416.0
51.10	7376.0
52.10	377.0
53.00	183.0
55.10	384.0
56.10	1791.0
57.10	3320.0
57.90	119.0
60.00	1363.0
61.10	5850.0
62.10	5872.0
63.10	5888.0
64.10	982.0
65.10	1534.0
66.10	115.0
67.00	299.0
68.10	13112.0
69.10	13530.0
70.10	1148.0
72.10	600.0
73.10	5925.0
74.10	22736.0
75.10	69824.0
76.10	6019.0
77.10	1014.0
78.00	495.0
79.00	4093.0
80.00	1275.0
81.00	4577.0
82.00	860.0
86.00	283.0
87.00	5918.0
88.10	5826.0
91.00	444.0
92.10	3665.0
93.10	6249.0
94.10	16728.0
95.10	139392.0
96.10	8998.0
97.10	260.0
104.10	453.0
105.00	259.0
106.00	575.0
106.90	147.0
111.10	104.0
114.80	150.0
115.90	323.0
117.00	1104.0
117.90	455.0
119.00	951.0
128.00	479.0
129.00	287.0
130.00	353.0
131.00	111.0
135.00	259.0
137.00	172.0
140.00	103.0
141.00	1332.0
142.20	144.0
143.10	1966.0
144.00	218.0
145.10	670.0
146.10	192.0
148.10	353.0
153.10	126.0
153.90	103.0
155.10	350.0
157.00	214.0
158.90	104.0
160.90	127.0
171.20	395.0
172.10	1798.0
173.10	1850.0
174.10	116808.0
175.10	9299.0
176.10	112480.0
177.10	7799.0
178.00	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33