

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
 Data File : VU057434.D
 Acq On : 09 Jan 2024 12:59
 Operator : MD/SY
 Sample : 01058-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 10 00:36:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 10 00:35:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	254163	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	252773	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	102887	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	79902	45.676	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.360%		
7) Chloroethane-d5	1.914	69	61891	45.719	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.440%		
11) 1,1-Dichloroethene-d2	2.557	63	124415	33.555	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.100%		
21) 2-Butanone-d5	4.634	46	87943	103.749	ug/L	-0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	103.750%		
24) Chloroform-d	5.055	84	183486	44.355	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.720%		
26) 1,2-Dichloroethane-d4	5.692	65	134838	49.341	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.680%		
32) Benzene-d6	5.721	84	328038	48.346	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.700%		
36) 1,2-Dichloropropane-d6	6.682	67	93139	48.634	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.260%		
41) Toluene-d8	7.891	98	294900	46.379	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.760%		
43) trans-1,3-Dichloroprop...	8.174	79	51272	44.854	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.700%		
47) 2-Hexanone-d5	8.644	63	64395	102.859	ug/L	-0.04
Spiked Amount 100.000	Range 45 - 130		Recovery =	102.860%		
56) 1,1,2,2-Tetrachloroeth...	10.753	84	134136	46.869	ug/L	-0.01
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.740%		
66) 1,2-Dichlorobenzene-d4	12.190	152	101565	50.471	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.940%		
Target Compounds						Qvalue
60) 1,2,3-Trichloropropane	11.807	75	10742	5.512	ug/L	# 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057434.D
Acq On : 09 Jan 2024 12:59
Operator : MD/SY
Sample : 01058-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jan 10 00:36:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 10 00:35:16 2024
Response via : Initial Calibration

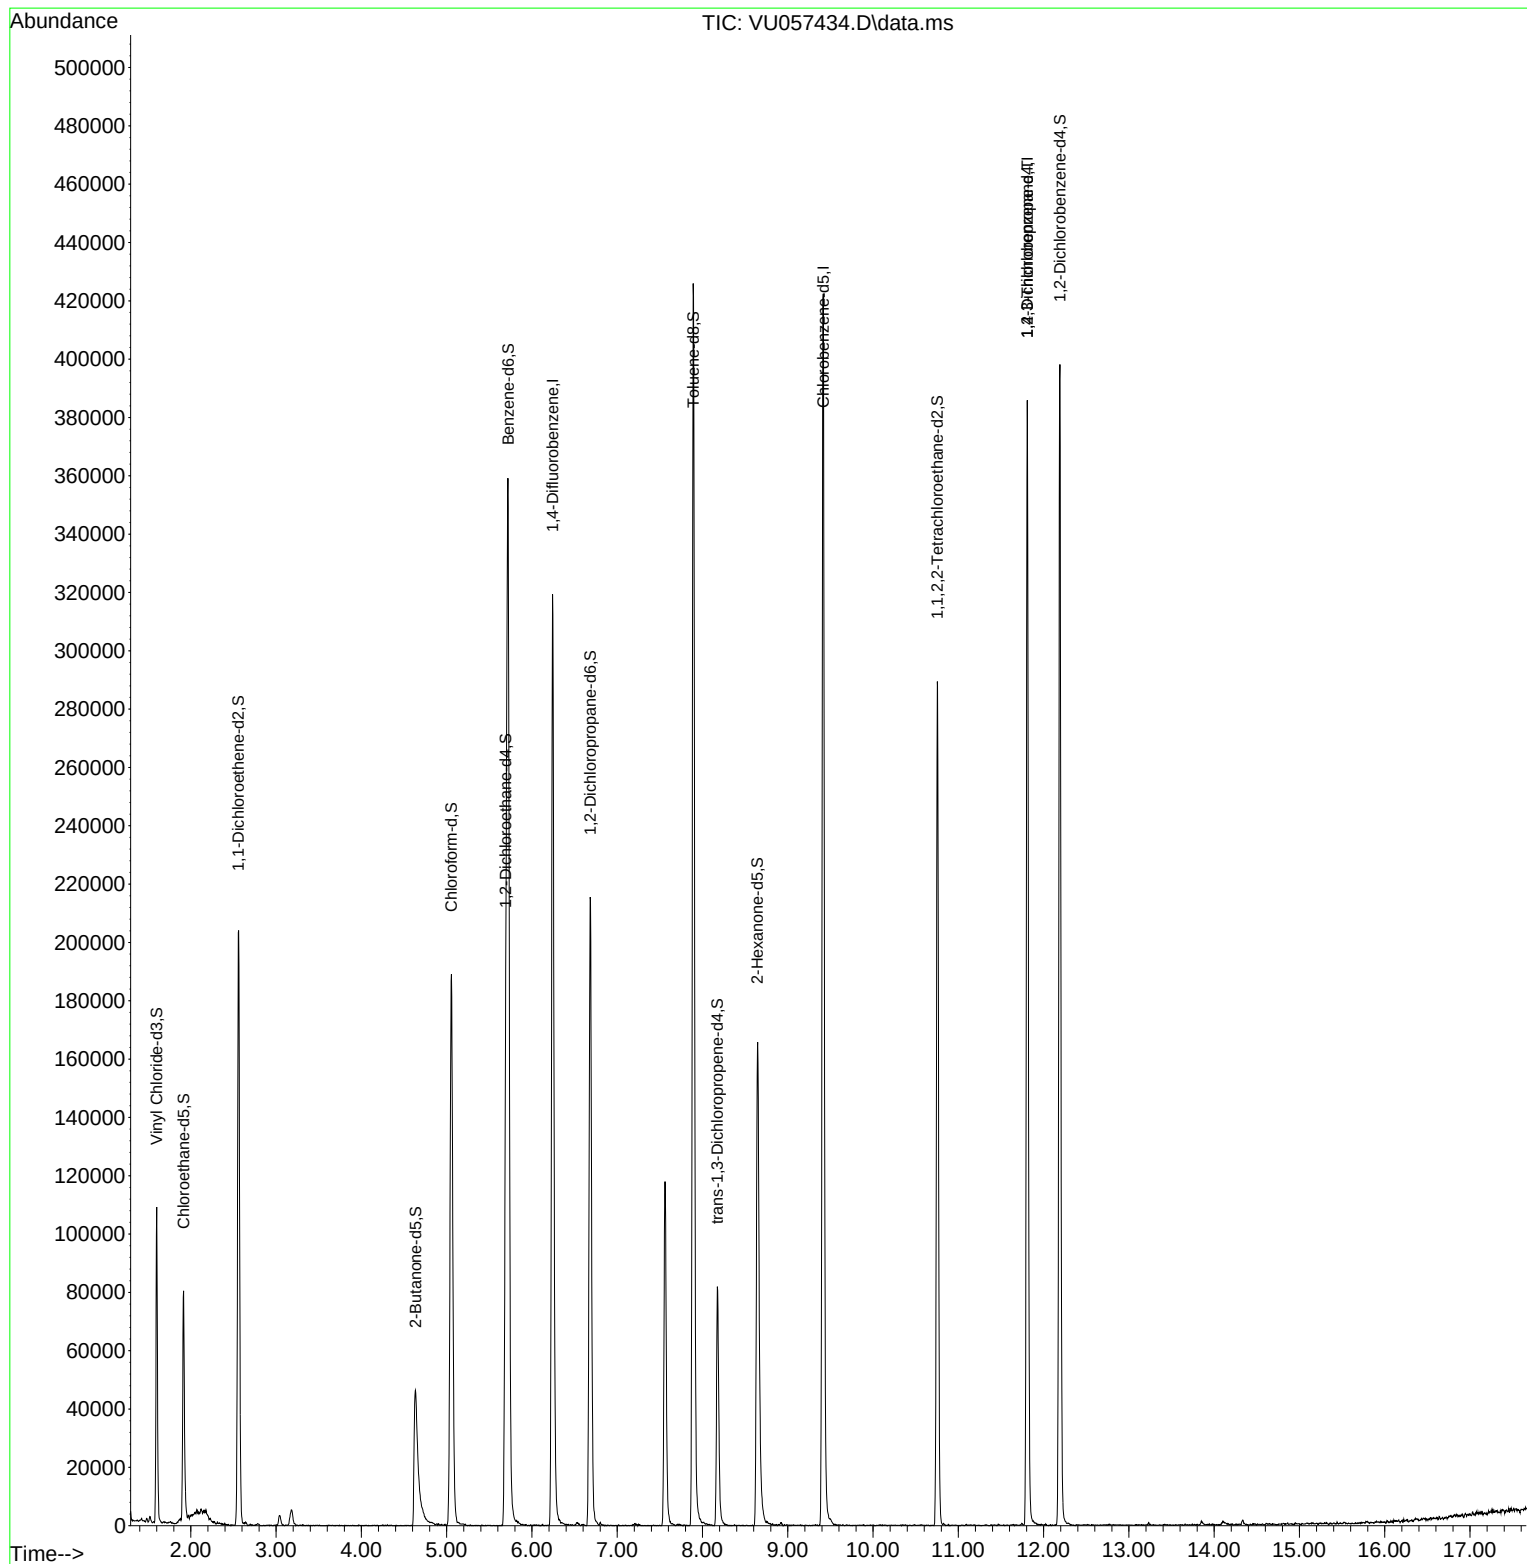

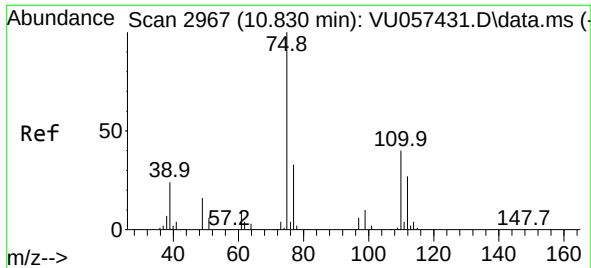

#60
1,2,3-Trichloropropane
Concen: 5.512 ug/L
RT: 11.807 min Scan# 31
Delta R.T. 0.978 min
Lab File: VU057434.D
Acq: 09 Jan 2024 12:59

Instrument :
MSVOA_U
ClientSampleId :

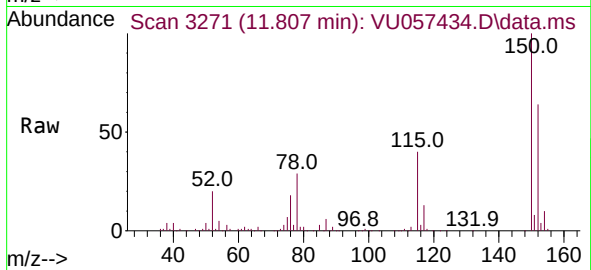

Tgt Ion	Ratio	Lower	Upper
75	100		
77	41.0	26.0	39.0#
110	3.2	33.6	50.4#

