

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
 Data File : VU057438.D
 Acq On : 09 Jan 2024 14:35
 Operator : MD/SY
 Sample : 01061-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 10 00:37:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 10 00:35:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	264024	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	253288	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	105055	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	70553	38.825	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.660%
7) Chloroethane-d5	1.914	69	57769	41.080	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.160%
11) 1,1-Dichloroethene-d2	2.560	63	117414	30.484	ug/L	0.01
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.960%
21) 2-Butanone-d5	4.631	46	78667	89.340	ug/L	-0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.340%
24) Chloroform-d	5.055	84	180881	42.093	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.180%
26) 1,2-Dichloroethane-d4	5.695	65	129759	45.709	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.420%
32) Benzene-d6	5.721	84	321170	47.237	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.480%
36) 1,2-Dichloropropane-d6	6.682	67	92667	48.289	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.580%
41) Toluene-d8	7.891	98	288063	45.211	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.420%
43) trans-1,3-Dichloroprop...	8.174	79	52860	46.149	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.300%
47) 2-Hexanone-d5	8.643	63	61589	98.177	ug/L	-0.04
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.180%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	130417	45.477	ug/L	-0.01
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.960%
66) 1,2-Dichlorobenzene-d4	12.190	152	102153	49.716	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.440%
Target Compounds						
60) 1,2,3-Trichloropropane	11.807	75	11180	5.618	ug/L	Qvalue # 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057438.D
Acq On : 09 Jan 2024 14:35
Operator : MD/SY
Sample : 01061-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jan 10 00:37:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 10 00:35:16 2024
Response via : Initial Calibration

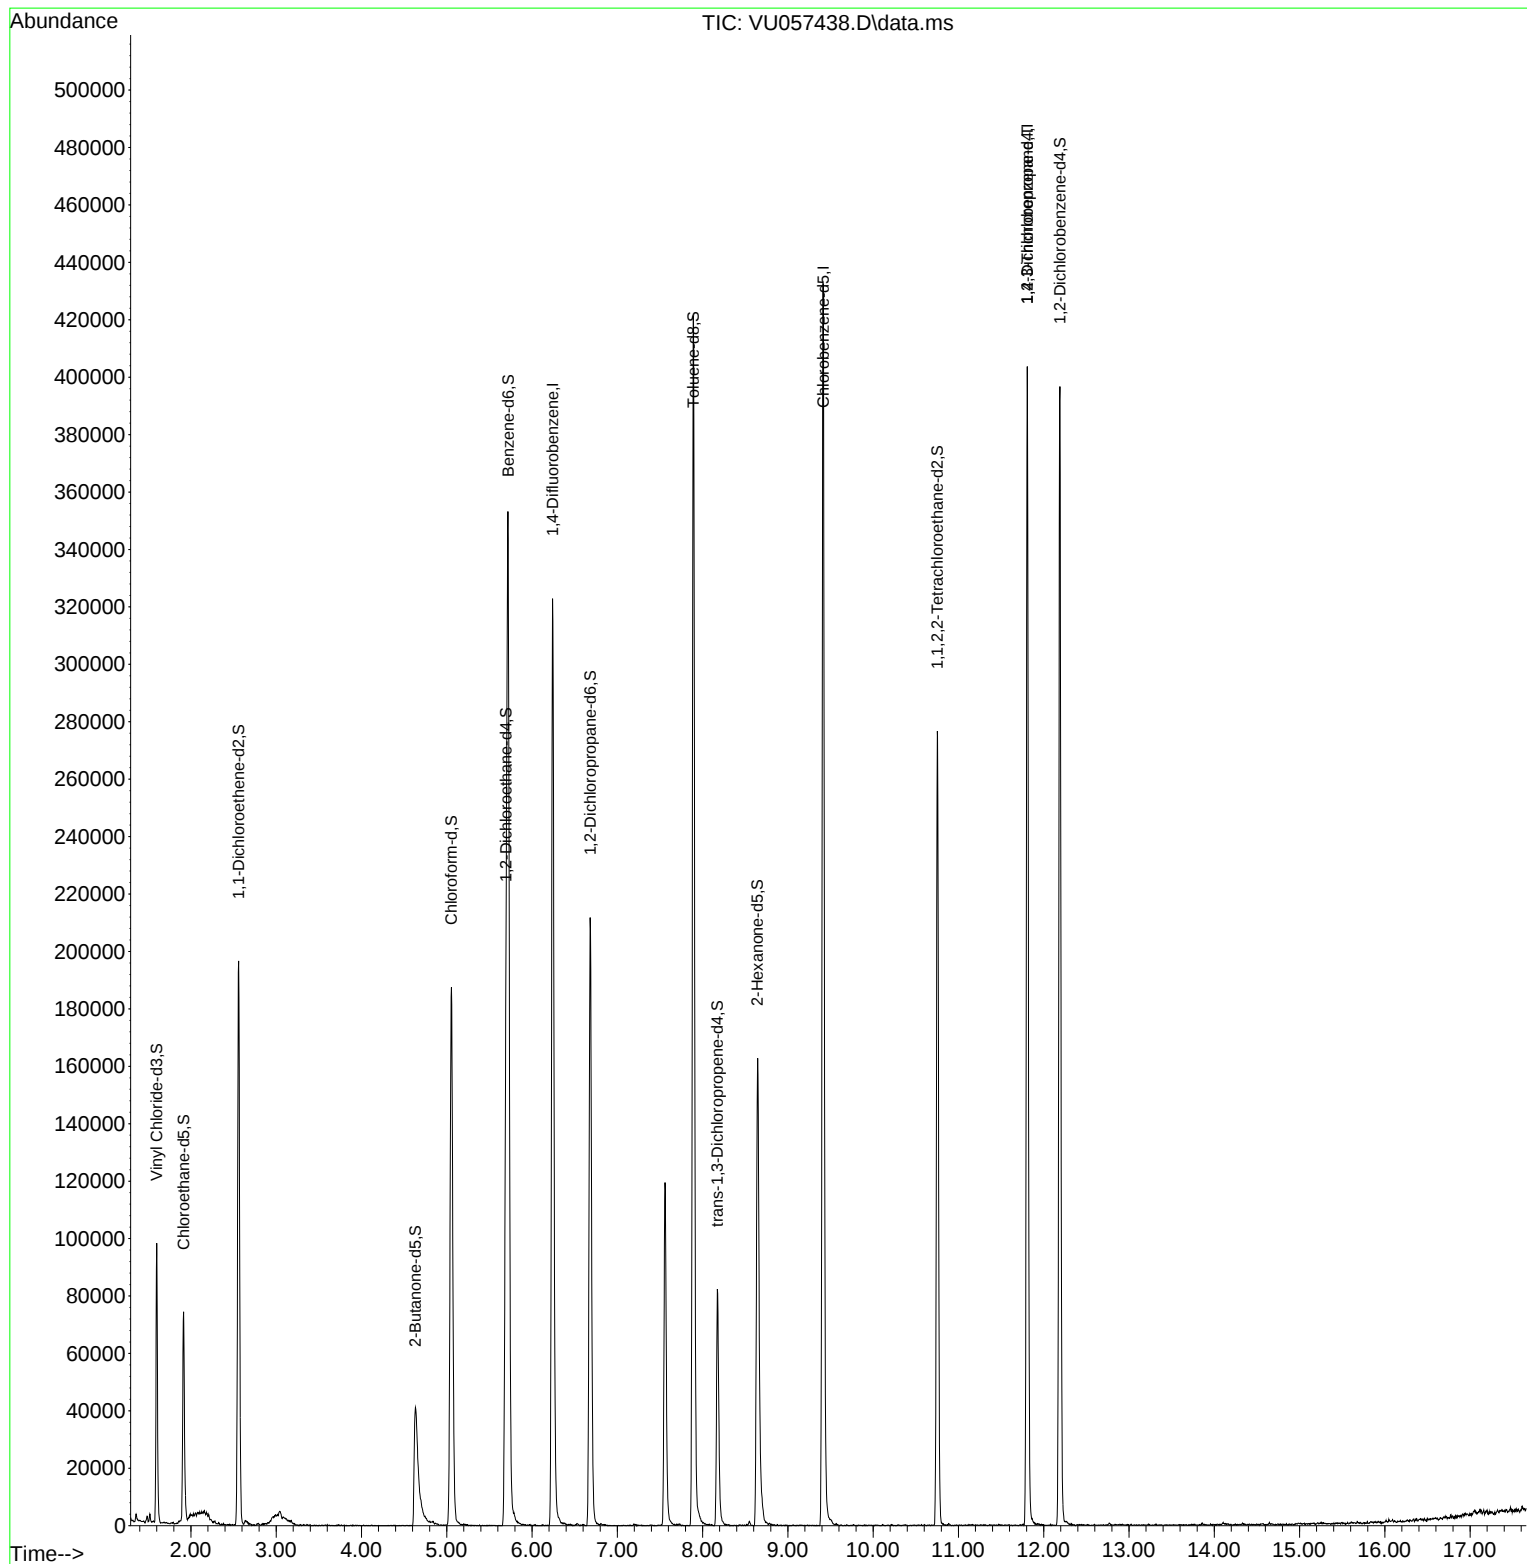

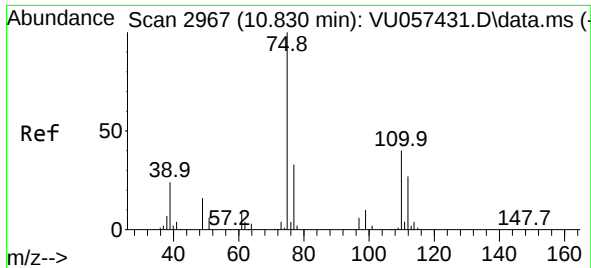

#60
1,2,3-Trichloropropane
Concen: 5.618 ug/L
RT: 11.807 min Scan# 31
Delta R.T. 0.977 min
Lab File: VU057438.D
Acq: 09 Jan 2024 14:35

Instrument :
MSVOA_U
ClientSampleId :

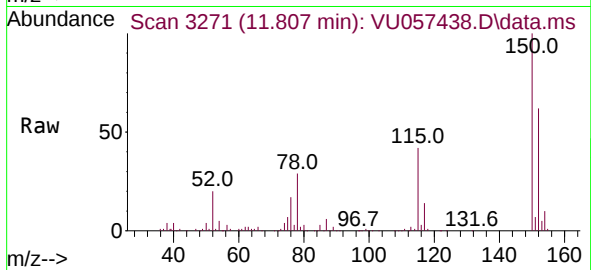

Tgt Ion:	75	Resp:	11180
Ion	Ratio	Lower	Upper
75	100		
77	39.5	26.0	39.0#
110	2.8	33.6	50.4#

