

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
 Data File : VU057432.D
 Acq On : 09 Jan 2024 12:11
 Operator : MD/SY
 Sample : VU0109WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK122

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

Signal : TIC: VU057432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	110	rVB	114707	139442	13.50%	1.818%
2	1.914	186	194	209	rBV	79259	116213	11.25%	1.515%
3	2.367	332	335	340	rVB4	786	617	0.06%	0.008%
4	2.403	343	346	351	rVB2	731	568	0.05%	0.007%
5	2.557	382	394	413	rBV	218995	362305	35.07%	4.724%
6	2.708	437	441	443	rBV	425	360	0.03%	0.005%
7	2.750	450	454	457	rBV	282	255	0.02%	0.003%
8	2.785	457	465	476	rVB2	1184	2212	0.21%	0.029%
9	2.988	526	528	532	rVV	299	225	0.02%	0.003%
10	3.042	535	545	566	rVV5	2781	6528	0.63%	0.085%
11	3.178	575	587	605	rBV2	4606	10555	1.02%	0.138%
12	3.245	606	608	612	rVB2	420	256	0.02%	0.003%
13	3.335	633	636	639	rBV2	467	316	0.03%	0.004%
14	3.817	785	786	791	rBB	224	177	0.02%	0.002%
15	3.927	816	820	822	rBB	235	157	0.02%	0.002%
16	4.631	1029	1039	1076	rBV	47186	155417	15.04%	2.026%
17	5.055	1155	1171	1191	rBV2	199170	447463	43.31%	5.834%
18	5.583	1330	1335	1337	rBV	167	169	0.02%	0.002%
19	5.718	1356	1377	1410	rBV2	367190	1033204	100.00%	13.470%
20	5.898	1431	1433	1441	rBV2	386	279	0.03%	0.004%
21	5.965	1452	1454	1457	rVB	291	161	0.02%	0.002%
22	6.036	1472	1476	1477	rVV	382	242	0.02%	0.003%
23	6.042	1477	1478	1481	rVB2	393	171	0.02%	0.002%
24	6.081	1487	1490	1493	rBB	294	187	0.02%	0.002%
25	6.242	1527	1540	1559	rBV	335625	647142	62.63%	8.437%
26	6.412	1591	1593	1601	rVB2	353	271	0.03%	0.004%
27	6.512	1618	1624	1625	rBV3	754	556	0.05%	0.007%
28	6.576	1640	1644	1646	rBV3	339	218	0.02%	0.003%
29	6.682	1664	1677	1696	rBV	222798	442895	42.87%	5.774%
30	6.801	1711	1714	1716	rBV	735	529	0.05%	0.007%
31	7.132	1814	1817	1824	rBB2	281	341	0.03%	0.004%
32	7.187	1827	1834	1835	rBV2	452	446	0.04%	0.006%
33	7.197	1835	1837	1840	rVV	662	538	0.05%	0.007%
34	7.226	1844	1846	1850	rVB2	360	233	0.02%	0.003%
35	7.258	1851	1856	1858	rBV	380	261	0.03%	0.003%
36	7.277	1858	1862	1865	rVB	497	273	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
 Data File : VU057432.D
 Acq On : 09 Jan 2024 12:11
 Operator : MD/SY
 Sample : VU0109WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK122

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

37	7.316	1871	1874	1877	rBV	233	182	0.02%	0.002%
38	7.357	1883	1887	1890	rBB	215	183	0.02%	0.002%
39	7.399	1897	1900	1902	rBB2	268	169	0.02%	0.002%
40	7.560	1938	1950	1973	rBV	123220	230976	22.36%	3.011%
41	7.682	1986	1988	1991	rBV	303	224	0.02%	0.003%
42	7.708	1991	1996	1997	rVV	656	619	0.06%	0.008%
43	7.891	2040	2053	2093	rBV	454566	822945	79.65%	10.729%
44	8.174	2129	2141	2167	rBV2	85675	163326	15.81%	2.129%
45	8.303	2177	2181	2186	rBB3	467	432	0.04%	0.006%
46	8.328	2186	2189	2191	rBV	222	159	0.02%	0.002%
47	8.373	2200	2203	2206	rBV	375	257	0.02%	0.003%
48	8.438	2221	2223	2229	rVB3	361	305	0.03%	0.004%
49	8.553	2258	2259	2262	rBV	360	187	0.02%	0.002%
50	8.650	2274	2289	2318	rBV3	168533	388180	37.57%	5.061%
51	8.801	2333	2336	2338	rBV2	362	252	0.02%	0.003%
52	8.853	2350	2352	2356	rVB2	299	220	0.02%	0.003%
53	8.917	2365	2372	2376	rBV5	928	1141	0.11%	0.015%
54	9.287	2482	2487	2489	rBV	153	177	0.02%	0.002%
55	9.361	2507	2510	2513	rBB	198	161	0.02%	0.002%
56	9.415	2513	2527	2567	rBV	443228	806107	78.02%	10.510%
57	9.698	2612	2615	2618	rVB2	558	369	0.04%	0.005%
58	9.717	2618	2621	2623	rVB	342	228	0.02%	0.003%
59	9.746	2624	2630	2633	rBB	172	205	0.02%	0.003%
60	9.772	2635	2638	2641	rBB	409	253	0.02%	0.003%
61	9.933	2683	2688	2691	rBV2	381	404	0.04%	0.005%
62	10.097	2735	2739	2740	rBV2	350	210	0.02%	0.003%
63	10.444	2843	2847	2851	rVB	276	274	0.03%	0.004%
64	10.544	2875	2878	2882	rBV	249	255	0.02%	0.003%
65	10.647	2906	2910	2913	rBB	275	184	0.02%	0.002%
66	10.672	2913	2918	2920	rBV	149	167	0.02%	0.002%
67	10.698	2923	2926	2928	rBV	271	212	0.02%	0.003%
68	10.756	2932	2944	2961	rBV	296528	483960	46.84%	6.310%
69	10.978	3009	3013	3016	rBV	346	250	0.02%	0.003%
70	11.090	3041	3048	3054	rBV3	916	1006	0.10%	0.013%
71	11.190	3076	3079	3083	rVB	305	245	0.02%	0.003%
72	11.222	3084	3089	3092	rBB	279	258	0.02%	0.003%
73	11.251	3093	3098	3101	rBV	256	254	0.02%	0.003%
74	11.473	3160	3167	3173	rBV4	1345	1625	0.16%	0.021%
75	11.531	3180	3185	3186	rBV4	319	248	0.02%	0.003%
76	11.746	3245	3252	3259	rBV2	1775	2247	0.22%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
 Data File : VU057432.D
 Acq On : 09 Jan 2024 12:11
 Operator : MD/SY
 Sample : VU0109WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK122

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

77	11.807	3259	3271	3290	rBV	412237	666332	64.49%	8.687%
78	12.190	3378	3390	3411	rBV	422194	687726	66.56%	8.966%
79	12.692	3543	3546	3549	rBV2	257	196	0.02%	0.003%
80	12.753	3563	3565	3567	rBV	322	223	0.02%	0.003%
81	13.090	3667	3670	3679	rVB2	351	359	0.03%	0.005%
82	13.135	3679	3684	3688	rBV2	269	280	0.03%	0.004%
83	13.229	3707	3713	3722	rVB4	2223	3085	0.30%	0.040%
84	13.274	3723	3727	3730	rBV2	228	201	0.02%	0.003%
85	13.331	3740	3745	3747	rBV	344	326	0.03%	0.004%
86	13.643	3840	3842	3844	rBV	310	159	0.02%	0.002%
87	13.843	3895	3904	3915	rBV6	4551	7594	0.73%	0.099%
88	14.093	3972	3982	3993	rBV3	5963	10710	1.04%	0.140%
89	14.238	4024	4027	4029	rBV	495	299	0.03%	0.004%
90	14.328	4048	4055	4064	rVB5	5474	8499	0.82%	0.111%
91	14.730	4176	4180	4182	rBV2	505	424	0.04%	0.006%
92	14.859	4218	4220	4227	rVB	393	393	0.04%	0.005%
93	14.891	4227	4230	4234	rBV2	590	522	0.05%	0.007%
94	14.971	4252	4255	4258	rBV2	517	417	0.04%	0.005%
95	15.110	4295	4298	4299	rBV	395	267	0.03%	0.003%
96	15.190	4318	4323	4327	rBV4	876	775	0.08%	0.010%
97	15.209	4327	4329	4335	rBV3	368	204	0.02%	0.003%
98	15.232	4335	4336	4339	rBV2	472	297	0.03%	0.004%
99	15.637	4461	4462	4463	rBV	632	175	0.02%	0.002%
100	15.701	4480	4482	4486	rBV2	724	503	0.05%	0.007%




Sum of corrected areas: 7670204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057432.D
Acq On : 09 Jan 2024 12:11
Operator : MD/SY
Sample : VU0109WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

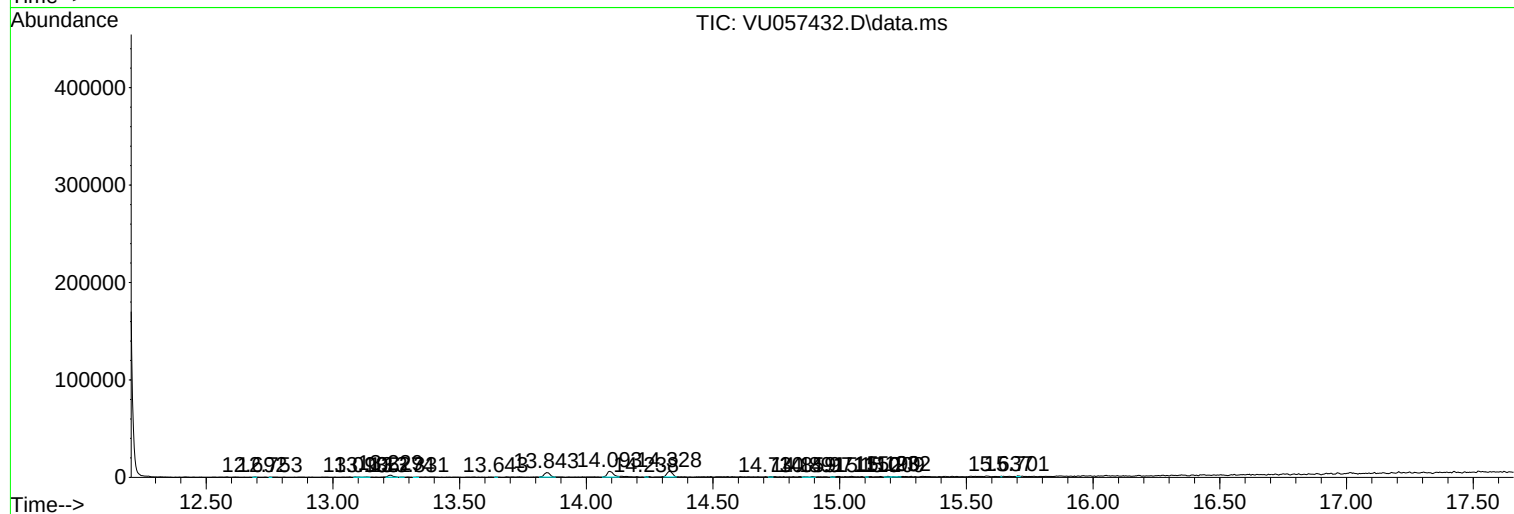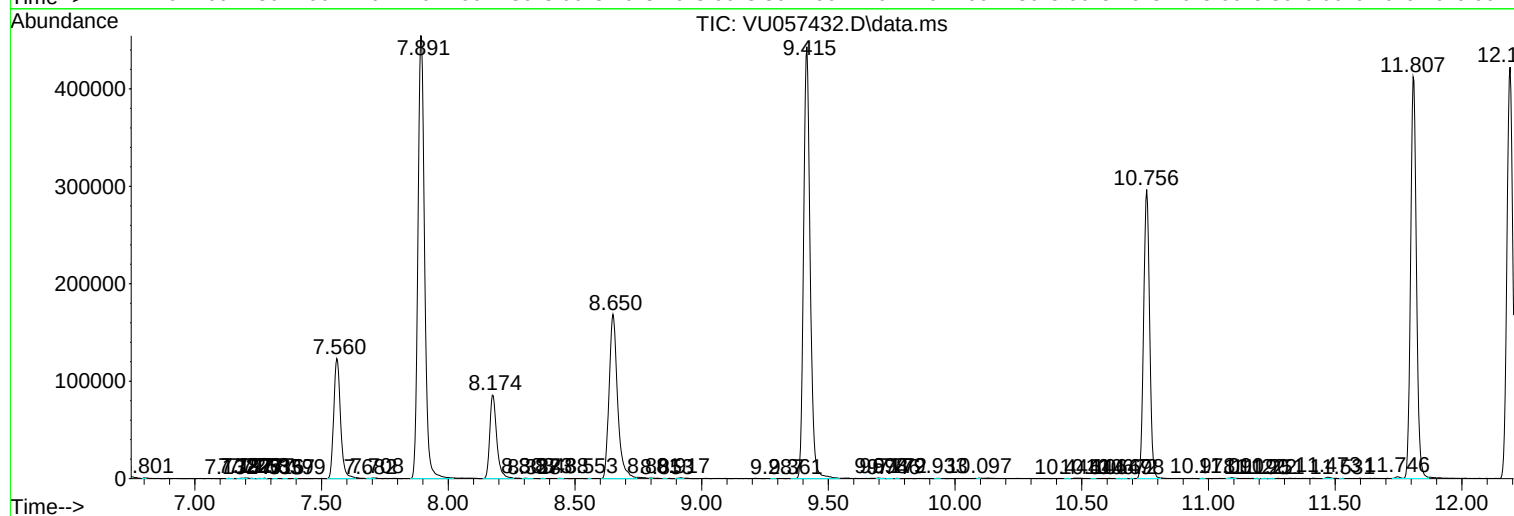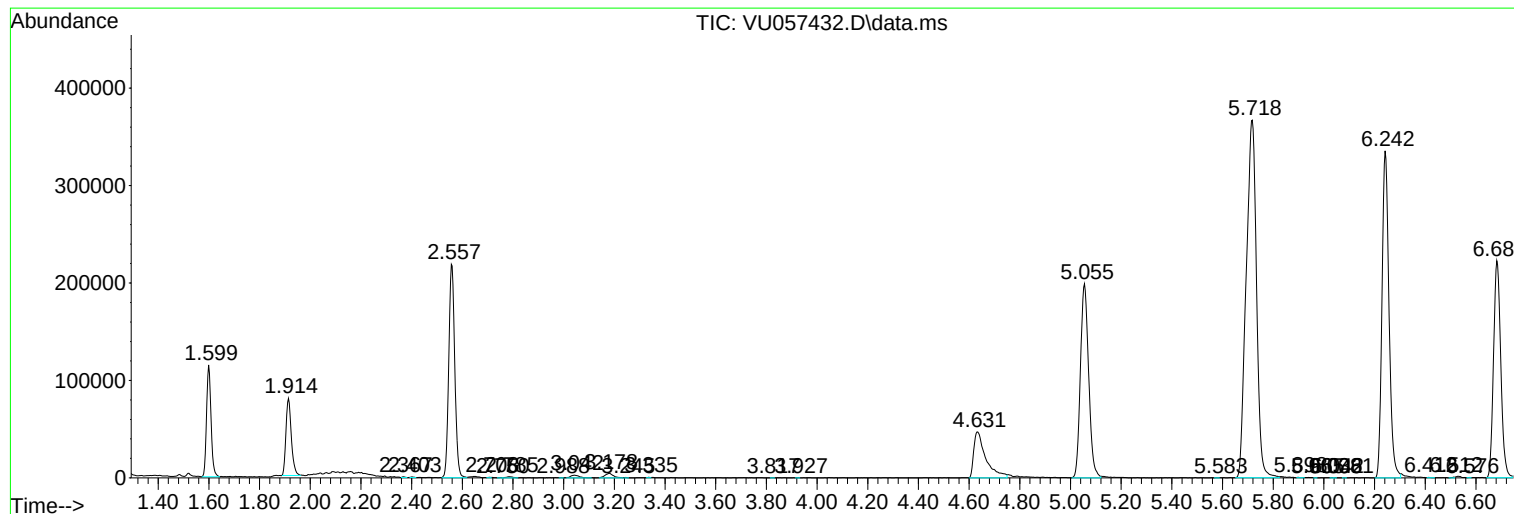

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057432.D
Acq On : 09 Jan 2024 12:11
Operator : MD/SY
Sample : VU0109WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057432.D
Acq On : 09 Jan 2024 12:11
Operator : MD/SY
Sample : VU0109WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------