

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
 Data File : VU057441.D
 Acq On : 09 Jan 2024 15:48
 Operator : MD/SY
 Sample : 05787-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

Signal : TIC: VU057441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.357	15	21	33	rBV2	19727	22048	2.30%	0.274%
2	1.599	86	96	109	rBV	94037	120541	12.56%	1.496%
3	1.911	186	193	210	rVB	68598	98893	10.31%	1.227%
4	2.306	313	316	317	rBV2	619	318	0.03%	0.004%
5	2.496	371	375	377	rBV	432	343	0.04%	0.004%
6	2.560	382	395	409	rBV	185619	304881	31.78%	3.783%
7	2.644	410	421	450	rVV	35850	97704	10.18%	1.212%
8	3.428	662	665	668	rVB	263	190	0.02%	0.002%
9	3.602	717	719	722	rVB	372	194	0.02%	0.002%
10	3.843	783	794	798	rBV3	3224	4968	0.52%	0.062%
11	3.914	812	816	818	rBB	216	175	0.02%	0.002%
12	4.164	891	894	899	rBB	235	235	0.02%	0.003%
13	4.219	909	911	914	rVB	306	179	0.02%	0.002%
14	4.515	1000	1003	1008	rBV	151	210	0.02%	0.003%
15	4.634	1029	1040	1075	rBV2	41541	151979	15.84%	1.886%
16	4.946	1134	1137	1140	rBV2	437	271	0.03%	0.003%
17	4.994	1150	1152	1155	rBV2	273	204	0.02%	0.003%
18	5.055	1155	1171	1200	rVV	185629	422036	43.99%	5.237%
19	5.325	1251	1255	1257	rBB2	307	210	0.02%	0.003%
20	5.402	1274	1279	1281	rBB2	267	194	0.02%	0.002%
21	5.557	1323	1327	1330	rBB2	277	189	0.02%	0.002%
22	5.717	1357	1377	1413	rBV2	345391	959456	100.00%	11.905%
23	5.994	1461	1463	1465	rVV2	337	172	0.02%	0.002%
24	6.016	1467	1470	1474	rVB2	316	258	0.03%	0.003%
25	6.049	1477	1480	1487	rBB3	306	366	0.04%	0.005%
26	6.242	1527	1540	1572	rBV	321799	638470	66.55%	7.922%
27	6.541	1623	1633	1644	rBB5	6789	12026	1.25%	0.149%
28	6.586	1644	1647	1648	rBV	368	213	0.02%	0.003%
29	6.631	1658	1661	1663	rBV	239	166	0.02%	0.002%
30	6.682	1663	1677	1706	rVV	207366	413926	43.14%	5.136%
31	6.782	1706	1708	1713	rVB3	582	383	0.04%	0.005%
32	6.804	1713	1715	1717	rBV	429	235	0.02%	0.003%
33	7.158	1821	1825	1828	rBB	289	208	0.02%	0.003%
34	7.200	1831	1838	1843	rBV2	546	951	0.10%	0.012%
35	7.270	1856	1860	1862	rBV	372	246	0.03%	0.003%
36	7.312	1870	1873	1875	rBB	318	194	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
 Data File : VU057441.D
 Acq On : 09 Jan 2024 15:48
 Operator : MD/SY
 Sample : 05787-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

37	7.560	1938	1950	1968	rBV	114316	213473	22.25%	2.649%
38	7.711	1994	1997	2001	rBV2	722	526	0.05%	0.007%
39	7.807	2022	2027	2030	rBV2	482	427	0.04%	0.005%
40	7.891	2040	2053	2071	rBV	404530	726981	75.77%	9.020%
41	8.174	2130	2141	2165	rBV	82034	152770	15.92%	1.896%
42	8.444	2224	2225	2230	rBV	254	177	0.02%	0.002%
43	8.473	2231	2234	2236	rVB2	402	204	0.02%	0.003%
44	8.547	2243	2257	2275	rBV	467265	790286	82.37%	9.806%
45	8.643	2276	2287	2318	rVB2	164421	360672	37.59%	4.475%
46	8.823	2339	2343	2344	rBV2	475	260	0.03%	0.003%
47	8.920	2371	2373	2377	rBV	318	279	0.03%	0.003%
48	8.987	2390	2394	2398	rBV	340	301	0.03%	0.004%
49	9.415	2513	2527	2549	rBV	442681	782437	81.55%	9.709%
50	9.695	2608	2614	2620	rBV3	460	484	0.05%	0.006%
51	9.875	2667	2670	2674	rVB	374	263	0.03%	0.003%
52	9.904	2675	2679	2682	rBB	280	185	0.02%	0.002%
53	9.955	2692	2695	2697	rVB	302	188	0.02%	0.002%
54	9.987	2700	2705	2707	rBV	239	240	0.03%	0.003%
55	10.036	2716	2720	2723	rBB	207	187	0.02%	0.002%
56	10.138	2748	2752	2754	rBV	177	189	0.02%	0.002%
57	10.241	2778	2784	2787	rBB	308	219	0.02%	0.003%
58	10.328	2807	2811	2814	rBV	357	291	0.03%	0.004%
59	10.409	2831	2836	2838	rBB	187	170	0.02%	0.002%
60	10.476	2854	2857	2861	rBV	261	260	0.03%	0.003%
61	10.511	2865	2868	2873	rBV	189	195	0.02%	0.002%
62	10.753	2930	2943	2964	rVV	281742	460799	48.03%	5.718%
63	10.830	2965	2967	2974	rVB2	667	634	0.07%	0.008%
64	11.042	3030	3033	3039	rVB2	189	199	0.02%	0.002%
65	11.148	3064	3066	3070	rVB	461	233	0.02%	0.003%
66	11.193	3077	3080	3085	rBB2	310	270	0.03%	0.003%
67	11.248	3092	3097	3100	rBV	308	278	0.03%	0.003%
68	11.309	3110	3116	3117	rBV	214	191	0.02%	0.002%
69	11.357	3129	3131	3134	rVB	413	234	0.02%	0.003%
70	11.370	3134	3135	3139	rBV	240	189	0.02%	0.002%
71	11.405	3142	3146	3153	rBV	552	547	0.06%	0.007%
72	11.470	3163	3166	3172	rVB2	433	472	0.05%	0.006%
73	11.746	3249	3252	3254	rVV	353	173	0.02%	0.002%
74	11.807	3260	3271	3295	rBV	403693	655961	68.37%	8.139%
75	12.023	3335	3338	3343	rBV2	271	177	0.02%	0.002%
76	12.048	3343	3346	3349	rVB2	276	181	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
 Data File : VU057441.D
 Acq On : 09 Jan 2024 15:48
 Operator : MD/SY
 Sample : 05787-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

77	12.068	3349	3352	3359	rVB	374	389	0.04%	0.005%
78	12.116	3362	3367	3369	rBV	543	482	0.05%	0.006%
79	12.190	3376	3390	3411	rBV	391405	645909	67.32%	8.015%
80	12.290	3419	3421	3424	rBV2	487	262	0.03%	0.003%
81	12.415	3457	3460	3464	rBV2	282	233	0.02%	0.003%
82	12.437	3464	3467	3470	rBV2	301	208	0.02%	0.003%
83	12.637	3526	3529	3532	rBV	335	244	0.03%	0.003%
84	12.762	3562	3568	3570	rBV3	577	647	0.07%	0.008%
85	13.145	3682	3687	3689	rBV	304	311	0.03%	0.004%
86	13.463	3783	3786	3790	rBV2	301	172	0.02%	0.002%
87	13.569	3817	3819	3823	rVB	295	189	0.02%	0.002%
88	13.698	3857	3859	3862	rVV	298	172	0.02%	0.002%
89	13.746	3869	3874	3877	rBV3	464	395	0.04%	0.005%
90	13.765	3877	3880	3884	rBV2	423	276	0.03%	0.003%
91	13.833	3898	3901	3902	rBV2	477	250	0.03%	0.003%
92	14.039	3960	3965	3971	rBV3	608	626	0.07%	0.008%
93	14.068	3971	3974	3977	rBV	363	257	0.03%	0.003%
94	14.283	4039	4041	4046	rBV2	273	235	0.02%	0.003%
95	14.447	4088	4092	4096	rBV	688	676	0.07%	0.008%
96	14.556	4123	4126	4128	rBV2	676	415	0.04%	0.005%
97	14.643	4151	4153	4155	rBV	404	224	0.02%	0.003%
98	14.830	4208	4211	4212	rBV	284	187	0.02%	0.002%
99	15.055	4277	4281	4282	rBV2	513	383	0.04%	0.005%
100	15.360	4369	4376	4379	rBV4	625	673	0.07%	0.008%




Sum of corrected areas: 8059249

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057441.D
Acq On : 09 Jan 2024 15:48
Operator : MD/SY
Sample : 05787-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

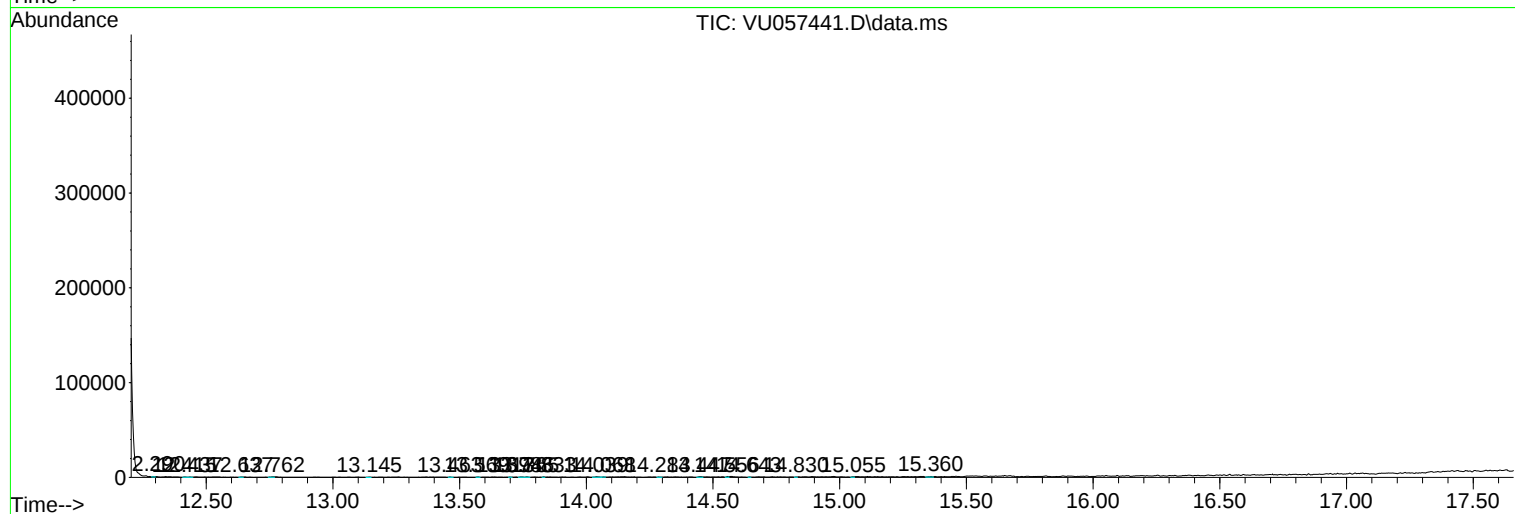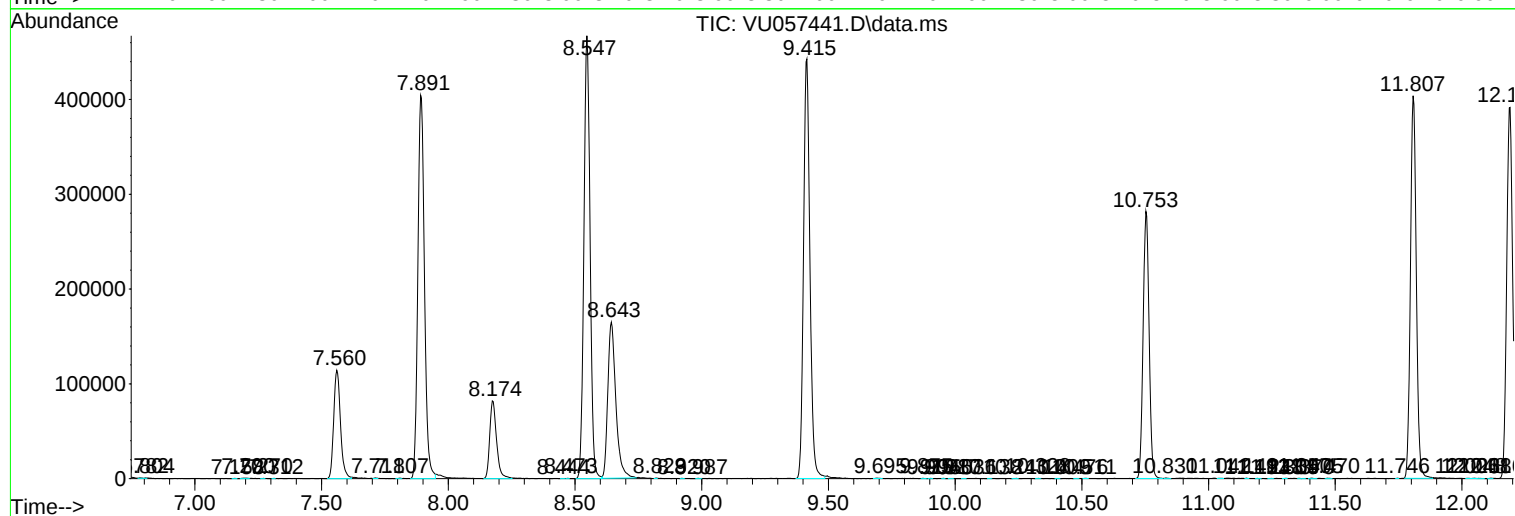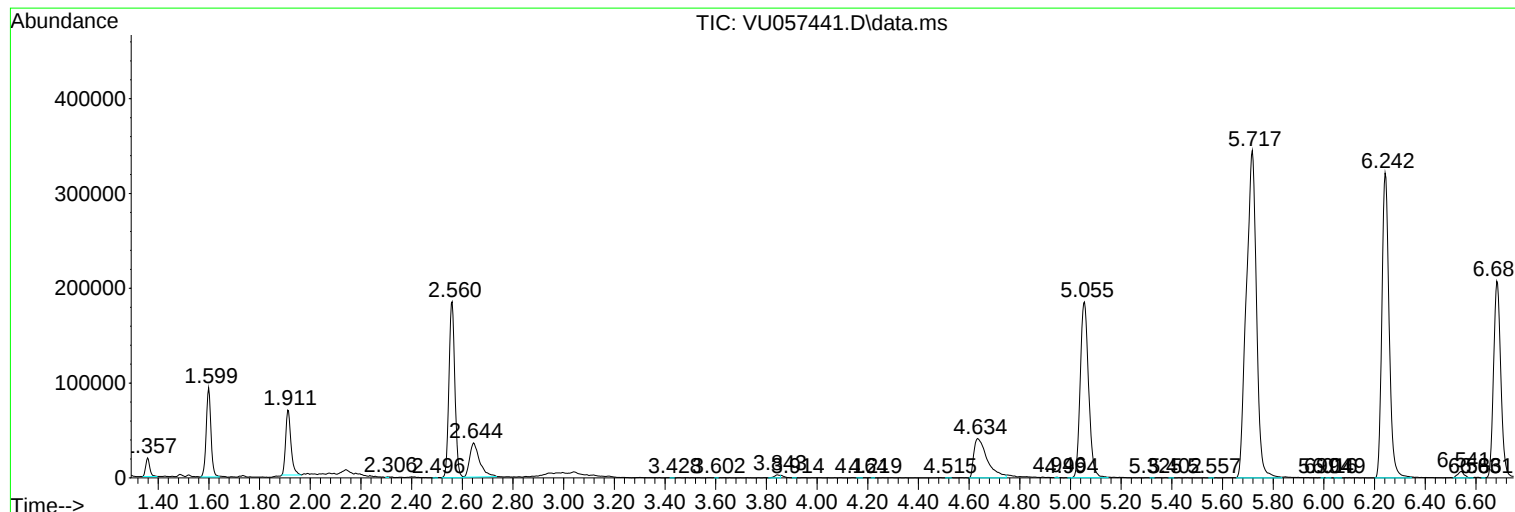

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057441.D
Acq On : 09 Jan 2024 15:48
Operator : MD/SY
Sample : 05787-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057441.D
Acq On : 09 Jan 2024 15:48
Operator : MD/SY
Sample : 05787-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------