

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
 Data File : VU057443.D
 Acq On : 09 Jan 2024 16:36
 Operator : MD/SY
 Sample : 05787-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

Signal : TIC: VU057443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	16	21	31	rVB	17368	17590	1.33%	0.202%
2	1.599	87	96	111	rVB	99506	123190	9.32%	1.417%
3	1.914	186	194	210	rVB	73762	104255	7.89%	1.199%
4	2.284	306	309	310	rBV2	518	298	0.02%	0.003%
5	2.364	332	334	337	rBV	258	173	0.01%	0.002%
6	2.560	382	395	411	rBV	188422	308409	23.33%	3.547%
7	2.785	459	465	467	rBV4	757	797	0.06%	0.009%
8	2.853	476	486	489	rBV4	1376	2200	0.17%	0.025%
9	3.274	614	617	620	rBB2	290	180	0.01%	0.002%
10	3.367	643	646	650	rBB	223	186	0.01%	0.002%
11	3.637	727	730	735	rBB	203	211	0.02%	0.002%
12	3.766	765	770	772	rBB	255	170	0.01%	0.002%
13	3.846	785	795	797	rBV2	3165	4228	0.32%	0.049%
14	3.946	824	826	828	rBV	276	169	0.01%	0.002%
15	4.528	1003	1007	1010	rBB	190	174	0.01%	0.002%
16	4.634	1025	1040	1075	rBV2	46660	172568	13.05%	1.985%
17	4.878	1114	1116	1119	rBV	329	265	0.02%	0.003%
18	4.914	1125	1127	1131	rVB2	341	174	0.01%	0.002%
19	4.981	1144	1148	1152	rVB	358	190	0.01%	0.002%
20	5.055	1155	1171	1193	rBV	186680	417526	31.58%	4.802%
21	5.222	1218	1223	1229	rVB	255	270	0.02%	0.003%
22	5.271	1235	1238	1241	rBB	301	204	0.02%	0.002%
23	5.396	1274	1277	1281	rBB	280	225	0.02%	0.003%
24	5.718	1357	1377	1409	rBV2	344317	957203	72.40%	11.009%
25	5.910	1433	1437	1440	rBV	245	220	0.02%	0.003%
26	5.933	1442	1444	1449	rVB2	384	261	0.02%	0.003%
27	5.978	1453	1458	1461	rBB3	259	222	0.02%	0.003%
28	6.000	1462	1465	1466	rBV	338	180	0.01%	0.002%
29	6.042	1476	1478	1481	rVB	460	224	0.02%	0.003%
30	6.242	1528	1540	1565	rVV2	320760	622173	47.06%	7.156%
31	6.386	1583	1585	1592	rVB2	347	314	0.02%	0.004%
32	6.496	1614	1619	1622	rBB	222	246	0.02%	0.003%
33	6.537	1622	1632	1647	rBB4	11562	22303	1.69%	0.257%
34	6.605	1651	1653	1655	rBV	370	252	0.02%	0.003%
35	6.682	1664	1677	1699	rBV2	209534	411606	31.13%	4.734%
36	6.808	1712	1716	1719	rVB3	982	861	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
 Data File : VU057443.D
 Acq On : 09 Jan 2024 16:36
 Operator : MD/SY
 Sample : 05787-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

37	6.894	1739	1743	1746	rBB2	249	194	0.01%	0.002%
38	7.164	1820	1827	1828	rBB	214	207	0.02%	0.002%
39	7.190	1829	1835	1843	rBV4	902	1255	0.09%	0.014%
40	7.364	1886	1889	1891	rBB	313	179	0.01%	0.002%
41	7.422	1905	1907	1911	rBB2	297	204	0.02%	0.002%
42	7.473	1920	1923	1927	rBV	313	210	0.02%	0.002%
43	7.560	1939	1950	1979	rBV	119090	214985	16.26%	2.473%
44	7.663	1979	1982	1985	rVB2	735	417	0.03%	0.005%
45	7.708	1989	1996	1998	rVV2	538	589	0.04%	0.007%
46	7.756	2009	2011	2016	rVB	284	210	0.02%	0.002%
47	7.807	2022	2027	2029	rBV2	510	460	0.03%	0.005%
48	7.891	2040	2053	2073	rBV	414864	737915	55.82%	8.487%
49	8.087	2111	2114	2120	rVB2	325	314	0.02%	0.004%
50	8.116	2120	2123	2127	rVB	333	308	0.02%	0.004%
51	8.174	2131	2141	2161	rBV2	82322	152660	11.55%	1.756%
52	8.380	2203	2205	2208	rVB	369	180	0.01%	0.002%
53	8.434	2220	2222	2226	rBV	291	233	0.02%	0.003%
54	8.473	2233	2234	2237	rVB	400	167	0.01%	0.002%
55	8.547	2243	2257	2275	rBV	771158	1322024	100.00%	15.206%
56	8.640	2276	2286	2315	rVB3	174571	364511	27.57%	4.193%
57	8.936	2374	2378	2380	rBV2	604	389	0.03%	0.004%
58	9.016	2400	2403	2405	rBV	403	275	0.02%	0.003%
59	9.074	2419	2421	2425	rBB	335	247	0.02%	0.003%
60	9.200	2457	2460	2461	rBV2	328	201	0.02%	0.002%
61	9.232	2468	2470	2474	rBB	337	246	0.02%	0.003%
62	9.412	2513	2526	2552	rBV	436951	758172	57.35%	8.720%
63	9.573	2573	2576	2579	rVB3	390	213	0.02%	0.002%
64	9.621	2590	2591	2596	rVB	267	195	0.01%	0.002%
65	9.663	2601	2604	2608	rBB	198	175	0.01%	0.002%
66	9.695	2611	2614	2615	rBV2	458	296	0.02%	0.003%
67	9.766	2631	2636	2637	rBV	248	215	0.02%	0.002%
68	9.917	2679	2683	2687	rBB	255	258	0.02%	0.003%
69	9.991	2703	2706	2710	rBB	220	198	0.01%	0.002%
70	10.020	2710	2715	2718	rBV	348	378	0.03%	0.004%
71	10.081	2730	2734	2736	rBV	211	191	0.01%	0.002%
72	10.106	2739	2742	2745	rBB	250	175	0.01%	0.002%
73	10.338	2810	2814	2816	rBV	265	223	0.02%	0.003%
74	10.624	2900	2903	2909	rVB2	365	292	0.02%	0.003%
75	10.753	2930	2943	2964	rBV	404169	663057	50.15%	7.626%
76	11.129	3057	3060	3063	rBV	283	210	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
 Data File : VU057443.D
 Acq On : 09 Jan 2024 16:36
 Operator : MD/SY
 Sample : 05787-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
 Title : VOC Analysis

77	11.312	3115	3117	3120	rVB2	529	280	0.02%	0.003%
78	11.335	3121	3124	3126	rBV	204	182	0.01%	0.002%
79	11.383	3135	3139	3142	rBB	174	166	0.01%	0.002%
80	11.402	3142	3145	3147	rBV	351	218	0.02%	0.003%
81	11.483	3167	3170	3172	rBV2	590	363	0.03%	0.004%
82	11.569	3193	3197	3198	rBV	292	236	0.02%	0.003%
83	11.730	3245	3247	3249	rBV	343	191	0.01%	0.002%
84	11.807	3259	3271	3292	rBV	401248	638985	48.33%	7.349%
85	12.042	3340	3344	3351	rBV	197	247	0.02%	0.003%
86	12.077	3351	3355	3358	rBV2	332	259	0.02%	0.003%
87	12.100	3358	3362	3366	rBV3	665	657	0.05%	0.008%
88	12.190	3377	3390	3409	rBV	395905	655964	49.62%	7.545%
89	12.299	3422	3424	3433	rVB3	556	457	0.03%	0.005%
90	12.762	3565	3568	3569	rBV	428	248	0.02%	0.003%
91	12.862	3595	3599	3602	rBV	321	314	0.02%	0.004%
92	13.290	3729	3732	3733	rBV	438	170	0.01%	0.002%
93	13.991	3947	3950	3952	rVV3	435	254	0.02%	0.003%
94	14.357	4061	4064	4067	rBV3	540	395	0.03%	0.005%
95	14.479	4099	4102	4104	rBV	511	286	0.02%	0.003%
96	14.547	4121	4123	4126	rBV	308	185	0.01%	0.002%
97	14.634	4147	4150	4151	rBV	474	300	0.02%	0.003%
98	14.666	4157	4160	4163	rBV	392	253	0.02%	0.003%
99	15.415	4389	4393	4395	rBV	710	530	0.04%	0.006%
100	15.473	4407	4411	4414	rBV2	779	663	0.05%	0.008%




Sum of corrected areas: 8694348

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057443.D
Acq On : 09 Jan 2024 16:36
Operator : MD/SY
Sample : 05787-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

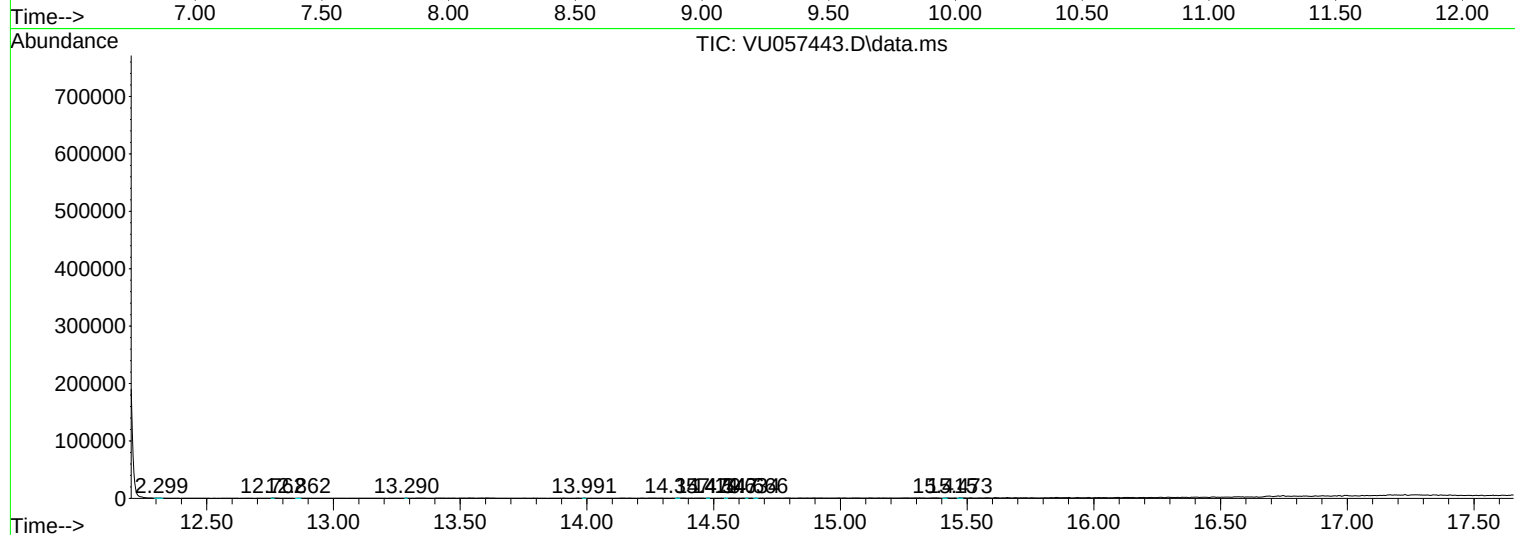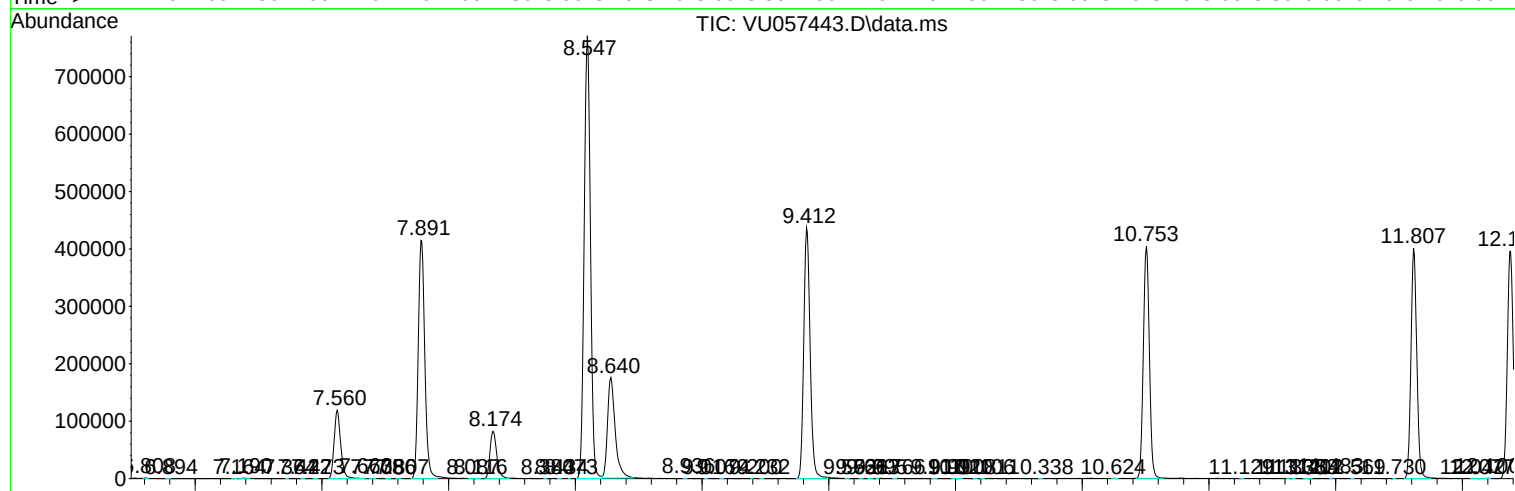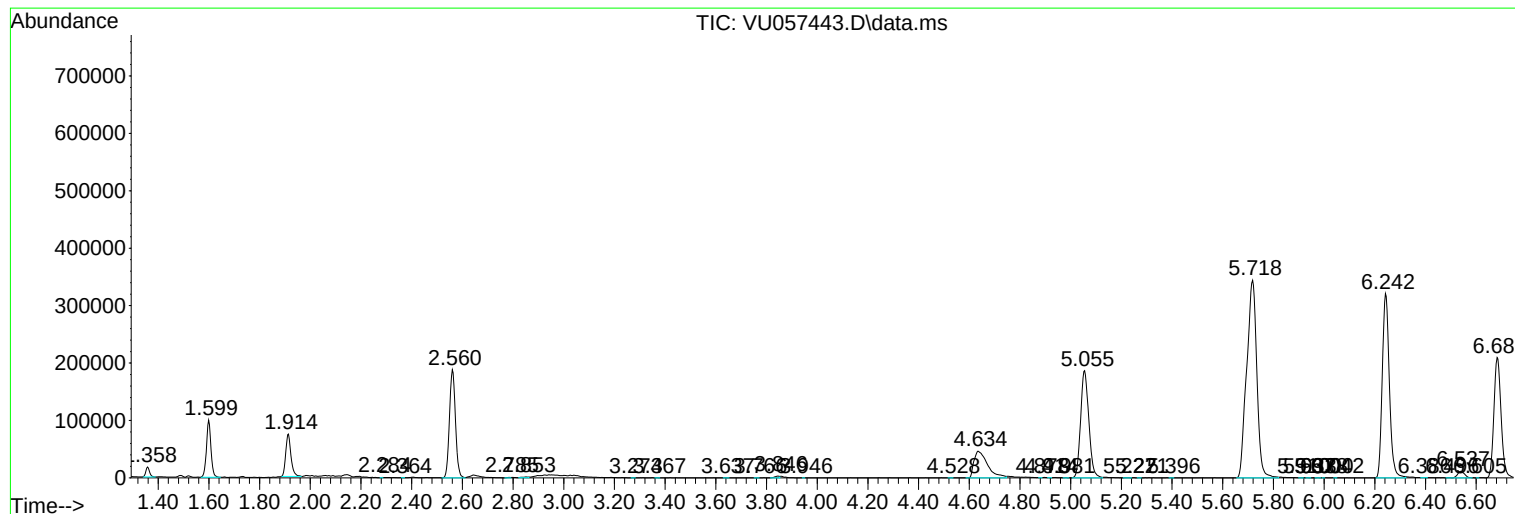

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057443.D
Acq On : 09 Jan 2024 16:36
Operator : MD/SY
Sample : 05787-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057443.D
Acq On : 09 Jan 2024 16:36
Operator : MD/SY
Sample : 05787-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------