
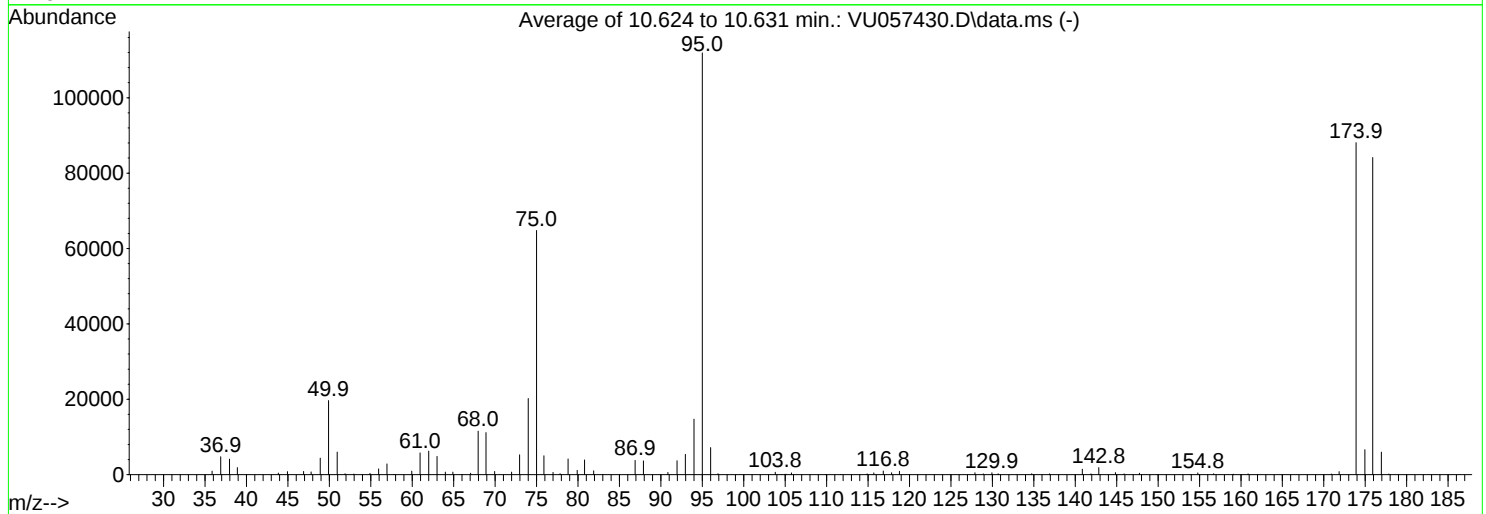


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010924\
Data File : VU057430.D
Acq On : 09 Jan 2024 10:52
Operator : MD/SY
Sample : BFB032
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB032

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010824WMA.M
Title : VOC Analysis
Last Update : Wed Jan 10 11:26:47 2024

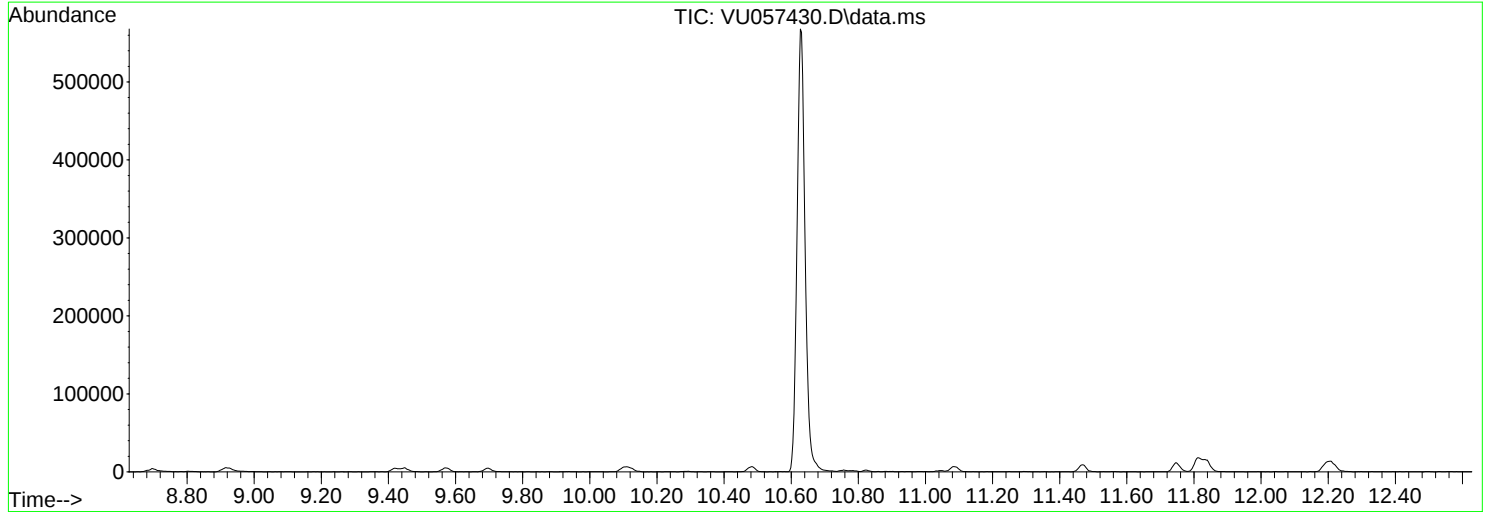

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	19664	PASS
75	95	30	80	57.9	64787	PASS
95	95	100	100	100.0	111923	PASS
96	95	5	9	6.4	7169	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.7	88096	PASS
175	174	5	9	7.5	6605	PASS
176	174	95	101	95.5	84165	PASS
177	176	5	9	7.1	5992	PASS

m/z	Abundance
44.00	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.90	887.0
36.90	4466.0
37.90	4049.0
38.90	1784.0
43.90	474.0
45.00	787.0
46.90	707.0
47.80	791.0
48.90	4348.0
49.90	18712.0
51.00	5883.0
51.90	289.0
53.00	173.0
54.90	296.0
55.90	1493.0
56.90	2793.0
57.80	107.0
60.00	871.0
61.00	5355.0
62.00	6022.0
63.00	4648.0
64.00	806.0
64.90	700.0
67.10	350.0
68.00	10740.0
68.90	10798.0
69.90	786.0
72.00	664.0
73.00	4635.0
74.00	19584.0
75.00	62456.0
75.90	4913.0
77.00	574.0
78.80	4044.0
79.90	1040.0
80.80	3892.0
81.90	941.0
83.00	114.0
86.90	3915.0
87.90	3456.0
90.90	545.0
91.90	3258.0
92.90	5036.0
94.00	13931.0
95.00	105936.0
96.00	6808.0
96.90	219.0
103.70	546.0
104.90	219.0
105.70	449.0
114.90	190.0
115.70	512.0
116.80	964.0
118.00	472.0
118.80	828.0
127.90	469.0
128.90	163.0
130.00	461.0
130.70	265.0
134.70	187.0
136.90	126.0
140.90	1230.0
141.80	244.0
142.80	1795.0
144.90	531.0
145.90	147.0
147.80	360.0
149.90	117.0
154.80	446.0
156.70	295.0
159.10	114.0
160.80	234.0
170.90	169.0
171.90	688.0
173.90	81648.0
175.00	6381.0
175.90	77128.0
177.00	5400.0
177.90	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.90	932.0
36.90	5031.0
37.90	4286.0
38.90	2004.0
43.90	566.0
45.00	867.0
46.90	888.0
47.80	761.0
48.90	4502.0
49.90	20536.0
51.00	6154.0
51.90	268.0
52.90	193.0
54.90	362.0
55.90	1505.0
56.90	2965.0
57.80	102.0
60.00	949.0
60.90	6000.0
62.00	6549.0
63.00	4988.0
64.00	702.0
64.90	644.0
66.00	102.0
67.00	399.0
68.00	11977.0
68.90	11404.0
70.00	876.0
72.00	755.0
72.90	5453.0
74.00	20696.0
75.00	67112.0
75.90	5162.0
77.00	607.0
77.90	380.0
78.80	4284.0
79.90	1171.0
80.80	4078.0
81.90	1088.0
83.00	125.0
86.90	3915.0
87.90	3746.0
90.80	624.0
91.90	3802.0
93.00	5566.0
94.00	15364.0
95.00	115304.0
96.00	7458.0
96.90	273.0
103.80	615.0
105.10	208.0
105.80	455.0
114.90	224.0
115.70	482.0
116.80	1022.0
117.80	522.0
118.80	909.0
127.90	554.0
128.90	202.0
130.00	536.0
130.70	259.0
134.80	232.0
136.90	192.0
140.90	1487.0
141.90	208.0
142.90	1857.0
144.80	595.0
145.90	239.0
147.70	416.0
154.80	483.0
156.70	275.0
159.10	126.0
160.80	232.0
170.90	182.0
171.90	803.0
173.90	91312.0
175.00	6737.0
175.90	86712.0
176.90	6136.0
177.90	175.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.80	978.0
36.90	4795.0
38.00	4002.0
38.90	1859.0
43.80	684.0
44.90	840.0
46.90	938.0
47.80	645.0
48.90	4307.0
49.90	19744.0
50.90	5919.0
51.90	230.0
52.90	190.0
54.90	364.0
56.00	1645.0
57.00	2835.0
59.90	1042.0
60.90	6007.0
62.00	6140.0
63.00	4912.0
64.00	569.0
64.90	648.0
67.00	372.0
67.90	11974.0
68.90	11294.0
70.00	923.0
72.00	676.0
72.90	5715.0
74.00	20304.0
75.00	64792.0
75.90	4937.0
77.00	612.0
77.80	374.0
78.80	4111.0
79.90	1234.0
80.80	3805.0
81.90	1082.0
86.90	3526.0
87.90	3711.0
90.80	590.0
92.00	4057.0
93.00	5596.0
94.00	14948.0
95.00	114528.0
96.00	7241.0
96.90	285.0
103.90	712.0
104.60	178.0
105.10	164.0
105.80	511.0
109.90	116.0
111.70	117.0
114.90	267.0
115.70	465.0
116.90	1009.0
117.80	516.0
118.80	943.0
127.90	481.0
128.90	261.0
129.90	505.0
130.70	243.0
134.80	292.0
136.90	281.0
140.80	1598.0
142.00	139.0
142.90	2003.0
144.80	599.0
145.90	285.0
147.70	374.0
153.90	129.0
154.80	443.0
156.70	218.0
159.10	131.0
160.90	221.0
170.90	174.0
171.80	882.0
173.90	91328.0
174.90	6696.0
175.90	88656.0
176.90	6441.0
177.80	166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032