

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU011019\
 Data File : VU029105.D
 Acq On : 10 Jan 2019 09:49
 Operator : MD/SY
 Sample : VU0110WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0110WBL01

Quant Time: Jan 11 02:59:08 2019
 Quant Method : Z:\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 04 02:22:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.98	168	104690	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.88	114	179413	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	159436	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	59204	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.30	65	71927	55.58	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.16%	
35) Dibromofluoromethane	4.88	113	64043	55.07	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.14%	
50) Toluene-d8	7.56	98	228468	49.76	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.52%	
62) 4-Bromofluorobenzene	10.30	95	65920	39.95	ug/l	0.00
Spiked Amount	50.000		Recovery	=	79.90%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU011019\
Data File : VU029105.D
Acq On : 10 Jan 2019 09:49
Operator : MD/SY
Sample : VU0110WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0110WBL01

Quant Time: Jan 11 02:59:08 2019
Quant Method : Z:\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
Quant Title : SW846 8260
QLast Update : Fri Jan 04 02:22:53 2019
Response via : Initial Calibration

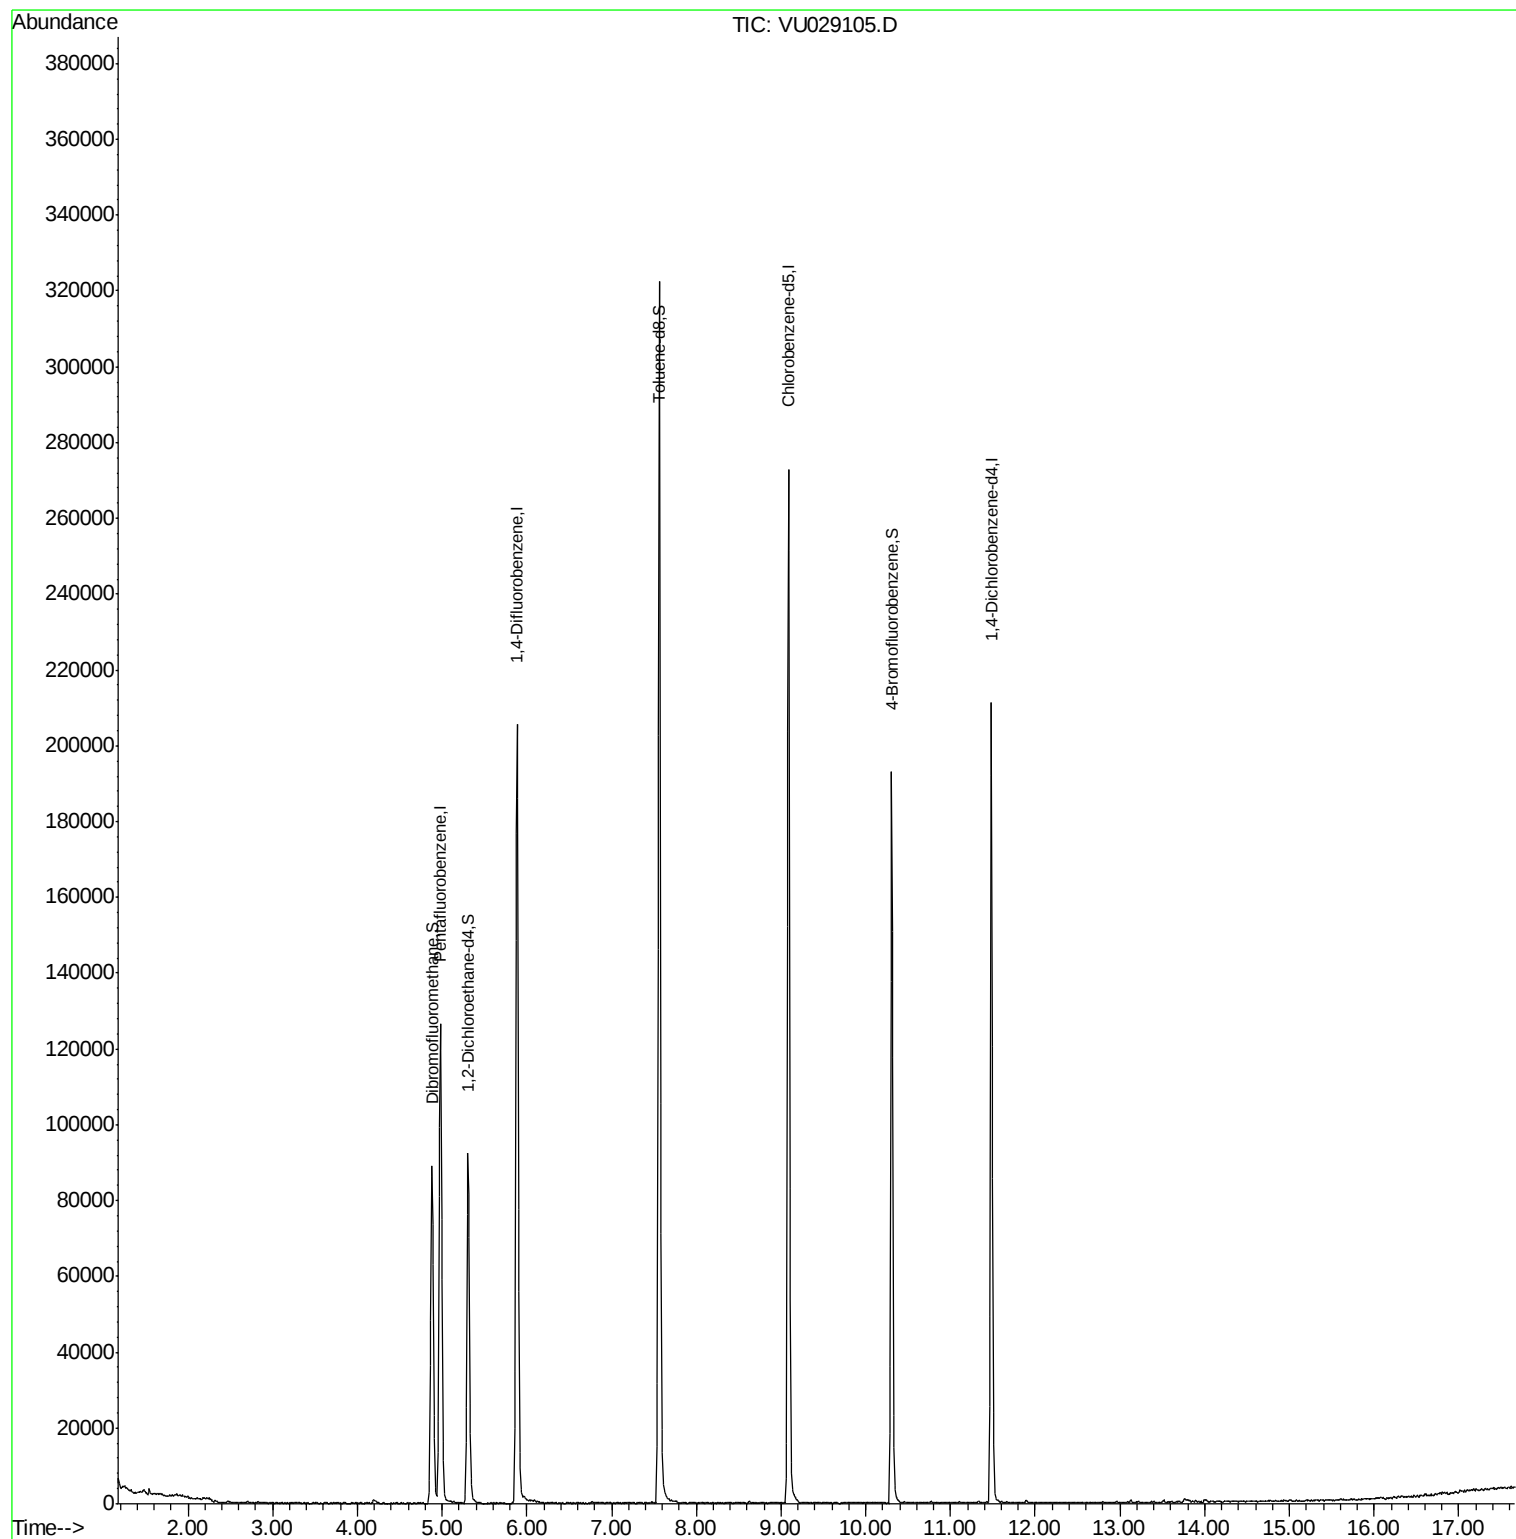

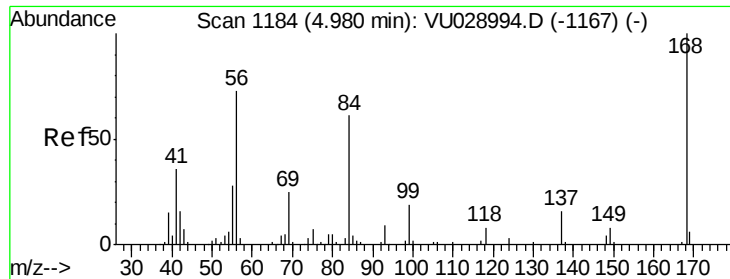

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1185

Delta R.T. 0.00 min

Lab File: VU029105.D

Acq: 10 Jan 2019 09:49

Instrument :

MSVOA_U

ClientSampleId :


VU0110WBL01

Tgt Ion: 168 Resp: 104690

Ion Ratio Lower Upper

168 100

99 52.4 42.0 63.0

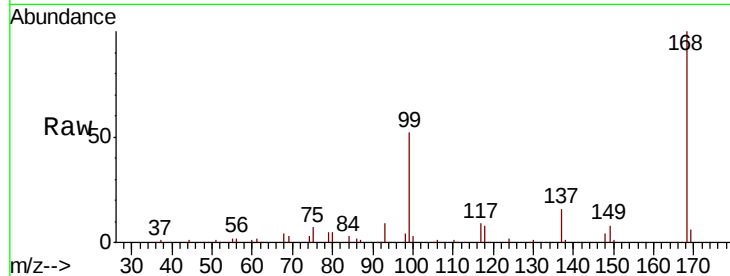

Abundance Ion 167.90 (167.60 to 168.60): VU028994.D (-1167) (-)

Ion 98.90 (98.60 to 99.60): VU029105.D (-1091) (-)

4.98

50000

40000

30000

20000

10000



0

4.90

5.00

5.10

Time-->

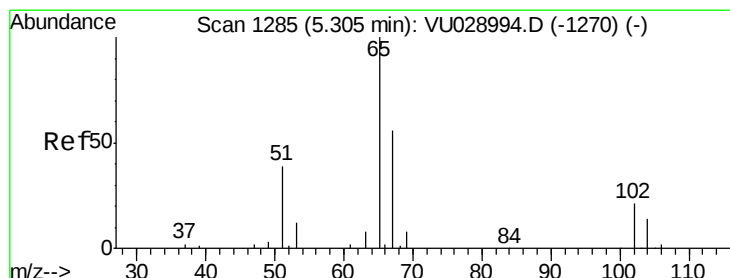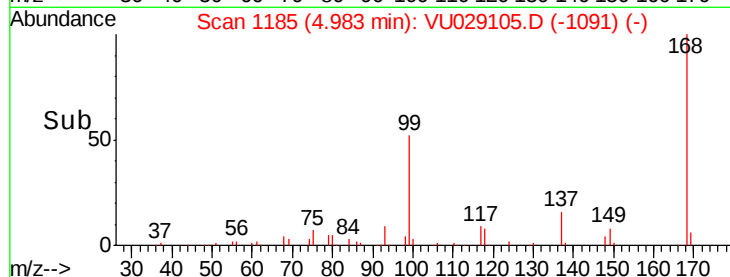

#33

1,2-Dichloroethane-d4

Concen: 55.578 ug/l

RT: 5.30 min Scan# 1285

Delta R.T. -0.00 min

Lab File: VU029105.D


Acq: 10 Jan 2019 09:49

Tgt Ion: 65 Resp: 71927

Ion Ratio Lower Upper

65 100

67 55.3 0.0 111.0

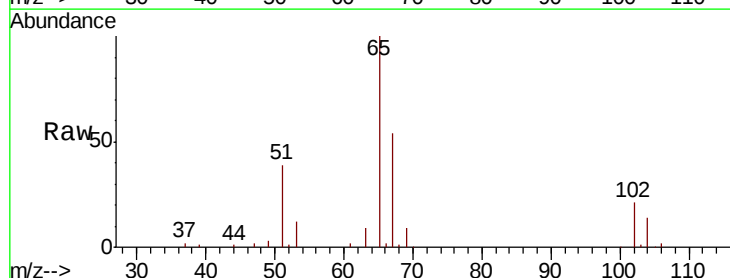

Abundance Ion 64.90 (64.60 to 65.60): VU028994.D (-1270) (-)

Ion 66.90 (66.60 to 67.60): VU029105.D (-1192) (-)

5.30

40000

30000

20000

10000


0


5.20

5.30

5.40

Time-->

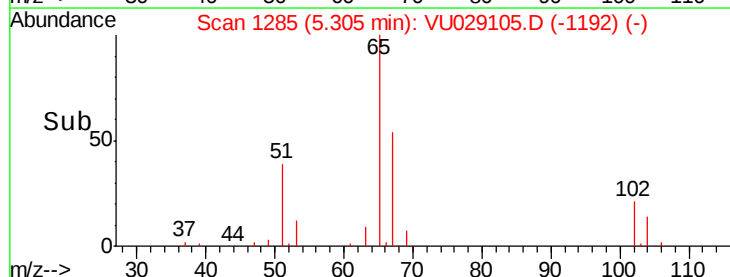


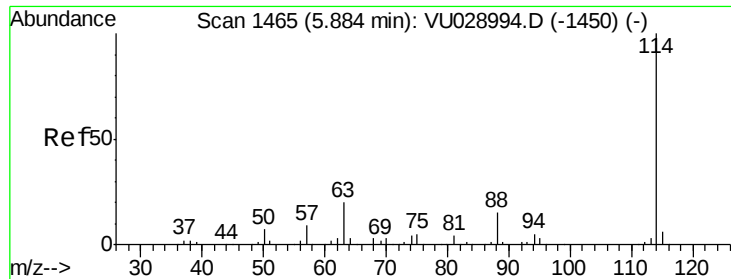




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.88 min Scan# 1465
 Delta R.T. -0.00 min
 Lab File: VU029105.D
 Acq: 10 Jan 2019 09:49

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0110WBL01

Tgt Ion:114 Resp: 179413
 Ion Ratio Lower Upper
 114 100
 63 21.7 0.0 40.2
 88 16.5 0.0 30.4

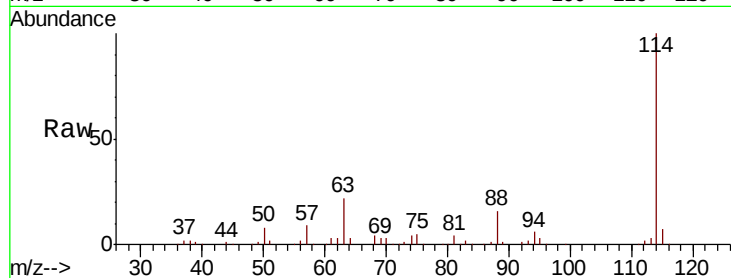


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VU0
 Ion 87.90 (87.60 to 88.60): VU0

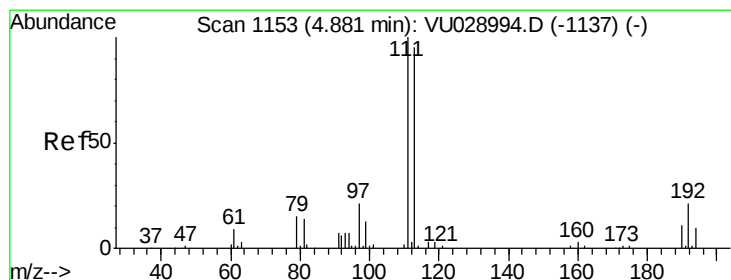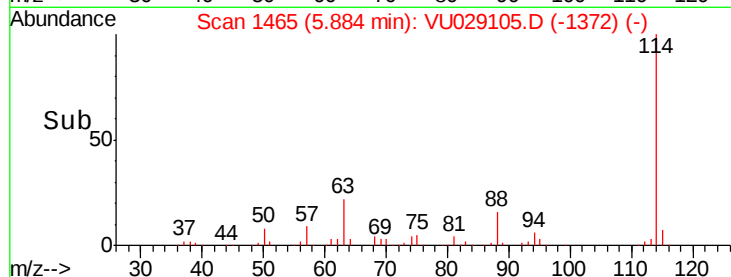
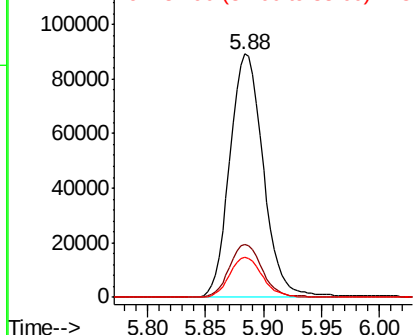



#35
 Dibromofluoromethane
 Concen: 55.067 ug/l
 RT: 4.88 min Scan# 1153
 Delta R.T. -0.00 min
 Lab File: VU029105.D
 Acq: 10 Jan 2019 09:49

Tgt Ion:113 Resp: 64043
 Ion Ratio Lower Upper
 113 100
 111 101.0 81.4 122.2
 192 20.6 16.8 25.2

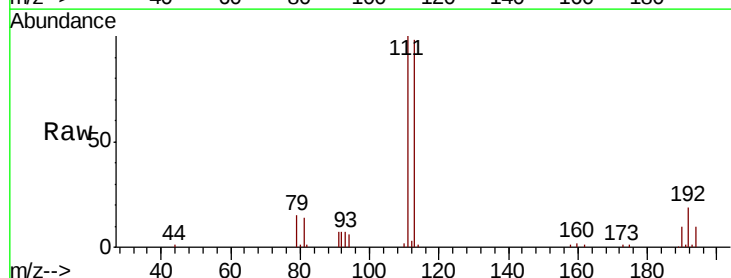

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

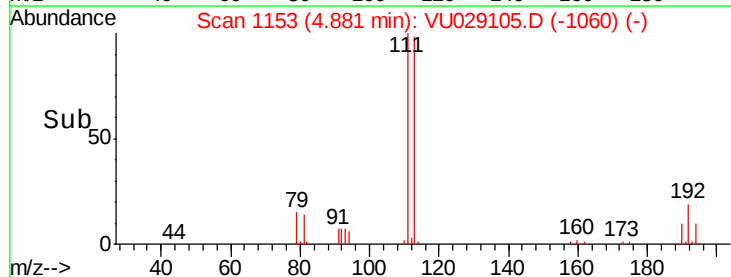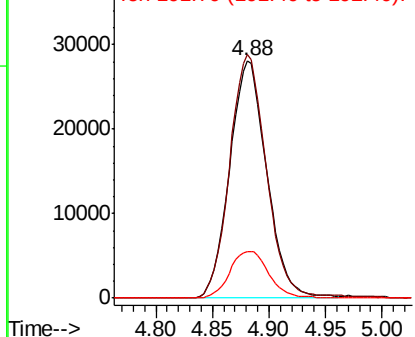

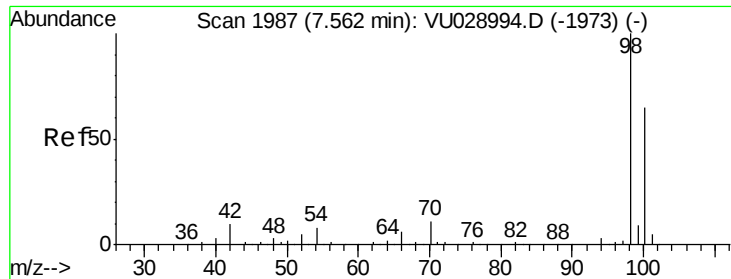

#50

Toluene-d8

Concen: 49.760 ug/l

RT: 7.56 min Scan# 1987

Delta R.T. -0.00 min

Lab File: VU029105.D

Acq: 10 Jan 2019 09:49

Instrument :

MSVOA_U

ClientSampleId :


VU0110WBL01

Tgt Ion: 98 Resp: 228468

Ion Ratio Lower Upper

98 100

100 63.6 51.6 77.4

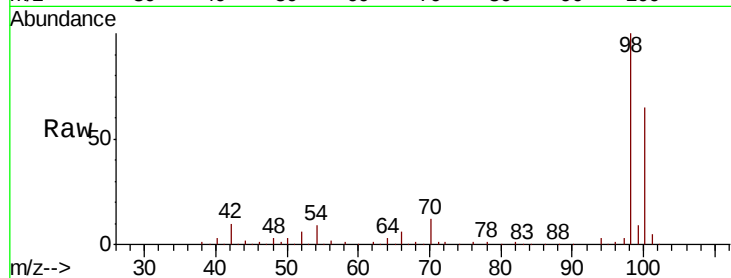

Abundance Ion 98.00 (97.70 to 98.70): VU028994.D (-1973) (-)

Ion 100.00 (99.70 to 100.70): VU028994.D (-1973) (-)

7.56



150000

100000

50000

0

Time-->

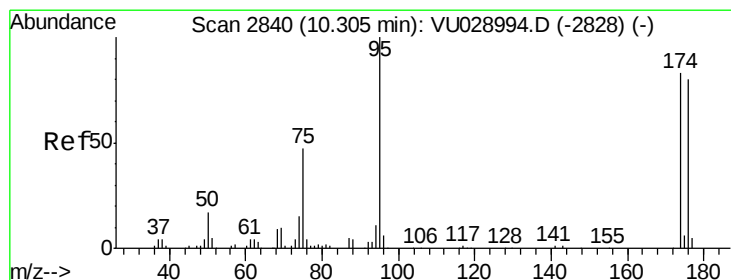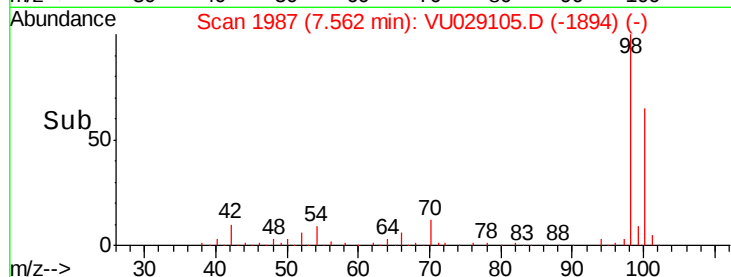

#62

4-Bromofluorobenzene

Concen: 39.950 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. -0.00 min

Lab File: VU029105.D

Acq: 10 Jan 2019 09:49


Tgt Ion: 95 Resp: 65920

Ion Ratio Lower Upper

95 100

174 86.8 0.0 170.6

176 82.1 0.0 165.0

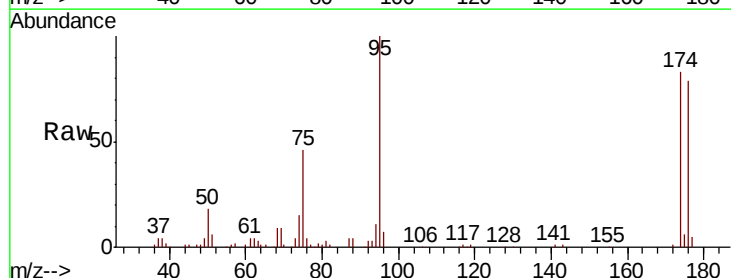

Abundance Ion 94.90 (94.60 to 95.60): VU028994.D (-2828) (-)

Ion 173.80 (173.50 to 174.50): VU028994.D (-2828) (-)

Ion 175.80 (175.50 to 176.50): VU028994.D (-2828) (-)

10.30

50000

40000


30000


20000

10000

0

Time-->

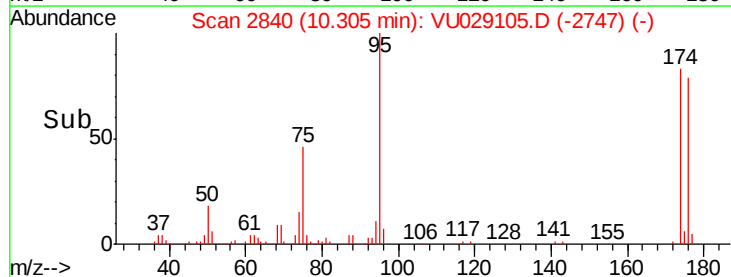


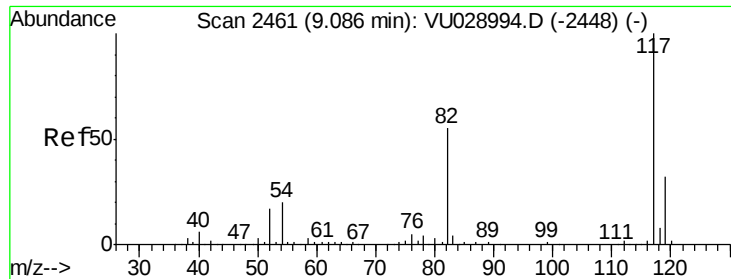




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2462
Delta R.T. 0.00 min
Lab File: VU029105.D
Acq: 10 Jan 2019 09:49

Instrument :
MSVOA_U
ClientSampleId :
VU0110WBL01

Tgt Ion:117 Resp: 159436
Ion Ratio Lower Upper
117 100
82 55.2 43.9 65.9
119 32.4 26.0 39.0

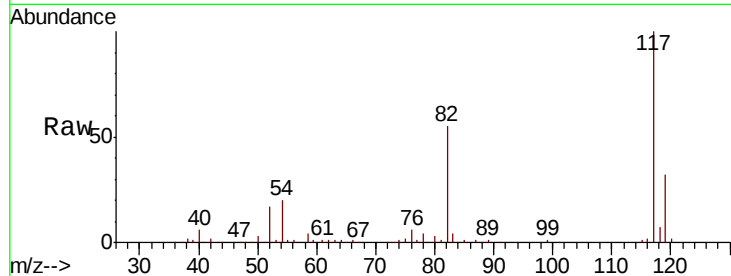


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VU0
Ion 118.90 (118.60 to 119.60): V

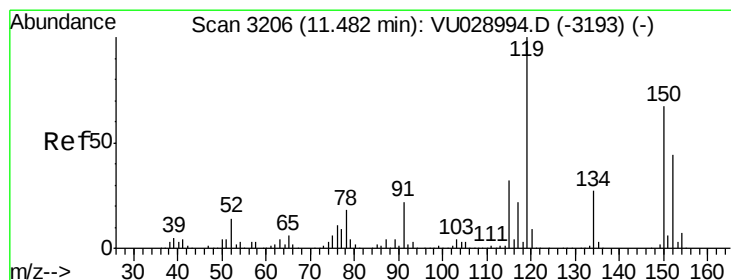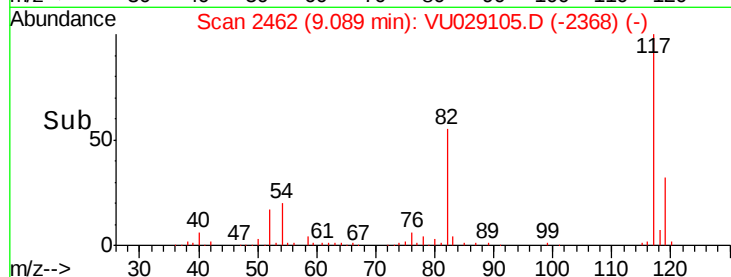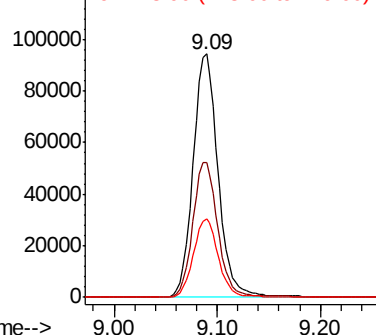

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.48 min Scan# 3207
Delta R.T. 0.00 min
Lab File: VU029105.D
Acq: 10 Jan 2019 09:49

Tgt Ion:152 Resp: 59204
Ion Ratio Lower Upper
152 100
115 55.8 40.1 120.3
150 155.9 0.0 345.2

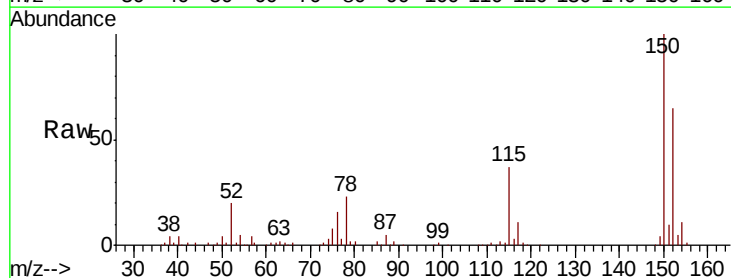

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

