


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU011020\
 Data File : VU036424.D
 Acq On : 10 Jan 2020 08:47
 Operator : JC/MD
 Sample : BFB37
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB37

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 10 22:57:35 2020

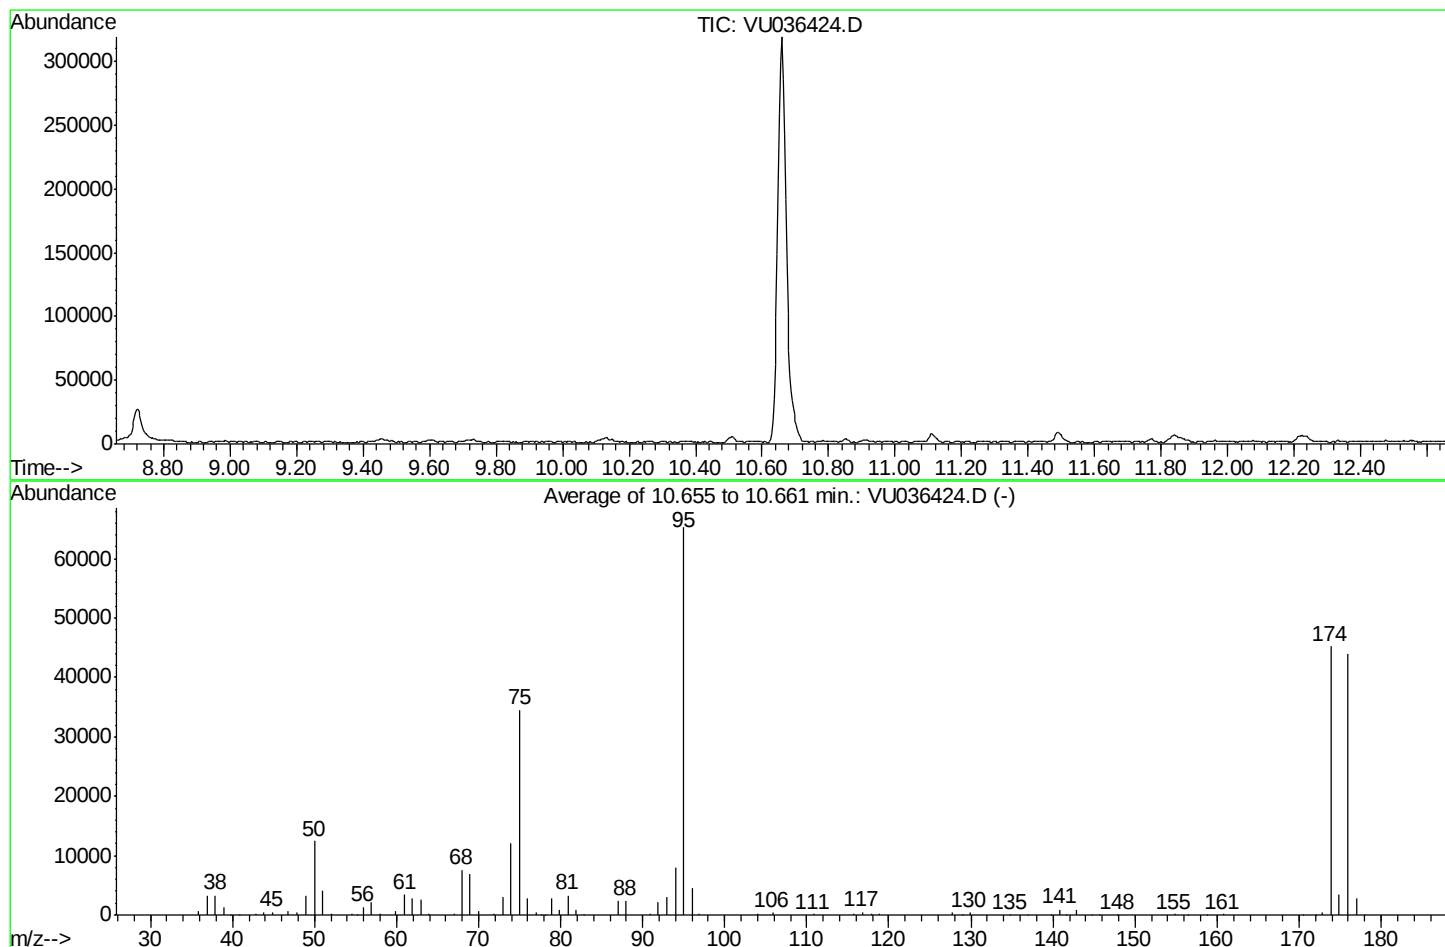

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	12465	PASS
75	95	30	80	52.9	34552	PASS
95	95	100	100	100.0	65277	PASS
96	95	5	9	6.9	4490	PASS
173	174	0.00	2	1.0	456	PASS
174	95	50	120	69.3	45245	PASS
175	174	5	9	7.7	3477	PASS
176	174	95	101	97.4	44066	PASS
177	176	5	9	6.1	2707	PASS

m/z	Abundance
35.90	609.0
36.90	3045.0
37.90	3363.0
39.00	1253.0
39.80	243.0
40.90	170.0
42.90	205.0
43.90	1163.0
44.90	472.0
46.80	533.0
47.80	397.0
48.90	3147.0
50.00	12119.0
50.90	3900.0
52.10	213.0
54.50	160.0
54.80	176.0
55.90	1311.0
57.00	2072.0
57.90	141.0
59.90	445.0
61.00	3261.0
62.00	2786.0
63.00	2473.0
67.00	175.0
68.00	7574.0
68.90	6872.0
70.00	719.0
71.90	305.0
72.90	3061.0
73.90	11747.0
75.00	33648.0
75.90	2840.0
77.00	366.0
78.10	297.0
78.90	2779.0
79.90	906.0
80.80	3047.0
81.80	836.0
86.90	2183.0
87.90	1908.0
90.90	312.0
91.80	2138.0
92.90	3073.0
94.00	7634.0
95.00	64024.0
96.00	4294.0
96.90	165.0
103.90	218.0
105.90	283.0
110.80	123.0
115.80	248.0
116.70	586.0
117.80	197.0
118.90	273.0
127.80	408.0
129.00	158.0
129.80	311.0
139.80	124.0
140.90	796.0
142.90	901.0
154.80	130.0
160.80	140.0
172.80	360.0
173.90	42904.0
174.90	3055.0
175.90	41368.0
176.90	2564.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
35.90	743.0
36.90	3344.0
37.90	3413.0
39.00	1314.0
39.80	240.0
40.90	108.0
42.90	210.0
44.00	1267.0
44.80	508.0
46.80	513.0
47.80	386.0
48.90	3312.0
50.00	12839.0
51.00	4191.0
52.10	158.0
54.60	201.0
56.00	1408.0
57.00	2212.0
58.00	202.0
59.90	577.0
61.00	3514.0
61.90	2975.0
63.00	2698.0
63.90	158.0
67.00	140.0
68.00	7820.0
68.90	6842.0
70.00	718.0
71.90	278.0
72.90	2939.0
73.90	12259.0
75.00	35336.0
75.90	2889.0
77.00	338.0
77.70	177.0
78.90	2902.0
79.80	753.0
80.90	3358.0
81.90	833.0
82.70	100.0
86.90	2431.0
87.90	2472.0
90.90	383.0
91.80	2192.0
93.00	3137.0
93.90	8185.0
95.00	67040.0
96.00	4559.0
96.90	184.0
104.00	305.0
105.90	423.0
110.80	124.0
115.70	287.0
116.70	496.0
117.90	226.0
118.90	342.0
127.80	380.0
129.00	135.0
129.90	368.0
137.00	102.0
140.90	879.0
142.90	820.0
147.90	121.0
154.80	158.0
158.70	106.0
160.80	194.0
172.10	136.0
172.80	480.0
173.90	46512.0
174.90	3602.0
175.90	45432.0
177.00	2691.0
178.00	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
35.90	793.0
36.90	3215.0
37.90	3099.0
38.90	1251.0
39.70	226.0
42.90	197.0
43.90	1265.0
44.80	599.0
46.70	624.0
47.90	439.0
48.90	3008.0
50.00	12439.0
51.00	3961.0
54.60	178.0
55.20	156.0
56.00	1363.0
56.90	2416.0
58.00	162.0
59.90	786.0
61.00	3390.0
61.90	2935.0
62.90	2558.0
63.90	239.0
67.00	131.0
67.90	7397.0
69.00	6759.0
70.00	592.0
71.90	312.0
72.90	2845.0
73.90	12103.0
75.00	34672.0
75.90	2725.0
77.00	356.0
77.70	144.0
78.90	2826.0
79.80	687.0
80.90	3415.0
81.90	709.0
82.80	137.0
87.00	2551.0
87.90	2837.0
90.90	403.0
91.80	1989.0
93.00	3014.0
93.90	7978.0
95.00	64768.0
96.00	4619.0
96.90	145.0
104.00	347.0
105.80	458.0
110.80	103.0
115.70	352.0
116.80	428.0
117.80	212.0
118.90	362.0
127.80	256.0
130.00	375.0
134.80	107.0
137.00	109.0
140.90	933.0
141.60	114.0
142.90	727.0
144.80	131.0
145.70	106.0
147.90	159.0
154.90	180.0
156.50	116.0
158.80	104.0
160.80	188.0
170.50	110.0
172.00	174.0
172.80	530.0
173.90	46320.0
174.90	3774.0
175.90	45400.0
177.00	2867.0
177.90	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

Scan 2884 (10.613 min): VU036424.D
BFB37

m/z	Abundance
39.80	210.0
41.20	212.0
41.90	103.0
43.80	725.0
55.00	126.0
91.00	160.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37