

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
 Data File : VU046711.D
 Acq On : 10 Jan 2022 11:55
 Operator : SY/MD
 Sample : VU0110MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

Signal : TIC: VU046711.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	102	rVB	70679	82675	12.61%	1.529%
2	1.919	171	180	199	rBV	57469	78423	11.96%	1.451%
3	2.285	291	294	299	rBV2	165	168	0.03%	0.003%
4	2.375	319	322	328	rBV	215	288	0.04%	0.005%
5	2.414	330	334	337	rBV	150	145	0.02%	0.003%
6	2.575	371	384	397	rBV	129655	212655	32.42%	3.934%
7	2.774	442	446	448	rBV	211	181	0.03%	0.003%
8	2.800	448	454	463	rVV	607	981	0.15%	0.018%
9	2.893	480	483	486	rBV	151	143	0.02%	0.003%
10	2.957	501	503	507	rBV	114	127	0.02%	0.002%
11	3.051	528	532	535	rBB2	373	298	0.05%	0.006%
12	4.227	894	898	901	rBV	145	164	0.03%	0.003%
13	4.652	1013	1030	1088	rVV	46277	192020	29.28%	3.552%
14	4.938	1114	1119	1122	rBV	181	186	0.03%	0.003%
15	5.009	1138	1141	1144	rBV	211	147	0.02%	0.003%
16	5.067	1144	1159	1186	rVV	121901	268876	41.00%	4.974%
17	5.182	1193	1195	1198	rVB	274	158	0.02%	0.003%
18	5.231	1205	1210	1213	rBB	135	161	0.02%	0.003%
19	5.729	1344	1365	1385	rBV2	241243	655839	100.00%	12.133%
20	6.253	1513	1528	1557	rBV	216094	412304	62.87%	7.628%
21	6.401	1569	1574	1577	rBV2	272	317	0.05%	0.006%
22	6.533	1607	1615	1622	rBB4	697	930	0.14%	0.017%
23	6.694	1651	1665	1687	rBV	153765	296407	45.20%	5.483%
24	6.829	1704	1707	1711	rBV	139	168	0.03%	0.003%
25	7.002	1758	1761	1764	rBB	149	124	0.02%	0.002%
26	7.067	1779	1781	1785	rBB	159	128	0.02%	0.002%
27	7.189	1812	1819	1825	rBB	525	587	0.09%	0.011%
28	7.436	1893	1896	1899	rBB	144	128	0.02%	0.002%
29	7.568	1925	1937	1952	rBV	84830	148712	22.68%	2.751%
30	7.671	1967	1969	1971	rBV	270	156	0.02%	0.003%
31	7.694	1971	1976	1982	rVB3	525	673	0.10%	0.012%
32	7.774	1999	2001	2005	rBV	153	143	0.02%	0.003%
33	7.806	2006	2011	2014	rVB	293	229	0.03%	0.004%
34	7.899	2027	2040	2058	rBV	297261	514796	78.49%	9.524%
35	7.970	2058	2062	2072	rVB2	3885	6003	0.92%	0.111%
36	8.028	2077	2080	2083	rVV	341	274	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
 Data File : VU046711.D
 Acq On : 10 Jan 2022 11:55
 Operator : SY/MD
 Sample : VU0110MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

37	8.044	2083	2085	2091	rVB2	269	250	0.04%	0.005%
38	8.105	2101	2104	2106	rBV	152	123	0.02%	0.002%
39	8.182	2117	2128	2152	rVV	60110	101674	15.50%	1.881%
40	8.298	2161	2164	2167	rBV	155	151	0.02%	0.003%
41	8.478	2214	2220	2226	rBB	378	450	0.07%	0.008%
42	8.639	2257	2270	2313	rBV	240393	431380	65.78%	7.980%
43	8.790	2313	2317	2321	rVB2	175	182	0.03%	0.003%
44	8.864	2337	2340	2344	rBB	156	157	0.02%	0.003%
45	8.909	2351	2354	2358	rBB	141	122	0.02%	0.002%
46	8.931	2359	2361	2365	rBB	137	120	0.02%	0.002%
47	8.976	2370	2375	2378	rBB	169	152	0.02%	0.003%
48	8.999	2379	2382	2384	rBB	159	110	0.02%	0.002%
49	9.150	2426	2429	2432	rBV	172	163	0.02%	0.003%
50	9.202	2442	2445	2448	rBB	168	144	0.02%	0.003%
51	9.256	2457	2462	2464	rBB	153	152	0.02%	0.003%
52	9.340	2485	2488	2492	rBB	142	115	0.02%	0.002%
53	9.420	2500	2513	2531	rBV	311596	512056	78.08%	9.473%
54	9.571	2556	2560	2567	rBV2	623	761	0.12%	0.014%
55	9.697	2592	2599	2606	rBV2	607	953	0.15%	0.018%
56	9.819	2633	2637	2639	rBB	135	113	0.02%	0.002%
57	9.893	2656	2660	2665	rBB	149	207	0.03%	0.004%
58	10.076	2714	2717	2719	rBV	161	128	0.02%	0.002%
59	10.111	2720	2728	2734	rVV4	543	868	0.13%	0.016%
60	10.208	2756	2758	2762	rBB	145	121	0.02%	0.002%
61	10.247	2765	2770	2773	rBV	179	220	0.03%	0.004%
62	10.372	2806	2809	2812	rBV	155	152	0.02%	0.003%
63	10.494	2836	2847	2854	rVB2	349	603	0.09%	0.011%
64	10.616	2881	2885	2890	rBB	165	187	0.03%	0.003%
65	10.645	2891	2894	2897	rBV	149	156	0.02%	0.003%
66	10.674	2897	2903	2909	rVV2	753	898	0.14%	0.017%
67	10.758	2917	2929	2946	rBV	249419	401554	61.23%	7.429%
68	10.890	2967	2970	2972	rBV	232	114	0.02%	0.002%
69	11.092	3028	3033	3039	rBV2	692	671	0.10%	0.012%
70	11.291	3091	3095	3098	rBV	132	163	0.02%	0.003%
71	11.369	3116	3119	3121	rBV	151	127	0.02%	0.002%
72	11.423	3131	3136	3139	rBV	175	208	0.03%	0.004%
73	11.462	3142	3148	3149	rBV3	835	707	0.11%	0.013%
74	11.623	3195	3198	3200	rBV	172	151	0.02%	0.003%
75	11.655	3205	3208	3210	rBV	169	143	0.02%	0.003%
76	11.687	3216	3218	3221	rBV	134	117	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
 Data File : VU046711.D
 Acq On : 10 Jan 2022 11:55
 Operator : SY/MD
 Sample : VU0110MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

77	11.751	3231	3238	3245	rBV3	1026	1327	0.20%	0.025%
78	11.812	3245	3257	3278	rVV	325666	515166	78.55%	9.530%
79	11.890	3278	3281	3283	rVV	209	158	0.02%	0.003%
80	11.906	3284	3286	3290	rVV	189	171	0.03%	0.003%
81	11.947	3294	3299	3301	rVV	327	322	0.05%	0.006%
82	11.973	3304	3307	3312	rVB3	484	434	0.07%	0.008%
83	12.195	3363	3376	3394	rBV	331169	534713	81.53%	9.892%
84	12.652	3510	3518	3521	rBV	82	133	0.02%	0.002%
85	13.037	3631	3638	3644	rBV	131	164	0.03%	0.003%
86	13.224	3689	3696	3704	rBV2	1758	2227	0.34%	0.041%
87	13.725	3848	3852	3855	rBV	123	111	0.02%	0.002%
88	13.844	3881	3889	3897	rBV4	2727	3725	0.57%	0.069%
89	14.089	3955	3965	3979	rBV2	4346	6989	1.07%	0.129%
90	14.330	4032	4040	4050	rVB3	3099	4484	0.68%	0.083%
91	15.311	4341	4345	4349	rBV	247	249	0.04%	0.005%
92	15.362	4357	4361	4364	rBV	202	184	0.03%	0.003%
93	15.545	4414	4418	4422	rVB2	257	209	0.03%	0.004%
94	15.581	4426	4429	4432	rBV	268	227	0.03%	0.004%
95	15.790	4487	4494	4496	rBV	255	312	0.05%	0.006%
96	16.565	4732	4735	4740	rBV2	342	387	0.06%	0.007%
97	16.661	4763	4765	4766	rBV	250	110	0.02%	0.002%
98	16.796	4803	4807	4811	rBV3	485	447	0.07%	0.008%
99	16.857	4824	4826	4830	rVB	557	261	0.04%	0.005%
100	17.237	4942	4944	4948	rBV2	586	437	0.07%	0.008%




Sum of corrected areas: 5405484

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
Data File : VU046711.D
Acq On : 10 Jan 2022 11:55
Operator : SY/MD
Sample : VU0110MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK058

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

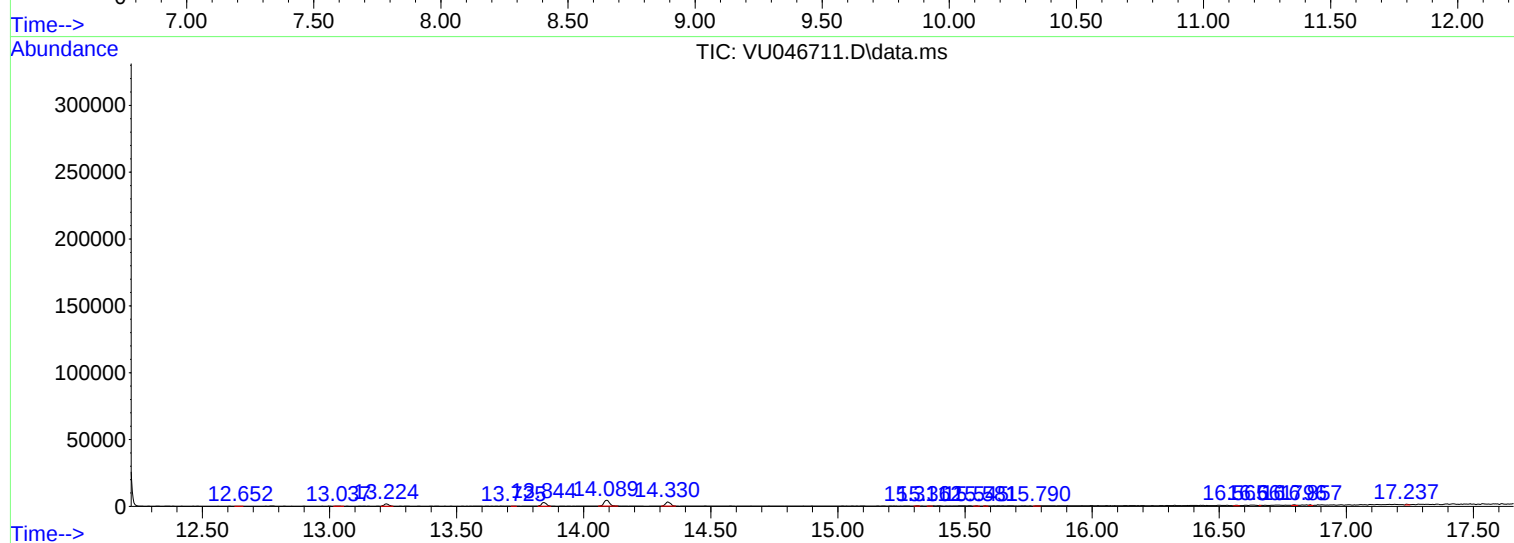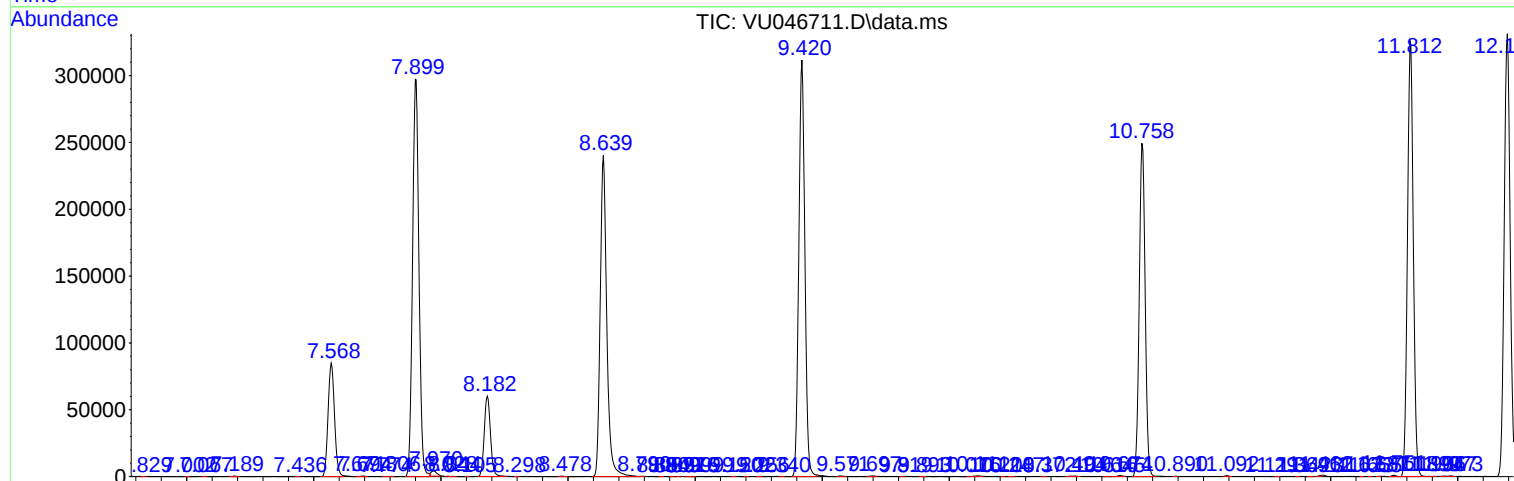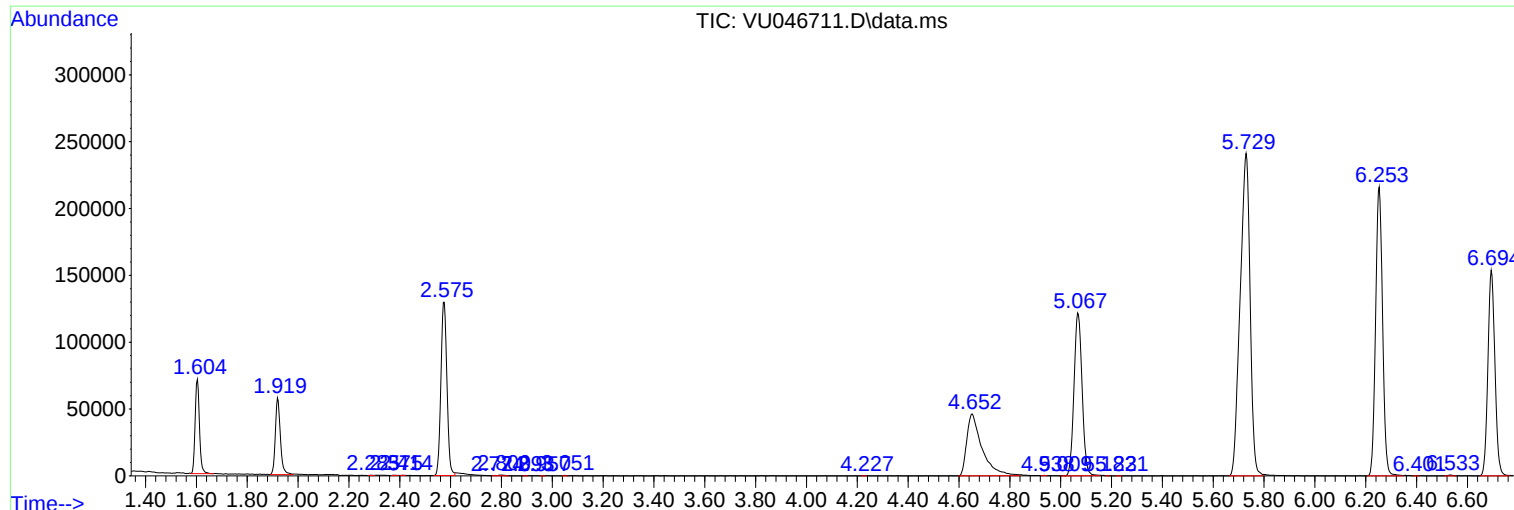

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
Data File : VU046711.D
Acq On : 10 Jan 2022 11:55
Operator : SY/MD
Sample : VU0110MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK058

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
Data File : VU046711.D
Acq On : 10 Jan 2022 11:55
Operator : SY/MD
Sample : VU0110MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK058

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc