

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
 Data File : VU046712.D
 Acq On : 10 Jan 2022 12:30
 Operator : SY/MD
 Sample : VU0110WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK059

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M

Title : VOC Analysis

Signal : TIC: VU046712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	98	rBV	89536	104582	15.18%	1.925%
2	1.919	171	180	198	rBV	65800	90161	13.09%	1.659%
3	2.208	265	270	273	rVV	228	209	0.03%	0.004%
4	2.308	296	301	304	rBV2	279	256	0.04%	0.005%
5	2.572	372	383	418	rBV	151100	253604	36.82%	4.667%
6	2.800	448	454	461	rVB2	421	614	0.09%	0.011%
7	2.954	499	502	506	rBB	169	166	0.02%	0.003%
8	2.977	506	509	513	rBB	188	170	0.02%	0.003%
9	3.051	530	532	538	rVB2	512	413	0.06%	0.008%
10	3.173	567	570	574	rBB	142	142	0.02%	0.003%
11	3.273	598	601	604	rBB	143	119	0.02%	0.002%
12	3.324	615	617	620	rBB	168	105	0.02%	0.002%
13	3.568	691	693	696	rBB	166	112	0.02%	0.002%
14	3.967	814	817	821	rBB	140	139	0.02%	0.003%
15	4.221	894	896	900	rBV	121	131	0.02%	0.002%
16	4.652	1012	1030	1072	rBV	38922	166196	24.13%	3.059%
17	4.964	1126	1127	1130	rBV	215	127	0.02%	0.002%
18	4.977	1130	1131	1135	rVB	225	136	0.02%	0.003%
19	5.067	1143	1159	1181	rBV	123619	270781	39.32%	4.983%
20	5.179	1191	1194	1197	rVB	247	143	0.02%	0.003%
21	5.385	1255	1258	1261	rBB	137	114	0.02%	0.002%
22	5.729	1344	1365	1394	rBV2	260346	688744	100.00%	12.675%
23	6.253	1512	1528	1553	rBV	221344	415098	60.27%	7.639%
24	6.340	1553	1555	1559	rVV	400	296	0.04%	0.005%
25	6.356	1559	1560	1565	rVV2	277	243	0.04%	0.004%
26	6.388	1565	1570	1574	rVB2	177	185	0.03%	0.003%
27	6.530	1609	1614	1618	rBV3	484	460	0.07%	0.008%
28	6.694	1651	1665	1688	rBV	155026	298291	43.31%	5.490%
29	6.806	1697	1700	1702	rBB	272	193	0.03%	0.004%
30	6.922	1733	1736	1738	rBB	223	107	0.02%	0.002%
31	6.983	1751	1755	1757	rBB	141	119	0.02%	0.002%
32	7.018	1763	1766	1768	rBV	129	114	0.02%	0.002%
33	7.057	1774	1778	1782	rBV2	274	295	0.04%	0.005%
34	7.179	1813	1816	1817	rBV2	327	194	0.03%	0.004%
35	7.189	1817	1819	1824	rVV2	475	478	0.07%	0.009%
36	7.311	1853	1857	1860	rBB	141	121	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
 Data File : VU046712.D
 Acq On : 10 Jan 2022 12:30
 Operator : SY/MD
 Sample : VU0110WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK059

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

37	7.568	1925	1937	1952	rBV	84396	148713	21.59%	2.737%
38	7.687	1971	1974	1977	rBV3	417	299	0.04%	0.006%
39	7.790	2003	2006	2010	rBB	156	125	0.02%	0.002%
40	7.903	2025	2041	2055	rBV	316160	555169	80.61%	10.217%
41	8.047	2083	2086	2090	rVB3	252	162	0.02%	0.003%
42	8.128	2108	2111	2114	rBV	143	145	0.02%	0.003%
43	8.182	2114	2128	2144	rVV	62146	103540	15.03%	1.906%
44	8.266	2151	2154	2157	rBV	268	235	0.03%	0.004%
45	8.366	2179	2185	2187	rBV	125	158	0.02%	0.003%
46	8.465	2212	2216	2217	rBV	251	168	0.02%	0.003%
47	8.478	2217	2220	2226	rVB2	274	298	0.04%	0.005%
48	8.565	2245	2247	2251	rBB	154	124	0.02%	0.002%
49	8.587	2251	2254	2258	rBV	129	161	0.02%	0.003%
50	8.639	2258	2270	2297	rBV	208918	381447	55.38%	7.020%
51	8.903	2347	2352	2357	rBB	162	218	0.03%	0.004%
52	8.938	2360	2363	2367	rBV	172	188	0.03%	0.003%
53	9.186	2437	2440	2444	rBB	142	139	0.02%	0.003%
54	9.237	2453	2456	2458	rBB	159	105	0.02%	0.002%
55	9.269	2463	2466	2471	rBV	132	187	0.03%	0.003%
56	9.420	2500	2513	2531	rBV	308171	512307	74.38%	9.428%
57	9.539	2547	2550	2552	rBV	123	109	0.02%	0.002%
58	9.571	2556	2560	2567	rBB2	418	552	0.08%	0.010%
59	9.700	2596	2600	2604	rVB	421	402	0.06%	0.007%
60	9.748	2612	2615	2617	rBV	121	108	0.02%	0.002%
61	9.803	2630	2632	2635	rBV	158	134	0.02%	0.002%
62	9.883	2653	2657	2661	rBV	151	187	0.03%	0.003%
63	9.925	2667	2670	2672	rBV	145	130	0.02%	0.002%
64	10.292	2780	2784	2786	rBB	149	127	0.02%	0.002%
65	10.308	2786	2789	2791	rBV	128	111	0.02%	0.002%
66	10.385	2808	2813	2815	rBV	171	200	0.03%	0.004%
67	10.452	2828	2834	2838	rBB	142	192	0.03%	0.004%
68	10.533	2857	2859	2862	rBV	117	106	0.02%	0.002%
69	10.671	2896	2902	2911	rBV3	1577	2134	0.31%	0.039%
70	10.758	2916	2929	2948	rBV	234564	372151	54.03%	6.849%
71	10.864	2959	2962	2965	rBV2	159	130	0.02%	0.002%
72	11.092	3029	3033	3037	rBB2	203	214	0.03%	0.004%
73	11.131	3041	3045	3051	rVB2	284	323	0.05%	0.006%
74	11.166	3051	3056	3060	rBV	156	241	0.03%	0.004%
75	11.324	3100	3105	3109	rBV	169	252	0.04%	0.005%
76	11.459	3139	3147	3158	rBV4	1066	1703	0.25%	0.031%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
 Data File : VU046712.D
 Acq On : 10 Jan 2022 12:30
 Operator : SY/MD
 Sample : VU0110WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK059

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

77	11.687	3215	3218	3220	rBV2	274	184	0.03%	0.003%
78	11.745	3232	3236	3242	rBV2	350	382	0.06%	0.007%
79	11.812	3245	3257	3284	rBV	330030	515384	74.83%	9.485%
80	11.941	3290	3297	3299	rBV2	466	481	0.07%	0.009%
81	12.195	3364	3376	3396	rVB	326886	532820	77.36%	9.806%
82	12.330	3416	3418	3421	rVB	274	132	0.02%	0.002%
83	12.365	3422	3429	3435	rBV	239	308	0.04%	0.006%
84	12.642	3512	3515	3517	rVB	166	113	0.02%	0.002%
85	12.738	3540	3545	3550	rBV	127	146	0.02%	0.003%
86	13.185	3680	3684	3687	rBV	135	121	0.02%	0.002%
87	13.230	3691	3698	3704	rVV2	533	727	0.11%	0.013%
88	13.844	3884	3889	3895	rVB3	726	875	0.13%	0.016%
89	14.092	3958	3966	3976	rVB2	1061	1834	0.27%	0.034%
90	14.330	4035	4040	4048	rBV2	1033	1206	0.18%	0.022%
91	14.578	4113	4117	4119	rBV	206	146	0.02%	0.003%
92	14.587	4119	4120	4131	rVB	217	158	0.02%	0.003%
93	15.227	4316	4319	4322	rBV2	172	142	0.02%	0.003%
94	15.459	4388	4391	4396	rVB2	301	282	0.04%	0.005%
95	15.484	4396	4399	4403	rBV	213	228	0.03%	0.004%
96	15.603	4434	4436	4439	rBV	230	152	0.02%	0.003%
97	15.970	4547	4550	4553	rBV	222	154	0.02%	0.003%
98	16.381	4675	4678	4682	rBV	247	227	0.03%	0.004%
99	16.568	4734	4736	4739	rBV	278	212	0.03%	0.004%
100	17.359	4979	4982	4986	rBV4	562	518	0.08%	0.010%




Sum of corrected areas: 5433684

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
Data File : VU046712.D
Acq On : 10 Jan 2022 12:30
Operator : SY/MD
Sample : VU0110WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK059

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

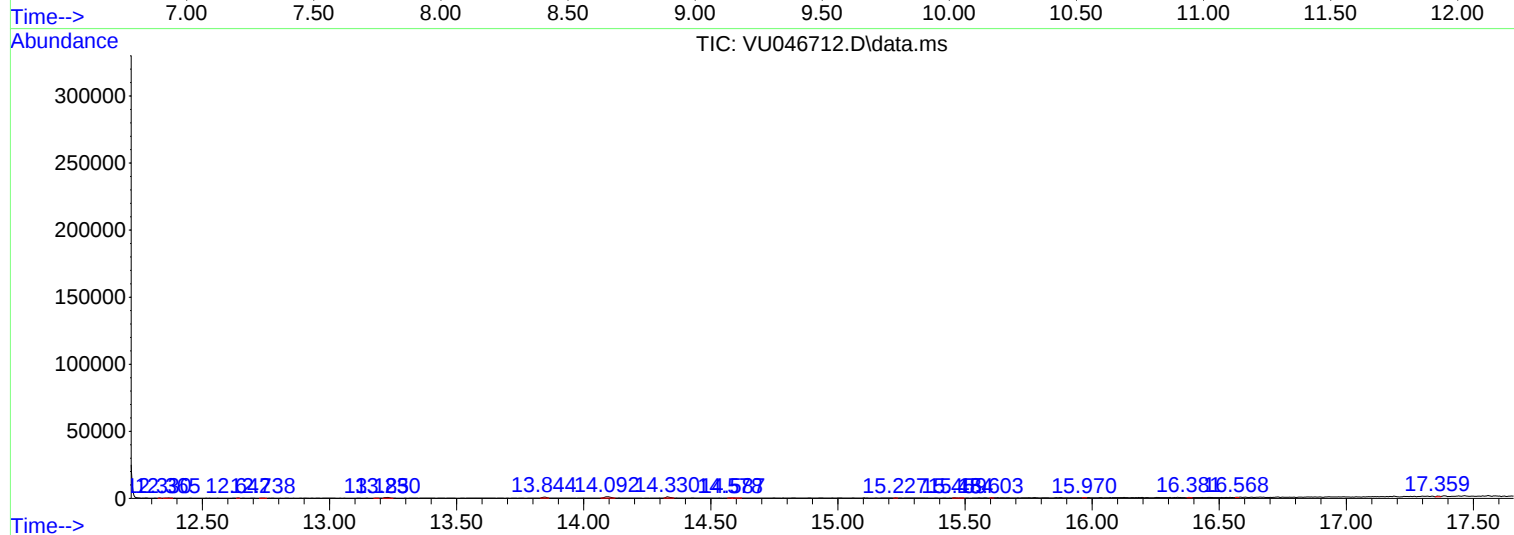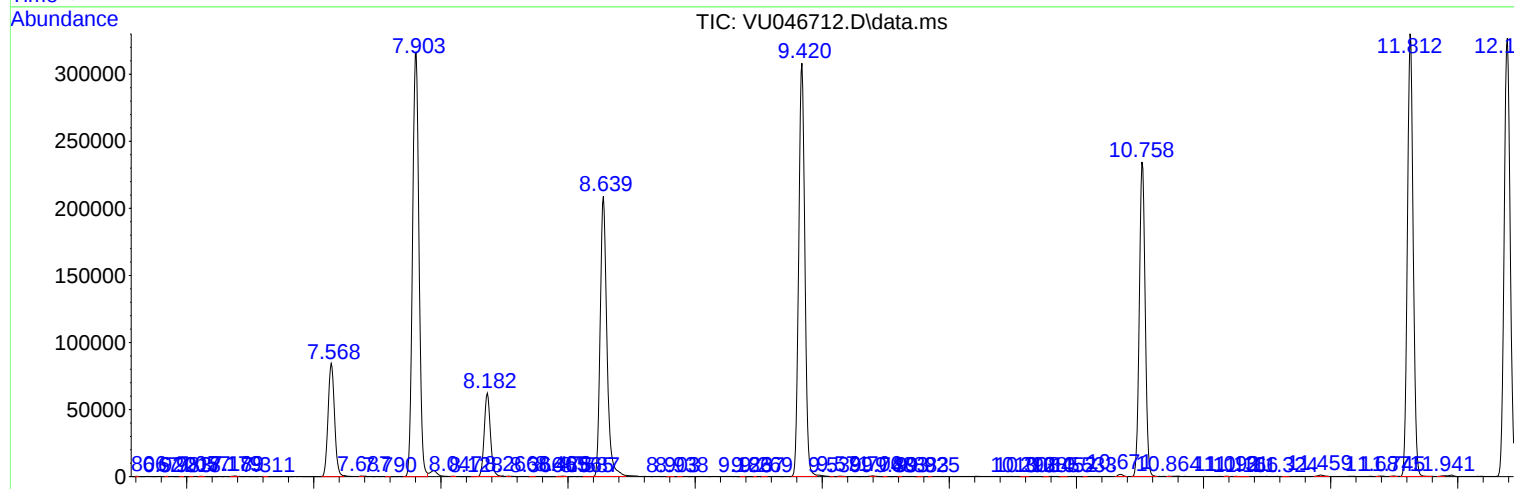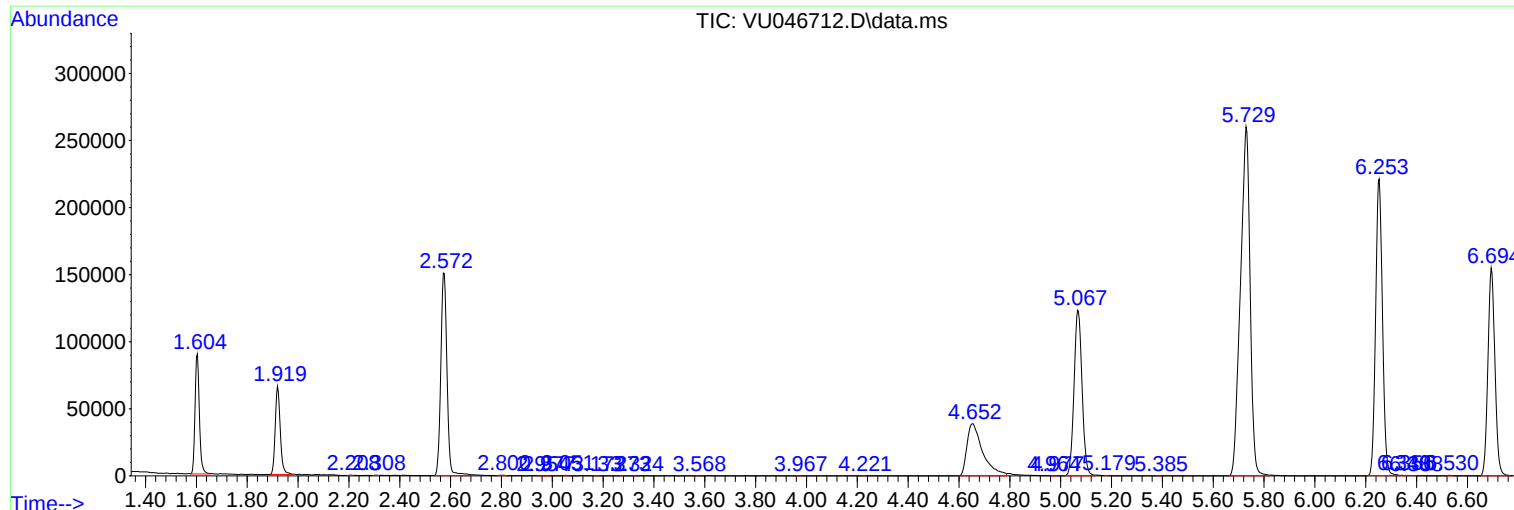

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
Data File : VU046712.D
Acq On : 10 Jan 2022 12:30
Operator : SY/MD
Sample : VU0110WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK059

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
Data File : VU046712.D
Acq On : 10 Jan 2022 12:30
Operator : SY/MD
Sample : VU0110WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK059

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc