

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
 Data File : VU046713.D
 Acq On : 10 Jan 2022 13:00
 Operator : SY/MD
 Sample : N1084-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGLL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

Signal : TIC: VU046713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	98	rBV	71783	84487	12.59%	1.598%
2	1.919	171	180	202	rBV	59740	81938	12.21%	1.550%
3	2.571	371	383	403	rBV	128853	215651	32.13%	4.078%
4	2.784	447	449	450	rBV	251	110	0.02%	0.002%
5	2.915	487	490	492	rBV	270	233	0.03%	0.004%
6	2.973	500	508	512	rBV2	528	627	0.09%	0.012%
7	3.047	529	531	533	rVB	238	102	0.02%	0.002%
8	3.118	550	553	558	rVB2	208	184	0.03%	0.003%
9	3.192	563	576	590	rVB2	2147	5099	0.76%	0.096%
10	3.764	751	754	757	rBV	129	137	0.02%	0.003%
11	3.960	813	815	818	rBV	151	127	0.02%	0.002%
12	4.395	947	950	953	rBB	127	111	0.02%	0.002%
13	4.649	1012	1029	1067	rBV2	49721	197097	29.36%	3.727%
14	5.067	1143	1159	1185	rBV	126162	276862	41.24%	5.236%
15	5.179	1191	1194	1198	rVB2	396	326	0.05%	0.006%
16	5.202	1198	1201	1206	rBB2	270	273	0.04%	0.005%
17	5.285	1222	1227	1229	rBV2	225	189	0.03%	0.004%
18	5.488	1287	1290	1293	rBB	141	125	0.02%	0.002%
19	5.729	1343	1365	1386	rBV2	247665	671276	100.00%	12.694%
20	5.890	1412	1415	1419	rVB2	155	100	0.01%	0.002%
21	5.931	1427	1428	1432	rBB	212	121	0.02%	0.002%
22	6.038	1456	1461	1463	rBB	228	159	0.02%	0.003%
23	6.253	1514	1528	1546	rBV	181701	342944	51.09%	6.485%
24	6.343	1553	1556	1558	rBV	202	126	0.02%	0.002%
25	6.391	1568	1571	1574	rVB2	155	99	0.01%	0.002%
26	6.529	1612	1614	1616	rVB	261	119	0.02%	0.002%
27	6.693	1651	1665	1686	rBV	156321	304318	45.33%	5.755%
28	6.819	1699	1704	1705	rBB	233	154	0.02%	0.003%
29	6.867	1716	1719	1722	rBV	150	146	0.02%	0.003%
30	7.041	1770	1773	1776	rBV	310	258	0.04%	0.005%
31	7.057	1776	1778	1779	rVV	235	115	0.02%	0.002%
32	7.063	1779	1780	1783	rVB2	247	112	0.02%	0.002%
33	7.111	1791	1795	1798	rBB	141	120	0.02%	0.002%
34	7.131	1799	1801	1804	rBB	146	101	0.02%	0.002%
35	7.189	1810	1819	1827	rVB2	597	1058	0.16%	0.020%
36	7.359	1870	1872	1875	rBB	146	101	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
 Data File : VU046713.D
 Acq On : 10 Jan 2022 13:00
 Operator : SY/MD
 Sample : N1084-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGLL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

37	7.465	1902	1905	1908	rBB	154	123	0.02%	0.002%
38	7.568	1924	1937	1959	rBV	86342	150115	22.36%	2.839%
39	7.642	1959	1960	1963	rVB	287	129	0.02%	0.002%
40	7.661	1964	1966	1969	rBB	223	107	0.02%	0.002%
41	7.690	1969	1975	1979	rBV2	668	755	0.11%	0.014%
42	7.793	2005	2007	2009	rBB	239	107	0.02%	0.002%
43	7.899	2027	2040	2057	rBV	301969	527516	78.58%	9.976%
44	7.970	2058	2062	2075	rVB	4860	7371	1.10%	0.139%
45	8.121	2107	2109	2113	rBB	131	111	0.02%	0.002%
46	8.182	2117	2128	2149	rBV	60827	102352	15.25%	1.936%
47	8.256	2149	2151	2156	rVV2	371	364	0.05%	0.007%
48	8.285	2158	2160	2162	rVB	236	112	0.02%	0.002%
49	8.475	2205	2219	2232	rBB2	15886	28551	4.25%	0.540%
50	8.542	2238	2240	2243	rBV	142	119	0.02%	0.002%
51	8.639	2256	2270	2303	rBV	234863	428626	63.85%	8.106%
52	8.793	2311	2318	2324	rVB4	1112	1743	0.26%	0.033%
53	8.828	2327	2329	2332	rVB	258	127	0.02%	0.002%
54	8.854	2333	2337	2340	rBB	148	146	0.02%	0.003%
55	8.873	2340	2343	2345	rBV	173	152	0.02%	0.003%
56	8.925	2357	2359	2363	rBV	142	143	0.02%	0.003%
57	8.989	2374	2379	2382	rBB	175	199	0.03%	0.004%
58	9.018	2385	2388	2390	rBB	178	123	0.02%	0.002%
59	9.147	2426	2428	2431	rBV	154	125	0.02%	0.002%
60	9.182	2436	2439	2441	rBV	118	107	0.02%	0.002%
61	9.253	2456	2461	2463	rBV	163	197	0.03%	0.004%
62	9.420	2499	2513	2537	rBV	262215	433714	64.61%	8.202%
63	9.571	2556	2560	2566	rVB2	236	262	0.04%	0.005%
64	9.635	2578	2580	2583	rBB	143	99	0.01%	0.002%
65	9.697	2592	2599	2604	rBV3	502	658	0.10%	0.012%
66	9.854	2643	2648	2653	rBB	161	224	0.03%	0.004%
67	9.902	2661	2663	2666	rVB	149	103	0.02%	0.002%
68	10.018	2696	2699	2701	rBV	146	120	0.02%	0.002%
69	10.070	2712	2715	2718	rBV	179	173	0.03%	0.003%
70	10.105	2723	2726	2730	rVB2	191	163	0.02%	0.003%
71	10.160	2739	2743	2746	rBV	205	220	0.03%	0.004%
72	10.301	2784	2787	2790	rBV	162	155	0.02%	0.003%
73	10.671	2895	2902	2909	rBV3	887	1007	0.15%	0.019%
74	10.758	2917	2929	2947	rBV	251424	405303	60.38%	7.665%
75	10.896	2960	2972	2984	rVV	15886	25062	3.73%	0.474%
76	11.089	3029	3032	3035	rBV	207	119	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
 Data File : VU046713.D
 Acq On : 10 Jan 2022 13:00
 Operator : SY/MD
 Sample : N1084-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGLL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

77	11.468	3141	3150	3161	rBV4	700	1223	0.18%	0.023%
78	11.690	3216	3219	3223	rBV	214	193	0.03%	0.004%
79	11.751	3235	3238	3240	rBV	185	136	0.02%	0.003%
80	11.812	3245	3257	3276	rVB	272132	428448	63.83%	8.102%
81	11.973	3303	3307	3315	rVB	465	512	0.08%	0.010%
82	12.063	3327	3335	3349	rVB5	2627	4168	0.62%	0.079%
83	12.195	3363	3376	3393	rBV	334165	537522	80.07%	10.165%
84	12.690	3526	3530	3534	rBV	109	111	0.02%	0.002%
85	12.774	3546	3556	3564	rBV2	3896	5431	0.81%	0.103%
86	12.889	3583	3592	3600	rBV3	656	787	0.12%	0.015%
87	13.211	3685	3692	3699	rBV4	2441	3178	0.47%	0.060%
88	13.844	3884	3889	3894	rBV3	533	590	0.09%	0.011%
89	14.095	3959	3967	3978	rVB2	763	1179	0.18%	0.022%
90	14.220	4004	4006	4012	rVB	104	105	0.02%	0.002%
91	14.333	4037	4041	4045	rBV2	434	421	0.06%	0.008%
92	14.577	4111	4117	4122	rBV2	321	427	0.06%	0.008%
93	14.725	4161	4163	4168	rVB	150	118	0.02%	0.002%
94	14.954	4232	4234	4237	rVV	195	102	0.02%	0.002%
95	14.970	4237	4239	4245	rVB	206	98	0.01%	0.002%
96	15.407	4373	4375	4379	rVB2	220	147	0.02%	0.003%
97	15.564	4421	4424	4427	rBV	193	154	0.02%	0.003%
98	15.648	4446	4450	4455	rVB2	242	274	0.04%	0.005%
99	15.793	4493	4495	4502	rVB2	237	185	0.03%	0.003%
100	16.854	4820	4825	4827	rBV3	469	498	0.07%	0.009%




Sum of corrected areas: 5288014

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
Data File : VU046713.D
Acq On : 10 Jan 2022 13:00
Operator : SY/MD
Sample : N1084-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGLL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

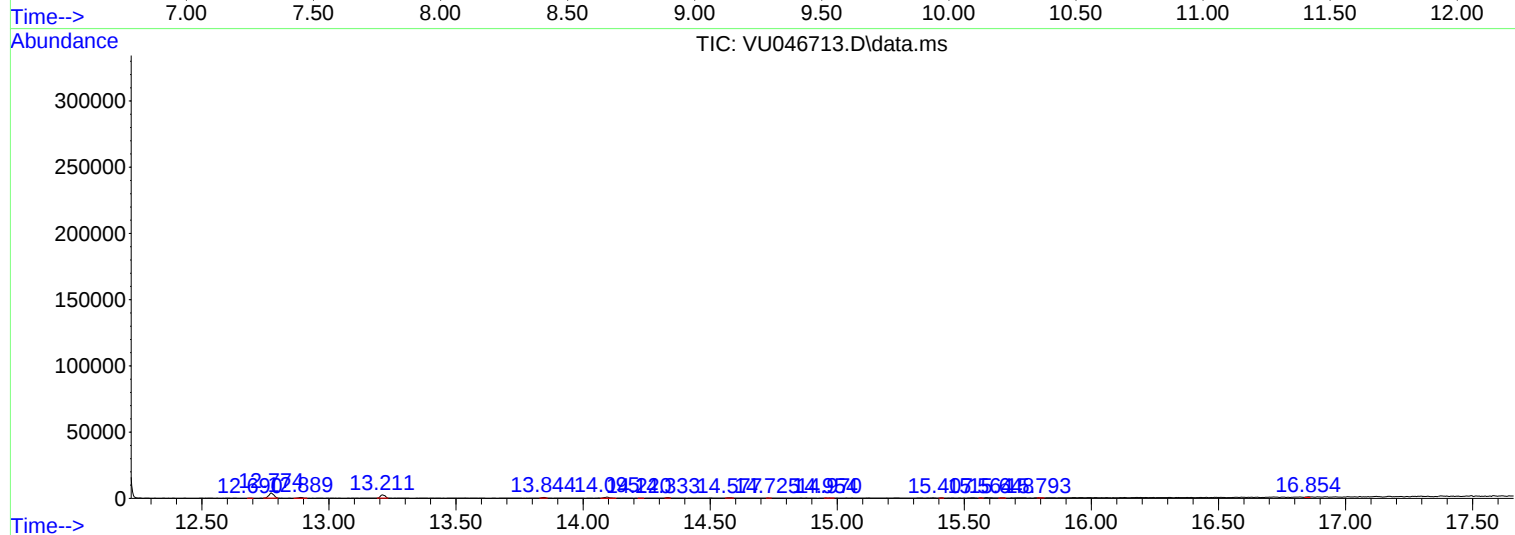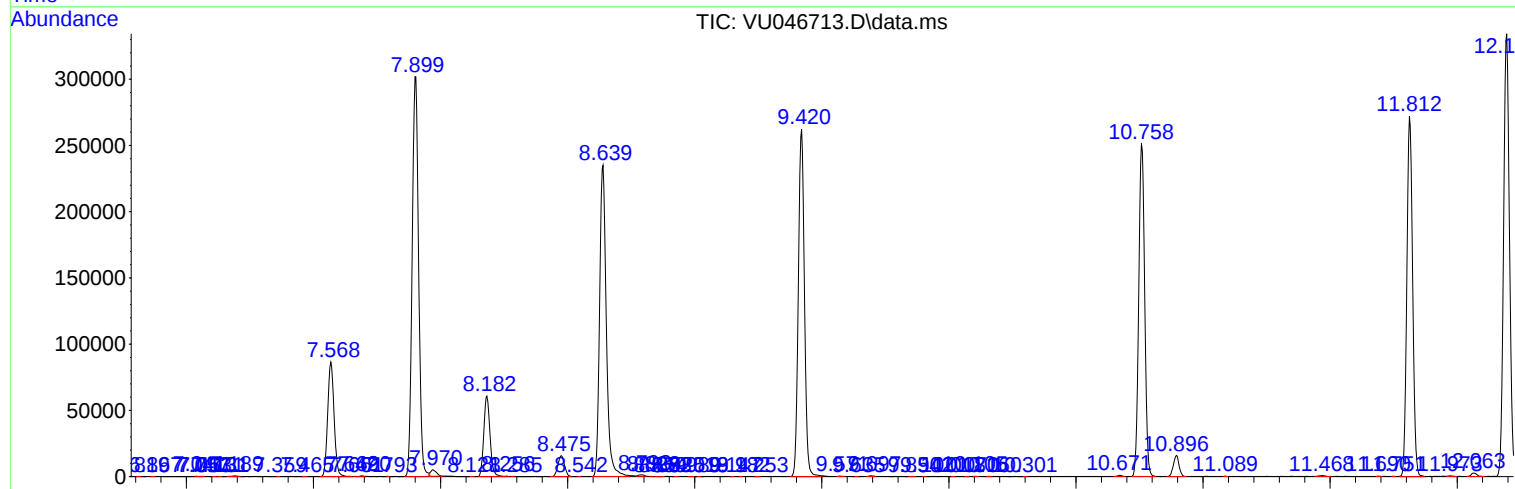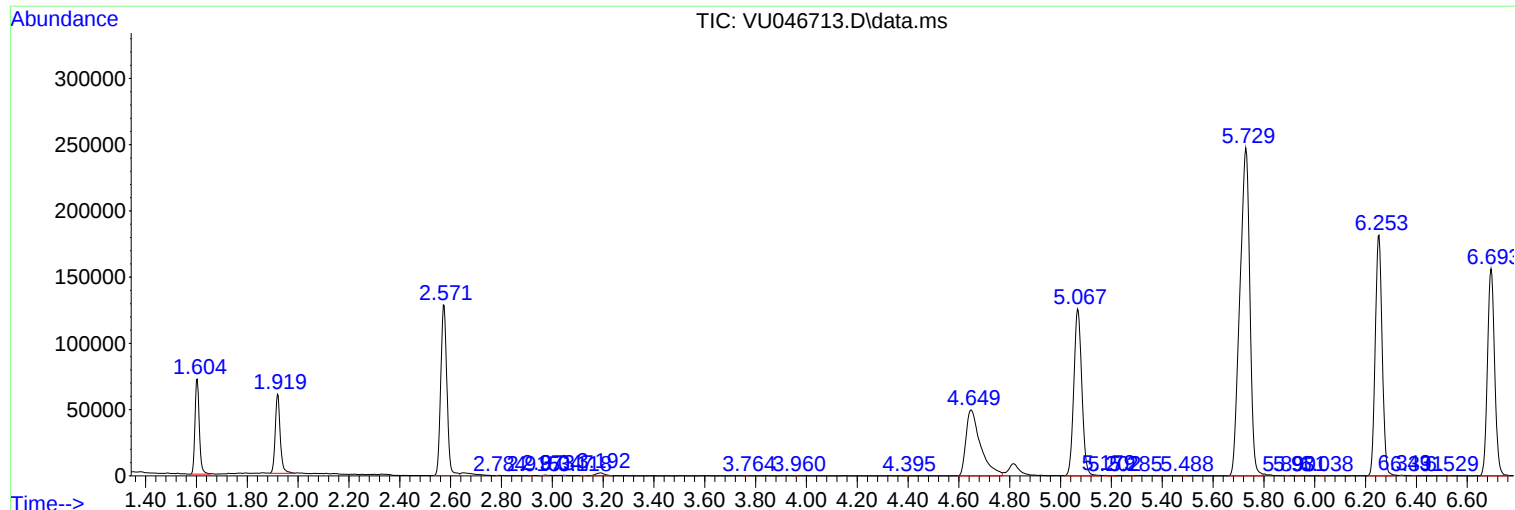

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
Data File : VU046713.D
Acq On : 10 Jan 2022 13:00
Operator : SY/MD
Sample : N1084-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGLL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
Data File : VU046713.D
Acq On : 10 Jan 2022 13:00
Operator : SY/MD
Sample : N1084-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGLL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------