


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011022\
 Data File : VU046709.D
 Acq On : 10 Jan 2022 10:07
 Operator : SY/MD
 Sample : BFB040
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB040

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 07 23:26:33 2022

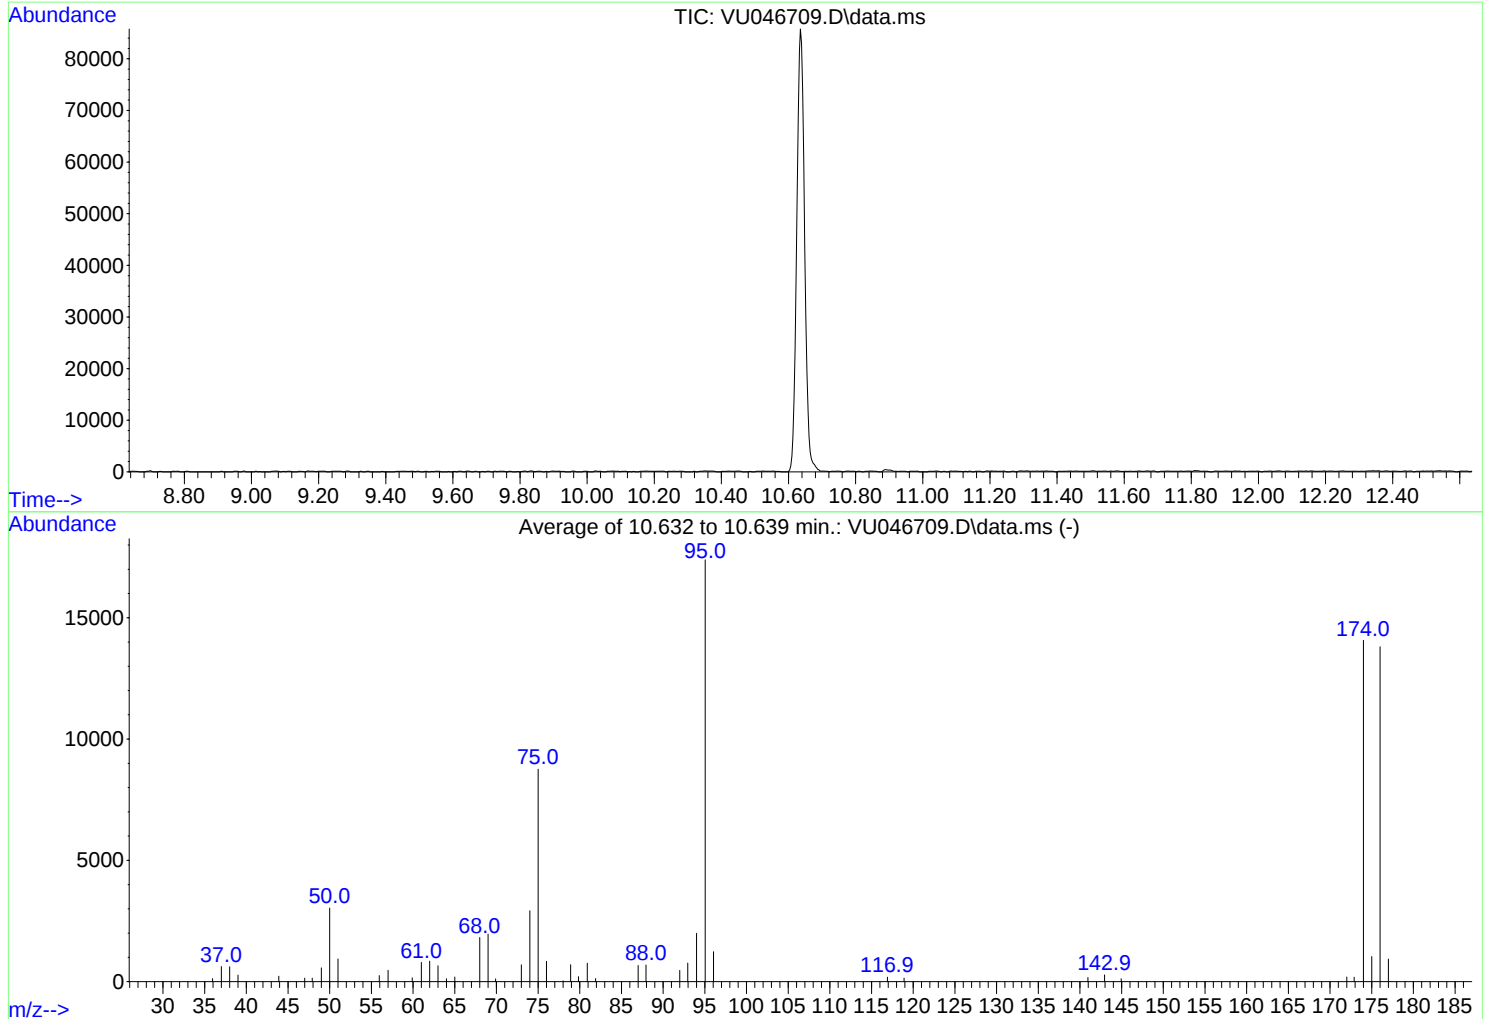

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	3037	PASS
75	95	30	80	50.4	8761	PASS
95	95	100	100	100.0	17389	PASS
96	95	5	9	7.1	1231	PASS
173	174	0.00	2	1.3	185	PASS
174	95	50	120	80.9	14068	PASS
175	174	5	9	7.3	1033	PASS
176	174	95	101	98.2	13808	PASS
177	176	5	9	6.7	930	PASS

m/z	Abundance
35.90	115.0
37.00	673.0
38.00	620.0
39.00	243.0
43.90	246.0
47.00	168.0
47.90	112.0
49.00	600.0
50.00	2989.0
51.00	918.0
56.00	259.0
57.00	408.0
59.90	160.0
61.00	785.0
62.00	892.0
63.00	648.0
64.00	119.0
65.00	229.0
68.00	1760.0
69.00	2055.0
69.90	112.0
73.00	683.0
74.00	2891.0
75.00	8659.0
76.00	807.0
78.90	724.0
79.80	199.0
80.90	716.0
81.90	127.0
87.00	633.0
87.90	646.0
92.00	468.0
92.90	737.0
94.00	1987.0
95.10	17144.0
96.00	1145.0
116.90	163.0
118.90	167.0
140.90	165.0
142.90	279.0
145.00	122.0
172.00	187.0
172.90	151.0
174.00	14113.0
175.00	1073.0
176.00	14040.0
177.00	868.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
35.90	119.0
37.00	635.0
38.00	617.0
39.00	287.0
43.90	219.0
47.00	135.0
47.90	167.0
49.00	593.0
50.00	3144.0
51.00	964.0
55.90	269.0
57.00	491.0
59.90	169.0
61.00	799.0
62.00	870.0
63.00	647.0
64.00	121.0
65.00	196.0
68.00	1897.0
69.00	2040.0
69.90	118.0
73.00	718.0
74.00	2959.0
75.00	8979.0
76.00	874.0
78.90	730.0
79.80	208.0
80.90	802.0
81.90	130.0
87.00	681.0
88.00	717.0
92.00	452.0
93.00	789.0
94.00	2044.0
95.00	17936.0
96.00	1275.0
116.90	195.0
118.90	153.0
140.90	166.0
142.90	279.0
144.90	117.0
172.00	189.0
172.90	193.0
174.00	14494.0
175.00	1066.0
176.00	14136.0
177.00	969.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
36.00	150.0
37.00	562.0
38.00	598.0
39.00	273.0
43.90	208.0
47.00	135.0
47.90	163.0
49.00	510.0
50.00	2978.0
51.00	939.0
55.90	222.0
57.00	511.0
59.90	149.0
61.00	789.0
62.00	763.0
63.00	659.0
64.00	111.0
65.00	147.0
68.00	1806.0
69.00	1792.0
69.90	106.0
73.00	679.0
74.00	2912.0
75.00	8646.0
76.00	829.0
78.00	100.0
78.90	644.0
79.90	206.0
80.90	755.0
81.90	123.0
87.00	693.0
88.00	686.0
92.00	471.0
93.00	762.0
94.00	1949.0
95.00	17088.0
96.10	1272.0
116.90	194.0
118.90	125.0
141.00	182.0
143.00	271.0
144.90	111.0
172.00	193.0
172.90	212.0
174.00	13596.0
175.00	959.0
176.00	13249.0
177.00	952.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB040