
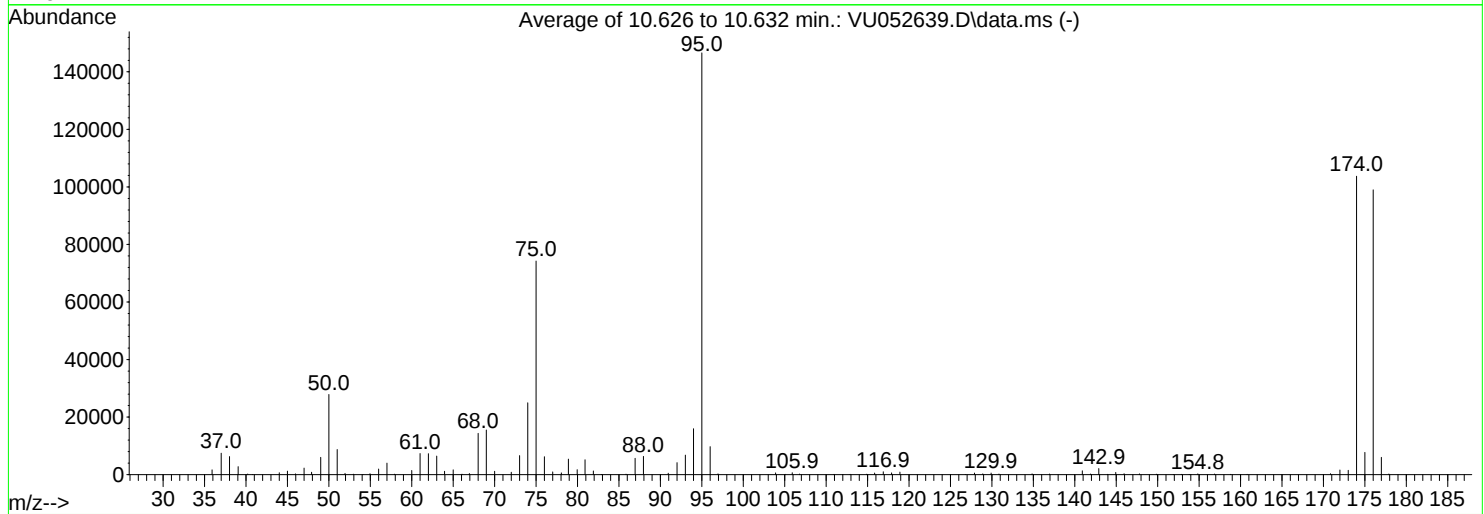


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011023\
 Data File : VU052639.D
 Acq On : 10 Jan 2023 09:20
 Operator : JC/MD
 Sample : BFB188
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB188

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jan 11 00:53:59 2023

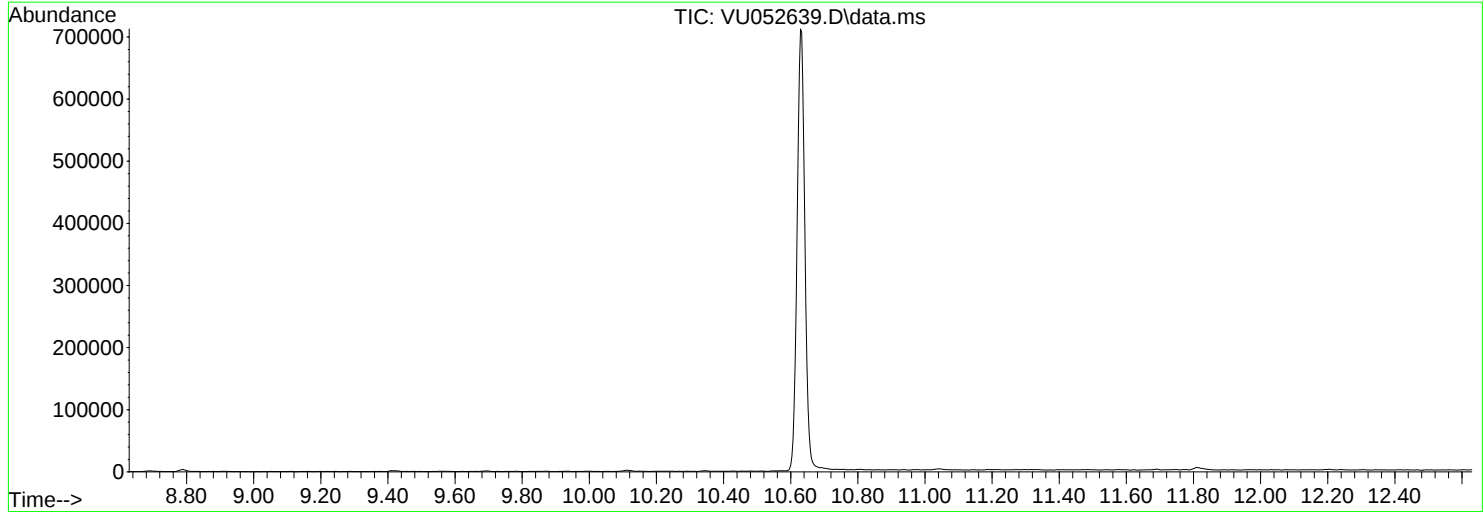

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	27859	PASS
75	95	30	80	50.6	74243	PASS
95	95	100	100	100.0	146603	PASS
96	95	5	9	6.6	9740	PASS
173	174	0.00	2	1.5	1533	PASS
174	95	50	120	70.7	103688	PASS
175	174	5	9	7.5	7746	PASS
176	174	95	101	95.5	98995	PASS
177	176	5	9	6.1	6034	PASS

m/z	Abundance
35.90	400.0
39.90	176.0
44.00	440.0
126.90	310.0
127.90	128.0
253.70	174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

m/z	Abundance
35.90	1954.0
37.00	7279.0
38.00	6092.0
39.10	2768.0
39.90	229.0
40.20	231.0
44.00	1160.0
45.00	1146.0
45.90	246.0
47.00	2263.0
47.90	810.0
49.00	5739.0
50.00	26304.0
51.00	8371.0
51.90	454.0
53.00	204.0
54.10	104.0
55.00	356.0
56.00	1840.0
57.00	3781.0
57.90	146.0
60.00	1382.0
61.00	7053.0
62.00	6841.0
63.00	6181.0
63.90	1087.0
65.00	1672.0
66.00	151.0
67.00	386.0
68.00	13950.0
69.00	14688.0
70.00	1144.0
72.00	798.0
73.00	6232.0
74.00	23880.0
75.00	70928.0
76.00	6148.0
77.00	783.0
78.00	616.0
78.90	5188.0
79.90	1776.0
80.90	5068.0
81.90	1153.0
82.90	153.0
85.90	215.0
87.00	5450.0
87.90	5886.0
91.00	467.0
92.00	3920.0
93.00	6512.0
94.00	15208.0
95.00	138560.0
96.00	8936.0
96.90	198.0
103.90	576.0
105.00	157.0
105.90	634.0
106.80	199.0
110.90	119.0
114.90	156.0
115.80	540.0
116.90	1017.0
117.90	627.0
118.90	951.0
126.80	427.0
127.90	624.0
128.90	305.0
129.90	507.0
130.90	183.0
134.90	218.0
137.00	167.0
140.90	1267.0
142.00	171.0
142.90	2062.0
143.90	125.0
145.00	760.0
146.00	326.0
147.80	264.0
149.80	153.0
153.80	104.0
154.90	247.0
156.80	233.0
158.80	138.0
160.80	138.0
170.90	311.0
172.00	1390.0
173.00	1413.0
174.00	95632.0
175.00	7297.0
176.00	90976.0
177.00	5735.0
177.90	214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

253.70

153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

m/z	Abundance
35.90	2148.0
37.00	7731.0
38.00	6480.0
39.00	2853.0
40.20	218.0
44.00	1129.0
45.00	1329.0
46.00	261.0
47.00	2361.0
47.90	873.0
49.00	6243.0
50.00	28712.0
51.00	8946.0
52.00	452.0
52.90	161.0
54.10	109.0
55.00	379.0
56.00	1964.0
57.00	4169.0
57.90	143.0
60.00	1534.0
61.00	7527.0
62.00	7516.0
63.00	6633.0
63.90	1217.0
65.00	1760.0
66.10	176.0
66.90	428.0
68.00	14836.0
69.00	16094.0
70.00	1208.0
72.00	831.0
73.00	6869.0
74.00	25824.0
75.00	76664.0
76.00	6442.0
77.00	981.0
78.10	654.0
78.90	5639.0
79.90	1795.0
80.90	5304.0
81.90	1336.0
82.90	104.0
85.90	173.0
86.90	5756.0
88.00	6532.0
90.90	540.0
92.00	4335.0
93.00	7045.0
94.00	16378.0
95.00	151680.0
96.00	10166.0
97.00	251.0
103.90	651.0
105.00	138.0
105.90	680.0
106.80	214.0
110.90	149.0
112.00	105.0
112.90	162.0
114.90	197.0
115.90	578.0
116.90	1060.0
117.90	641.0
118.90	920.0
126.80	359.0
127.90	703.0
128.90	298.0
129.90	638.0
130.90	218.0
134.80	272.0
136.90	200.0
140.90	1354.0
141.90	212.0
142.90	2187.0
143.90	145.0
144.90	801.0
145.90	354.0
147.80	307.0
149.80	170.0
152.80	121.0
154.80	271.0
156.80	257.0
158.80	135.0
160.80	125.0
170.80	365.0
172.00	1618.0
173.00	1577.0
174.00	107128.0
175.00	7967.0
176.00	102000.0
177.00	6242.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

177.90219.0

253.80142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

m/z	Abundance
36.00	2163.0
37.00	7295.0
38.00	6316.0
39.00	2745.0
40.20	224.0
40.80	106.0
44.00	1017.0
45.00	1221.0
46.00	264.0
47.00	2261.0
47.90	824.0
49.00	6094.0
50.00	28560.0
51.00	8970.0
52.00	381.0
53.00	155.0
54.90	349.0
56.00	2008.0
57.00	4087.0
57.90	150.0
60.00	1486.0
61.00	7382.0
62.00	7487.0
63.00	6497.0
64.00	1156.0
65.00	1568.0
66.10	185.0
66.90	430.0
68.00	14328.0
69.00	15758.0
70.00	1160.0
72.00	820.0
73.00	6819.0
74.00	25168.0
75.00	75136.0
76.00	6150.0
77.00	1041.0
78.10	671.0
78.90	5321.0
80.00	1593.0
80.90	5196.0
81.90	1432.0
85.80	180.0
86.90	5765.0
88.00	6543.0
90.90	558.0
92.00	4263.0
93.00	6872.0
94.00	16290.0
95.00	149568.0
96.00	10119.0
97.00	326.0
103.90	657.0
105.10	110.0
105.90	655.0
106.80	207.0
111.00	152.0
112.90	151.0
114.90	170.0
115.90	569.0
116.90	1005.0
117.90	555.0
118.90	845.0
126.80	337.0
127.90	724.0
128.90	245.0
129.90	621.0
130.80	243.0
134.80	323.0
136.90	243.0
140.90	1354.0
141.80	226.0
142.90	2137.0
144.00	155.0
144.90	738.0
145.90	311.0
147.80	319.0
149.90	141.0
151.90	110.0
152.90	156.0
154.00	103.0
154.80	270.0
156.90	260.0
158.80	136.0
160.80	129.0
170.80	343.0
172.00	1777.0
173.00	1609.0
174.00	108304.0
175.00	7973.0
176.00	104008.0
177.00	6126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

177.90
253.90

171.0
162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188