

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011121\
 Data File : VU041950.D
 Acq On : 12 Jan 2021 03:23
 Operator : SY/MD
 Sample : M1027-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXK7

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011121WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	9	16	25	rVB2	20798	23454	1.23%	0.339%
2	1.478	36	43	53	rBV3	19378	23202	1.22%	0.335%
3	1.604	75	82	93	rVB	70482	74285	3.91%	1.073%
4	1.922	171	181	190	rBV	64123	79191	4.16%	1.144%
5	2.578	373	385	399	rBV	105523	175380	9.22%	2.534%
6	3.375	621	633	650	rBV3	11018	26307	1.38%	0.380%
7	4.655	1013	1031	1069	rBV2	75590	293930	15.46%	4.247%
8	5.079	1144	1163	1184	rBV2	88678	196191	10.32%	2.835%
9	5.739	1347	1368	1385	rBV2	168163	438873	23.08%	6.341%
10	6.259	1516	1530	1545	rBV	131771	247433	13.01%	3.575%
11	6.552	1607	1621	1643	rBV	494828	927485	48.77%	13.401%
12	6.700	1653	1667	1683	rVB3	104920	204148	10.73%	2.950%
13	7.571	1926	1938	1953	rBV2	57367	99942	5.26%	1.444%
14	7.903	2028	2041	2057	rBV	203184	353621	18.59%	5.110%
15	8.185	2118	2129	2143	rBV	38541	65922	3.47%	0.953%
16	8.555	2230	2244	2259	rBV	1123769	1901727	100.00%	27.479%
17	8.639	2259	2270	2309	rVB	381296	746048	39.23%	10.780%
18	9.417	2500	2512	2541	rBV	199577	338409	17.79%	4.890%
19	10.754	2916	2928	2944	rVB	90586	148628	7.82%	2.148%
20	11.806	3243	3255	3271	rVB	165470	267023	14.04%	3.858%
21	12.189	3358	3374	3389	rBV	177030	289574	15.23%	4.184%


Sum of corrected areas: 6920773

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU011121\
Data File : VU041950.D
Acq On : 12 Jan 2021 03:23
Operator : SY/MD
Sample : M1027-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXK7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011121WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

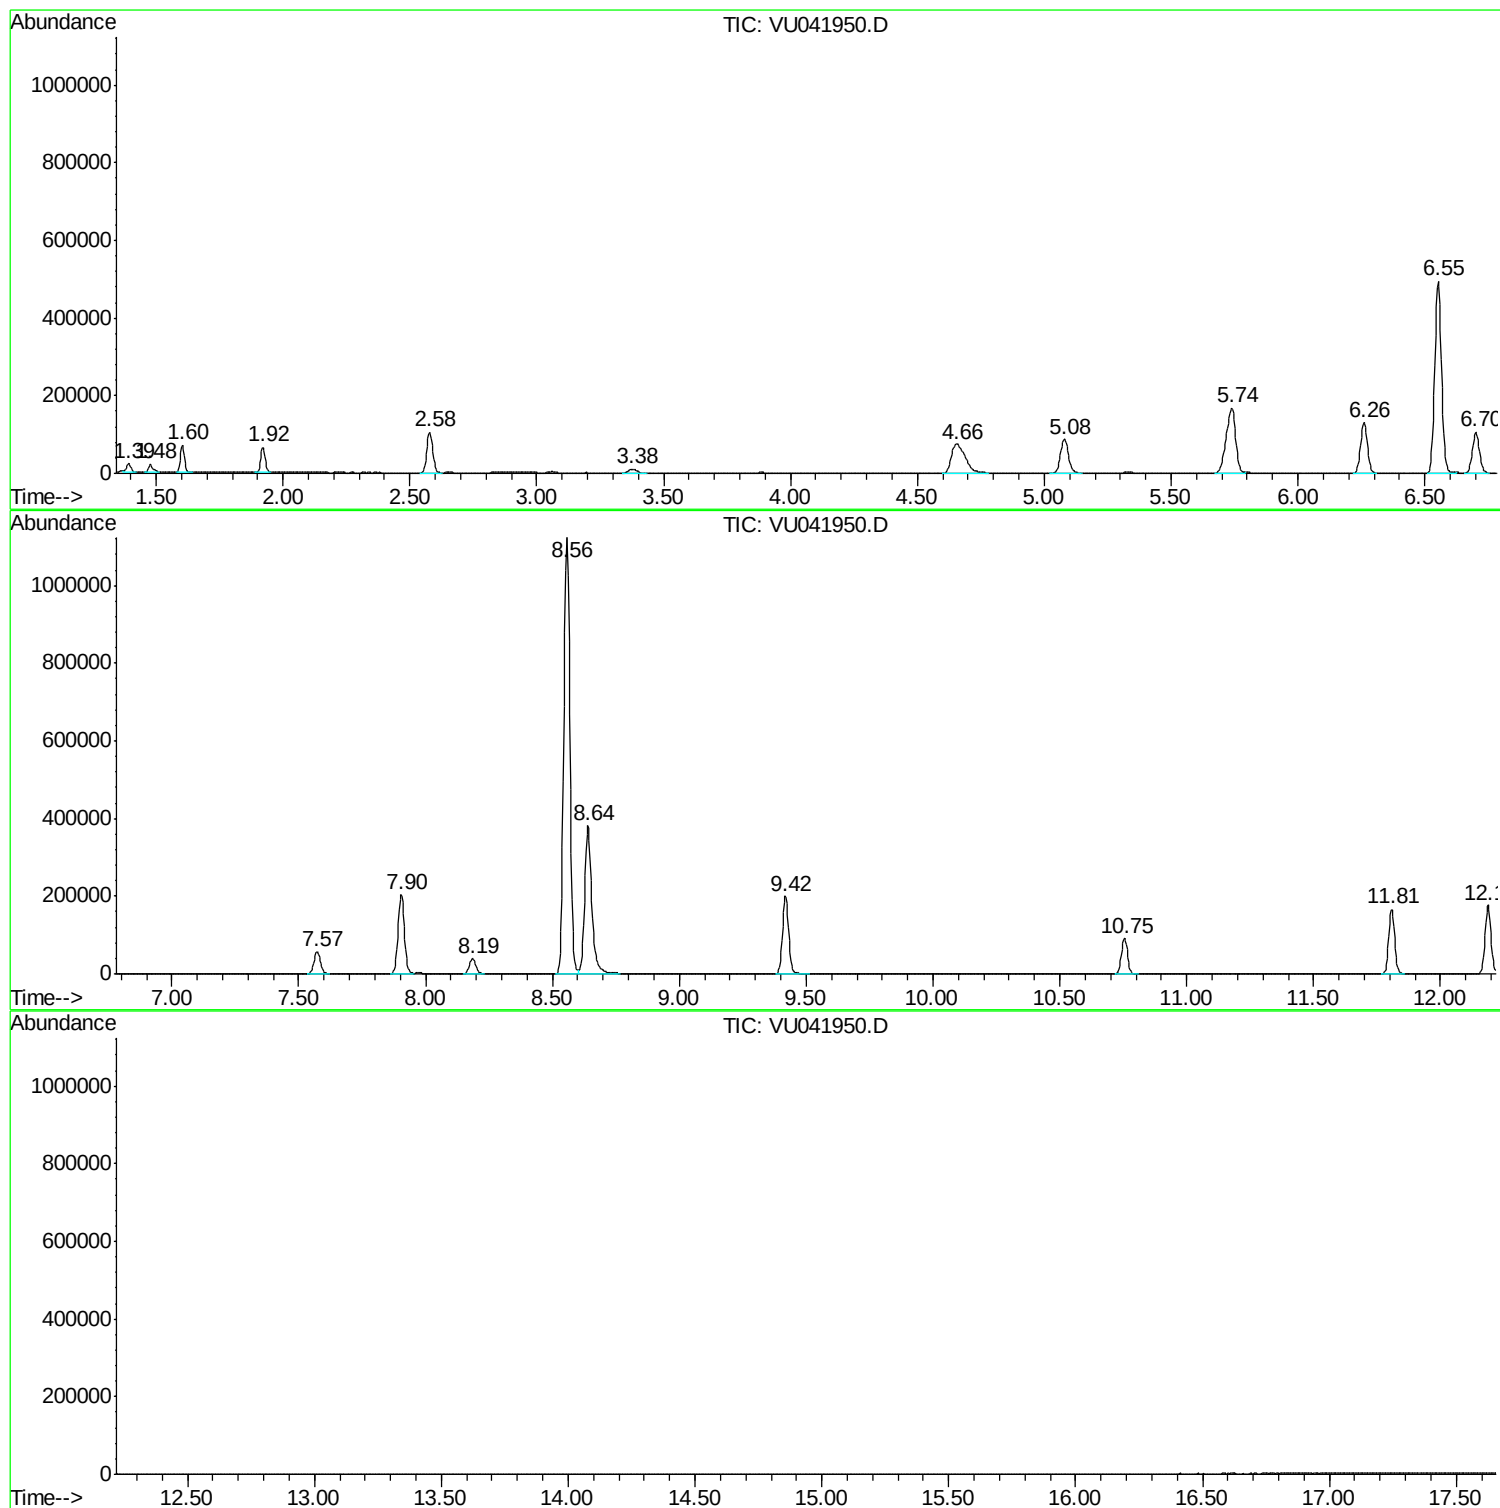

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011121\
Data File : VU041950.D
Acq On : 12 Jan 2021 03:23
Operator : SY/MD
Sample : M1027-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXK7










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011121WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.57	2.02 ug/L	99942	1,4-Difluorobenzene	6.26

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Thiatricyclo[3.1.1.0(2,4)]heptane	112	C6H8S	1000221-37-0	37
2			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
3			1,3-Cyclohexadiene	80	C6H8	000592-57-4	25
4			Thiophosgene	114	CCl2S	000463-71-8	9
5			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9

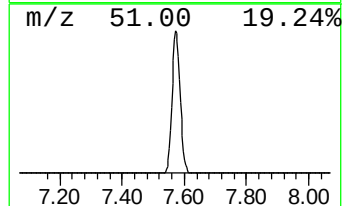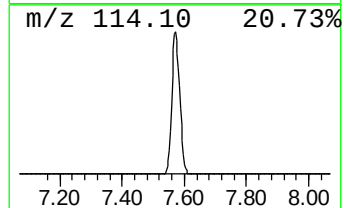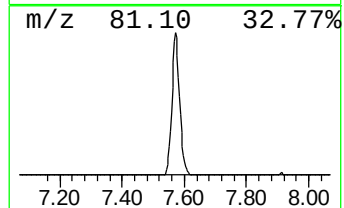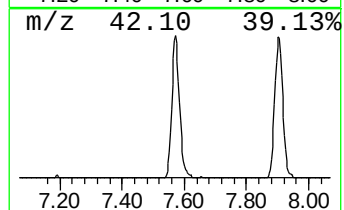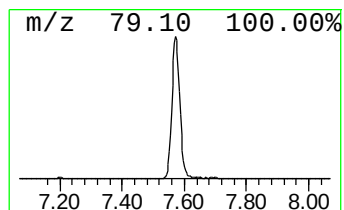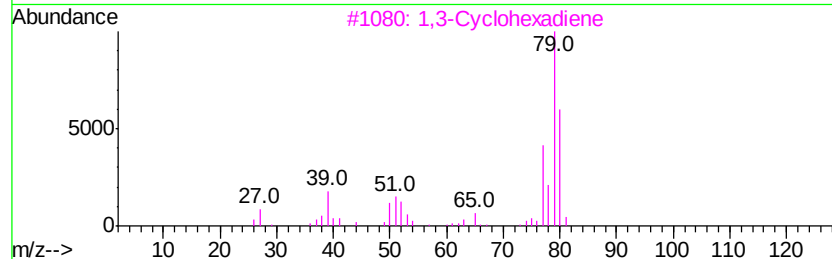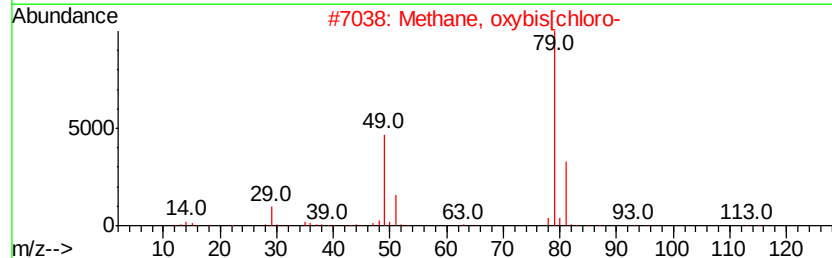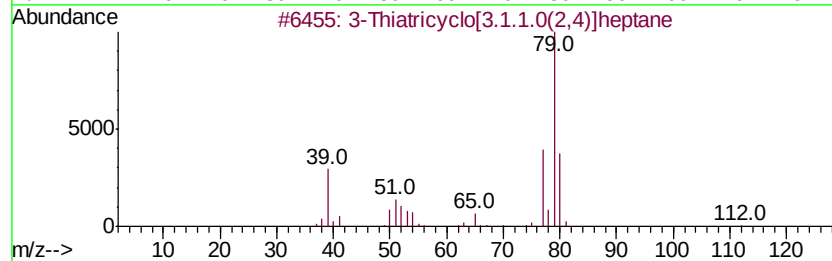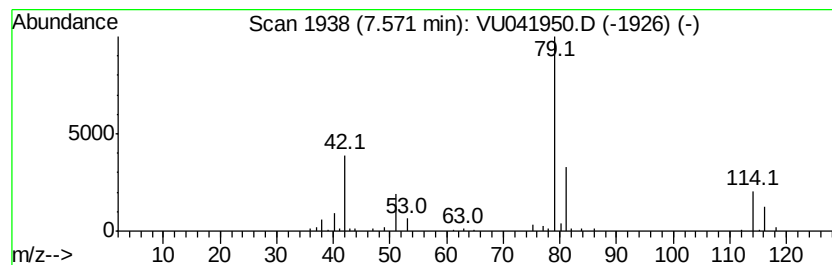

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU011121\
Data File : VU041950.D
Acq On : 12 Jan 2021 03:23
Operator : SY/MD
Sample : M1027-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXK7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011121WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.57	2.0	ug/L	99942	1	6.26	247433	5.0