

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
 Data File : VU046723.D
 Acq On : 11 Jan 2022 12:49
 Operator : SY/MD
 Sample : VU0111WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

Signal : TIC: VU046723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	100	rVB	83809	97966	14.93%	1.913%
2	1.919	171	180	199	rBV	62490	85340	13.01%	1.667%
3	2.256	283	285	288	rVB	260	124	0.02%	0.002%
4	2.301	297	299	303	rVB2	186	115	0.02%	0.002%
5	2.353	313	315	319	rVB	141	120	0.02%	0.002%
6	2.430	336	339	343	rVB	204	114	0.02%	0.002%
7	2.575	372	384	401	rBV	142333	233275	35.56%	4.555%
8	2.732	430	433	434	rBV	233	136	0.02%	0.003%
9	2.739	434	435	439	rVB	179	116	0.02%	0.002%
10	2.800	452	454	458	rVB2	190	159	0.02%	0.003%
11	2.957	499	503	506	rBB	132	131	0.02%	0.003%
12	3.176	568	571	573	rBV2	278	218	0.03%	0.004%
13	3.195	574	577	581	rVB2	380	315	0.05%	0.006%
14	3.272	597	601	605	rBB	122	127	0.02%	0.002%
15	3.681	725	728	731	rBV	139	146	0.02%	0.003%
16	4.436	960	963	968	rBB	120	150	0.02%	0.003%
17	4.645	1014	1028	1072	rBV2	42943	165620	25.25%	3.234%
18	4.909	1107	1110	1115	rVB	190	163	0.02%	0.003%
19	5.002	1135	1139	1142	rBB	154	130	0.02%	0.003%
20	5.067	1143	1159	1184	rBV	120053	261537	39.87%	5.107%
21	5.729	1343	1365	1399	rBV2	243102	656025	100.00%	12.811%
22	6.253	1513	1528	1551	rBV	199252	377790	57.59%	7.378%
23	6.394	1570	1572	1574	rVB	222	124	0.02%	0.002%
24	6.417	1575	1579	1583	rBB	287	251	0.04%	0.005%
25	6.529	1612	1614	1620	rVB3	493	370	0.06%	0.007%
26	6.693	1650	1665	1688	rBV	149948	289324	44.10%	5.650%
27	6.812	1700	1702	1705	rBB	247	125	0.02%	0.002%
28	7.137	1799	1803	1806	rBV	146	177	0.03%	0.003%
29	7.169	1811	1813	1815	rVV	297	199	0.03%	0.004%
30	7.189	1817	1819	1824	rVB	553	351	0.05%	0.007%
31	7.568	1924	1937	1953	rBV	81392	140424	21.41%	2.742%
32	7.648	1959	1962	1965	rVB	308	265	0.04%	0.005%
33	7.693	1970	1976	1981	rBB3	473	606	0.09%	0.012%
34	7.899	2025	2040	2057	rBV	310817	528717	80.59%	10.325%
35	8.070	2090	2093	2096	rBV	174	157	0.02%	0.003%
36	8.182	2115	2128	2141	rBV	57320	96406	14.70%	1.883%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
 Data File : VU046723.D
 Acq On : 11 Jan 2022 12:49
 Operator : SY/MD
 Sample : VU0111WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

37	8.256	2149	2151	2154	rVB	257	160	0.02%	0.003%
38	8.275	2154	2157	2161	rBB2	222	160	0.02%	0.003%
39	8.545	2236	2241	2242	rBB2	123	113	0.02%	0.002%
40	8.636	2257	2269	2300	rBV	207365	372916	56.84%	7.282%
41	8.754	2304	2306	2309	rVB2	332	189	0.03%	0.004%
42	8.816	2322	2325	2327	rBV	141	120	0.02%	0.002%
43	8.851	2333	2336	2337	rBV	155	112	0.02%	0.002%
44	8.883	2343	2346	2348	rBV	155	129	0.02%	0.003%
45	8.983	2371	2377	2382	rBB	159	237	0.04%	0.005%
46	9.102	2409	2414	2416	rBB	152	155	0.02%	0.003%
47	9.176	2433	2437	2439	rBB	157	128	0.02%	0.002%
48	9.285	2468	2471	2476	rBV	149	194	0.03%	0.004%
49	9.417	2500	2512	2533	rBV	282962	472704	72.06%	9.231%
50	9.558	2553	2556	2558	rBV	172	142	0.02%	0.003%
51	9.571	2558	2560	2563	rVB	286	179	0.03%	0.003%
52	9.594	2564	2567	2569	rBV	144	123	0.02%	0.002%
53	9.629	2573	2578	2581	rBV	140	166	0.03%	0.003%
54	9.700	2593	2600	2606	rVB2	575	779	0.12%	0.015%
55	9.738	2609	2612	2616	rBB	139	118	0.02%	0.002%
56	9.777	2621	2624	2627	rBV	154	149	0.02%	0.003%
57	9.809	2631	2634	2637	rBV	188	166	0.03%	0.003%
58	10.008	2693	2696	2699	rVB	196	153	0.02%	0.003%
59	10.124	2729	2732	2735	rBV	158	155	0.02%	0.003%
60	10.201	2753	2756	2758	rBV	156	130	0.02%	0.003%
61	10.272	2775	2778	2781	rBV	184	168	0.03%	0.003%
62	10.398	2814	2817	2819	rBV	127	114	0.02%	0.002%
63	10.539	2858	2861	2871	rBV	158	330	0.05%	0.006%
64	10.616	2882	2885	2887	rBV	140	120	0.02%	0.002%
65	10.668	2894	2901	2910	rVB3	1668	2046	0.31%	0.040%
66	10.758	2917	2929	2948	rBV	225853	364976	55.63%	7.127%
67	10.857	2957	2960	2965	rBV	228	203	0.03%	0.004%
68	10.883	2965	2968	2972	rVB	241	189	0.03%	0.004%
69	11.359	3109	3116	3119	rBV	185	288	0.04%	0.006%
70	11.462	3139	3148	3150	rBV3	925	1191	0.18%	0.023%
71	11.693	3216	3220	3221	rBV	262	206	0.03%	0.004%
72	11.751	3233	3238	3239	rBV	272	146	0.02%	0.003%
73	11.812	3244	3257	3274	rBV	289237	454319	69.25%	8.872%
74	11.934	3291	3295	3296	rBV	258	190	0.03%	0.004%
75	11.947	3296	3299	3301	rVV2	535	362	0.06%	0.007%
76	11.970	3302	3306	3314	rVB3	1352	1562	0.24%	0.031%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
 Data File : VU046723.D
 Acq On : 11 Jan 2022 12:49
 Operator : SY/MD
 Sample : VU0111WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

77	12.192	3362	3375	3397	rBV	314788	502762	76.64%	9.818%
78	12.272	3397	3400	3404	rBV2	158	145	0.02%	0.003%
79	12.327	3414	3417	3420	rBV2	301	189	0.03%	0.004%
80	12.423	3442	3447	3449	rBV	161	189	0.03%	0.004%
81	12.465	3456	3460	3465	rBV	127	139	0.02%	0.003%
82	12.770	3551	3555	3561	rVB2	221	208	0.03%	0.004%
83	13.221	3691	3695	3696	rBV	169	126	0.02%	0.002%
84	13.819	3877	3881	3885	rBV	130	116	0.02%	0.002%
85	13.841	3885	3888	3893	rVB2	439	436	0.07%	0.009%
86	14.092	3959	3966	3972	rBV2	342	483	0.07%	0.009%
87	14.333	4037	4041	4046	rVB2	283	179	0.03%	0.003%
88	15.127	4285	4288	4291	rBV2	225	168	0.03%	0.003%
89	15.394	4369	4371	4376	rBV	186	123	0.02%	0.002%
90	15.465	4390	4393	4397	rBV2	182	201	0.03%	0.004%
91	15.529	4411	4413	4418	rVB	221	163	0.02%	0.003%
92	15.606	4432	4437	4439	rBV2	292	291	0.04%	0.006%
93	15.648	4445	4450	4452	rBV2	152	158	0.02%	0.003%
94	15.741	4476	4479	4484	rVB2	171	153	0.02%	0.003%
95	15.770	4484	4488	4489	rBV	190	156	0.02%	0.003%
96	15.828	4503	4506	4510	rBV	244	190	0.03%	0.004%
97	15.889	4522	4525	4527	rBV	199	134	0.02%	0.003%
98	15.941	4538	4541	4545	rBV	242	212	0.03%	0.004%
99	16.208	4622	4624	4629	rBV2	240	152	0.02%	0.003%
100	17.323	4968	4971	4974	rBV2	571	400	0.06%	0.008%




Sum of corrected areas: 5120773

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
Data File : VU046723.D
Acq On : 11 Jan 2022 12:49
Operator : SY/MD
Sample : VU0111WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK061

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

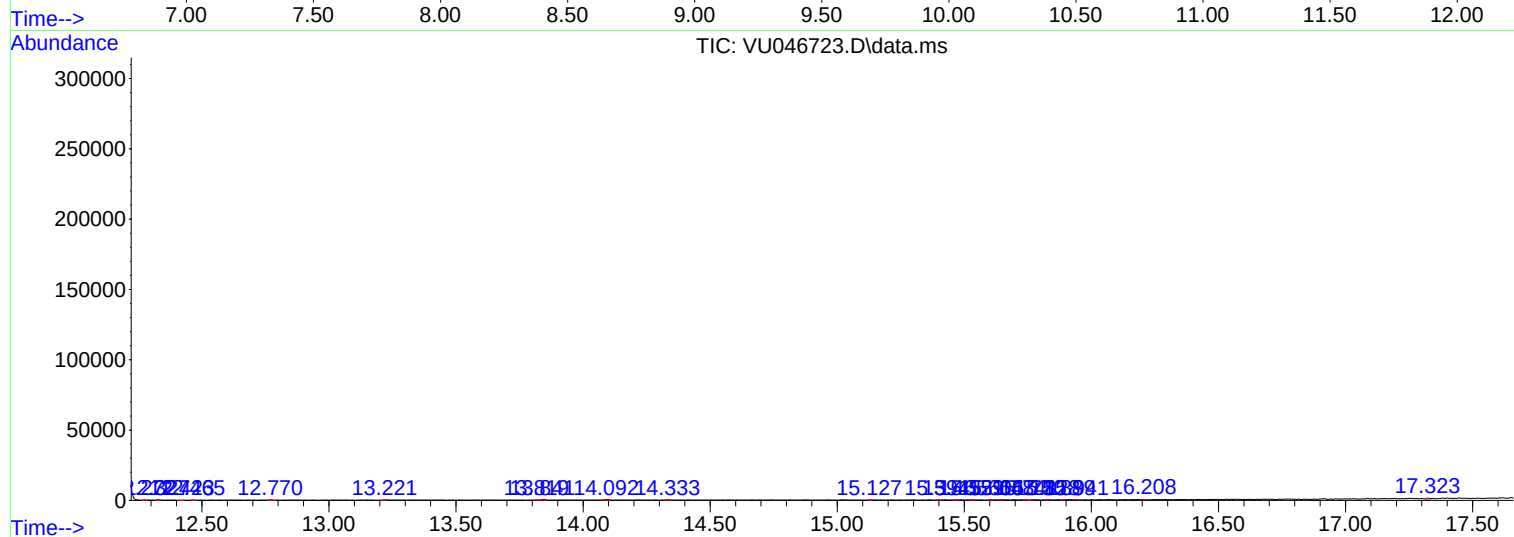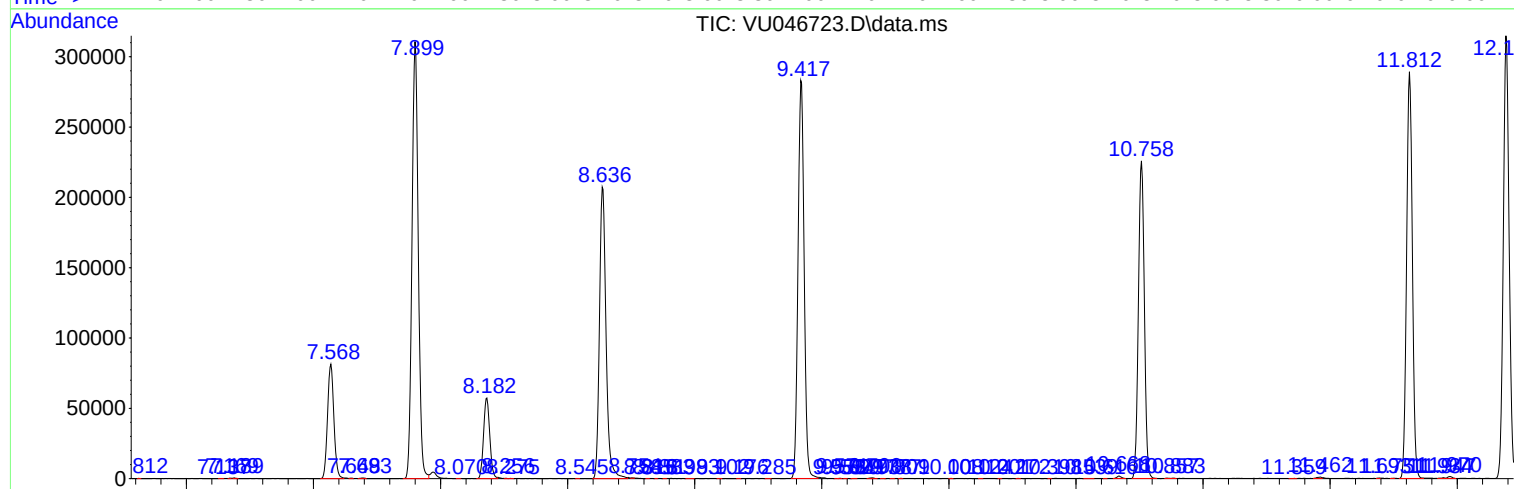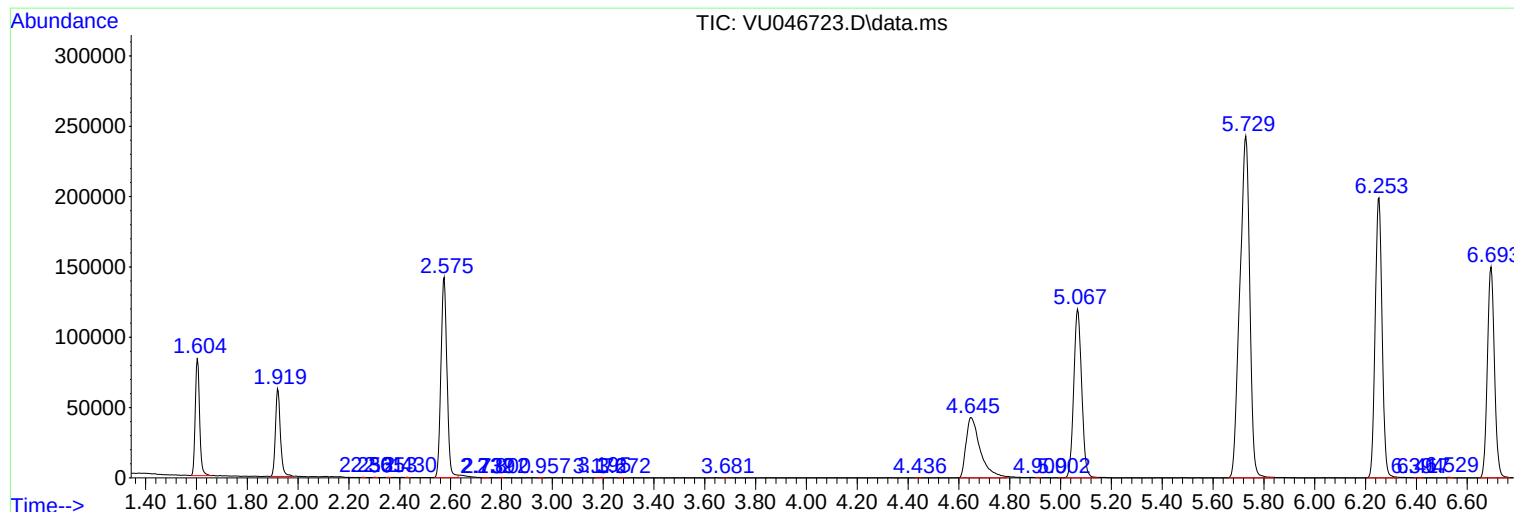

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
Data File : VU046723.D
Acq On : 11 Jan 2022 12:49
Operator : SY/MD
Sample : VU0111WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK061

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
Data File : VU046723.D
Acq On : 11 Jan 2022 12:49
Operator : SY/MD
Sample : VU0111WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK061

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------