

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
 Data File : VU046726.D
 Acq On : 11 Jan 2022 14:29
 Operator : SY/MD
 Sample : N1084-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M

Title : VOC Analysis

Signal : TIC: VU046726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	107	rVB	75327	87874	14.04%	1.797%
2	1.919	171	180	199	rBV	57756	78124	12.48%	1.598%
3	2.195	264	266	270	rVB	255	126	0.02%	0.003%
4	2.224	271	275	278	rBV2	159	112	0.02%	0.002%
5	2.273	288	290	294	rBV	125	113	0.02%	0.002%
6	2.420	334	336	341	rVB	211	109	0.02%	0.002%
7	2.575	371	384	398	rBV	125639	210533	33.63%	4.305%
8	2.748	434	438	441	rBB	163	161	0.03%	0.003%
9	2.771	442	445	447	rBV	136	121	0.02%	0.002%
10	2.803	449	455	458	rVB2	301	366	0.06%	0.007%
11	2.887	478	481	483	rBV	125	109	0.02%	0.002%
12	2.954	497	502	504	rBB	141	141	0.02%	0.003%
13	3.150	559	563	566	rBB	151	157	0.03%	0.003%
14	3.195	566	577	582	rBV2	998	1959	0.31%	0.040%
15	3.218	582	584	586	rVV	354	209	0.03%	0.004%
16	3.408	641	643	647	rBB	129	111	0.02%	0.002%
17	4.372	940	943	945	rBB	147	103	0.02%	0.002%
18	4.645	1013	1028	1062	rBV2	45829	168774	26.96%	3.451%
19	4.877	1096	1100	1106	rVV	149	149	0.02%	0.003%
20	4.912	1109	1111	1114	rVB	186	124	0.02%	0.003%
21	4.964	1124	1127	1129	rBB	256	123	0.02%	0.003%
22	5.067	1143	1159	1182	rBV	113880	247733	39.58%	5.066%
23	5.202	1199	1201	1204	rVB	173	114	0.02%	0.002%
24	5.292	1227	1229	1232	rBB2	255	164	0.03%	0.003%
25	5.729	1343	1365	1390	rBV2	229944	625945	100.00%	12.801%
26	6.250	1513	1527	1544	rBV	188321	355376	56.77%	7.268%
27	6.362	1559	1562	1567	rVB2	194	152	0.02%	0.003%
28	6.385	1567	1569	1573	rVB2	284	210	0.03%	0.004%
29	6.407	1574	1576	1577	rBV2	231	114	0.02%	0.002%
30	6.530	1610	1614	1618	rBB2	354	277	0.04%	0.006%
31	6.616	1638	1641	1643	rBB	145	98	0.02%	0.002%
32	6.694	1651	1665	1685	rBV	141804	277598	44.35%	5.677%
33	6.806	1698	1700	1701	rBV	236	114	0.02%	0.002%
34	7.186	1813	1818	1825	rBB2	533	592	0.09%	0.012%
35	7.372	1873	1876	1878	rBV	131	109	0.02%	0.002%
36	7.565	1924	1936	1956	rBV	77570	136438	21.80%	2.790%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
 Data File : VU046726.D
 Acq On : 11 Jan 2022 14:29
 Operator : SY/MD
 Sample : N1084-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

37	7.645	1958	1961	1964	rVB2	255	211	0.03%	0.004%
38	7.681	1965	1972	1973	rBV2	397	332	0.05%	0.007%
39	7.838	2019	2021	2026	rBB	129	115	0.02%	0.002%
40	7.899	2027	2040	2056	rBV	284636	490877	78.42%	10.039%
41	8.054	2085	2088	2089	rBV	144	102	0.02%	0.002%
42	8.179	2115	2127	2146	rBV	54816	93103	14.87%	1.904%
43	8.247	2146	2148	2153	rVB	298	246	0.04%	0.005%
44	8.449	2207	2211	2212	rVV	231	156	0.02%	0.003%
45	8.465	2212	2216	2217	rVV	506	405	0.06%	0.008%
46	8.475	2217	2219	2226	rVV	867	865	0.14%	0.018%
47	8.526	2232	2235	2238	rBB	184	144	0.02%	0.003%
48	8.636	2257	2269	2298	rBV	212739	378916	60.54%	7.749%
49	8.768	2307	2310	2313	rVB3	236	145	0.02%	0.003%
50	8.813	2322	2324	2327	rVB	189	121	0.02%	0.002%
51	8.832	2327	2330	2333	rBB	171	133	0.02%	0.003%
52	8.848	2333	2335	2338	rBB	162	110	0.02%	0.002%
53	8.877	2339	2344	2350	rBB	171	243	0.04%	0.005%
54	8.915	2351	2356	2365	rBB2	668	1018	0.16%	0.021%
55	9.012	2382	2386	2389	rBV	136	157	0.03%	0.003%
56	9.102	2412	2414	2417	rBV	143	123	0.02%	0.003%
57	9.134	2421	2424	2427	rBV	139	140	0.02%	0.003%
58	9.298	2473	2475	2480	rBB	158	158	0.03%	0.003%
59	9.330	2481	2485	2488	rBB	180	175	0.03%	0.004%
60	9.417	2498	2512	2542	rBV	273927	455073	72.70%	9.306%
61	9.575	2557	2561	2565	rBB2	279	258	0.04%	0.005%
62	9.629	2575	2578	2581	rBB	143	122	0.02%	0.002%
63	9.655	2582	2586	2590	rBB	127	134	0.02%	0.003%
64	9.681	2591	2594	2595	rBV	222	118	0.02%	0.002%
65	9.697	2596	2599	2602	rVV2	420	270	0.04%	0.006%
66	9.739	2609	2612	2615	rBV	141	139	0.02%	0.003%
67	9.841	2640	2644	2648	rBB	138	138	0.02%	0.003%
68	9.925	2665	2670	2672	rBB	140	147	0.02%	0.003%
69	10.118	2726	2730	2734	rBB	155	154	0.02%	0.003%
70	10.263	2770	2775	2778	rBV	142	169	0.03%	0.003%
71	10.671	2893	2902	2909	rBV4	1769	2388	0.38%	0.049%
72	10.758	2916	2929	2946	rVB	221206	359879	57.49%	7.360%
73	10.886	2962	2969	2979	rBV5	1187	2064	0.33%	0.042%
74	10.999	2999	3004	3006	rBV	150	151	0.02%	0.003%
75	11.153	3048	3052	3057	rBV	176	253	0.04%	0.005%
76	11.456	3139	3146	3155	rVB4	796	1147	0.18%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
 Data File : VU046726.D
 Acq On : 11 Jan 2022 14:29
 Operator : SY/MD
 Sample : N1084-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

77	11.558	3173	3178	3181	rVB	192	206	0.03%	0.004%
78	11.581	3181	3185	3187	rBV2	252	213	0.03%	0.004%
79	11.610	3191	3194	3199	rVV	121	114	0.02%	0.002%
80	11.693	3216	3220	3221	rBV	233	172	0.03%	0.004%
81	11.812	3244	3257	3274	rBV	270152	429233	68.57%	8.778%
82	11.935	3289	3295	3297	rBV	222	278	0.04%	0.006%
83	11.970	3301	3306	3313	rVB3	1009	1194	0.19%	0.024%
84	12.192	3360	3375	3393	rBV	293755	469865	75.06%	9.609%
85	12.266	3395	3398	3400	rVV	194	144	0.02%	0.003%
86	12.282	3400	3403	3410	rVB	212	172	0.03%	0.004%
87	12.404	3433	3441	3447	rBV	207	424	0.07%	0.009%
88	12.642	3511	3515	3517	rBV	212	178	0.03%	0.004%
89	12.771	3549	3555	3562	rVB	516	595	0.10%	0.012%
90	13.150	3670	3673	3675	rBV2	155	98	0.02%	0.002%
91	13.446	3759	3765	3768	rBV	121	141	0.02%	0.003%
92	15.349	4355	4357	4360	rBV	197	121	0.02%	0.002%
93	15.369	4360	4363	4368	rVV	294	226	0.04%	0.005%
94	15.404	4372	4374	4378	rVB2	205	150	0.02%	0.003%
95	15.442	4383	4386	4389	rBV	164	125	0.02%	0.003%
96	15.549	4416	4419	4425	rVB2	211	208	0.03%	0.004%
97	15.793	4493	4495	4499	rVB	157	124	0.02%	0.003%
98	16.491	4709	4712	4714	rBV	327	207	0.03%	0.004%
99	16.584	4738	4741	4747	rBV2	300	252	0.04%	0.005%
100	16.664	4763	4766	4768	rBV	320	218	0.03%	0.004%




Sum of corrected areas: 4889889

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
Data File : VU046726.D
Acq On : 11 Jan 2022 14:29
Operator : SY/MD
Sample : N1084-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

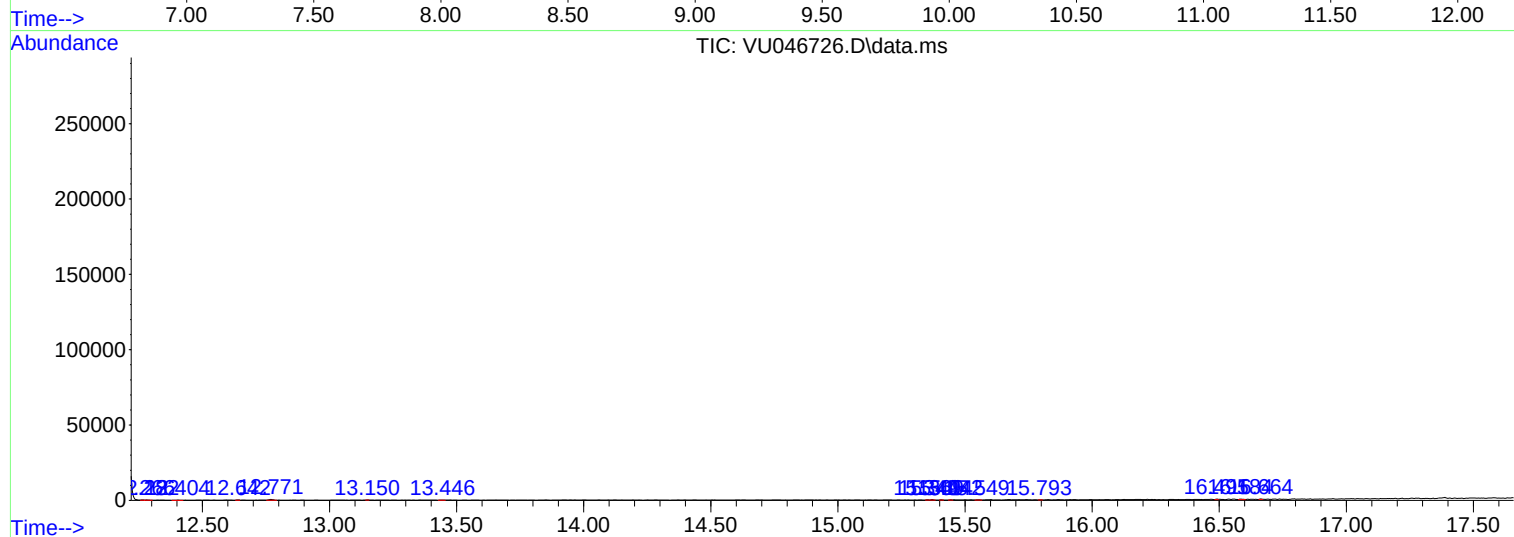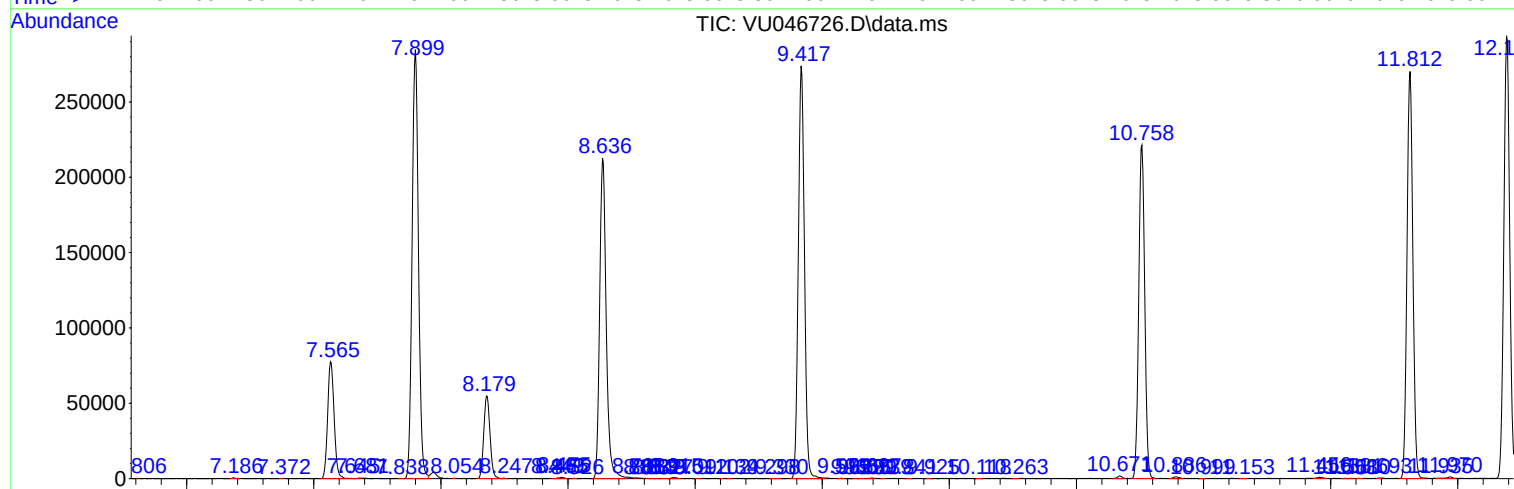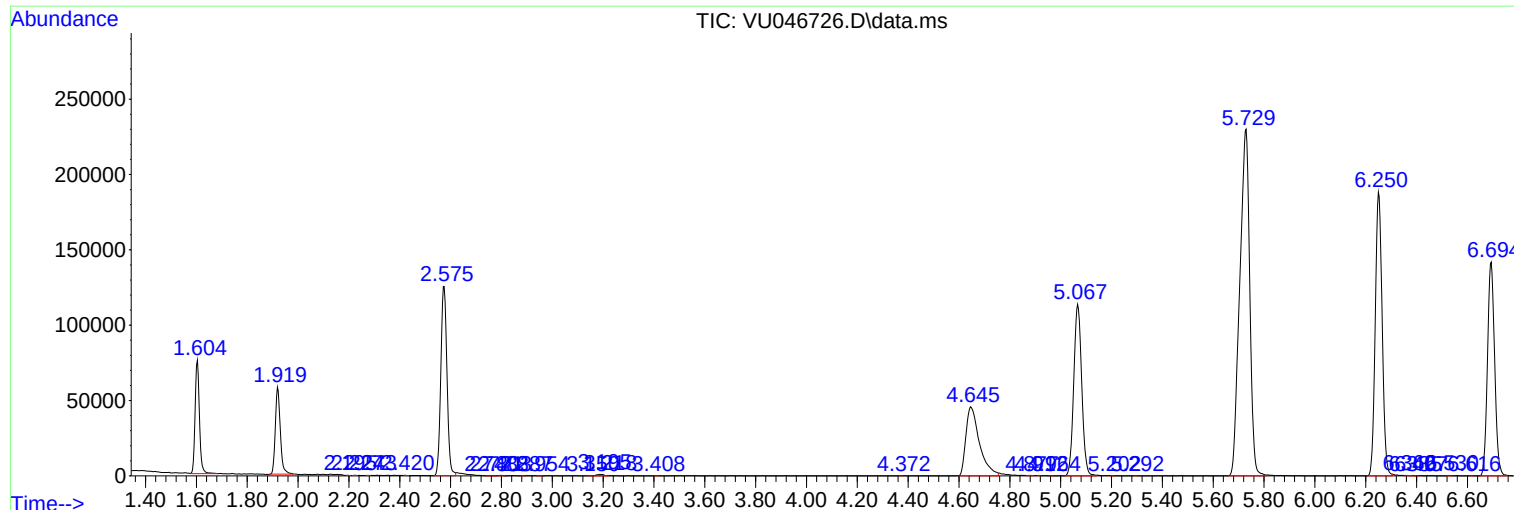

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
Data File : VU046726.D
Acq On : 11 Jan 2022 14:29
Operator : SY/MD
Sample : N1084-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011122\
Data File : VU046726.D
Acq On : 11 Jan 2022 14:29
Operator : SY/MD
Sample : N1084-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------